

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030381.D
 Acq On : 03 Oct 2024 19:09
 Operator : SY/MD
 Sample : P4284-02
 Misc : 5.48g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ3

Quant Time: Oct 04 01:10:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	362151	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	298568	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	106569	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	64331	22.732	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.920%
7) Chloroethane-d5	2.899	69	48389	23.501	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.000%
11) 1,1-Dichloroethene-d2	4.021	65	37317	18.065	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.240%
21) 2-Butanone-d5	7.081	46	34515	30.328	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.660%
24) Chloroform-d	7.648	84	165983	17.060	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	68.240%
26) 1,2-Dichloroethane-d4	8.307	65	86532	17.040	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	68.160%#
32) Benzene-d6	8.276	84	324734	19.406	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.640%
36) 1,2-Dichloropropane-d6	9.276	67	100413	19.951	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.800%
41) Toluene-d8	10.325	98	277319	18.073	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.280%
43) trans-1,3-Dichloroprop...	10.575	79	34635	16.545	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.160%
47) 2-Hexanone-d5	10.922	63	26832	32.285	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.580%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	62774	16.691	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	66.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	60459	17.087	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	68.360%#
Target Compounds					Qvalue	
13) Acetone	4.118	43	7277	6.028	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030381.D
Acq On : 03 Oct 2024 19:09
Operator : SY/MD
Sample : P4284-02
Misc : 5.48g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EQ3

Quant Time: Oct 04 01:10:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 04 01:05:34 2024
Response via : Initial Calibration

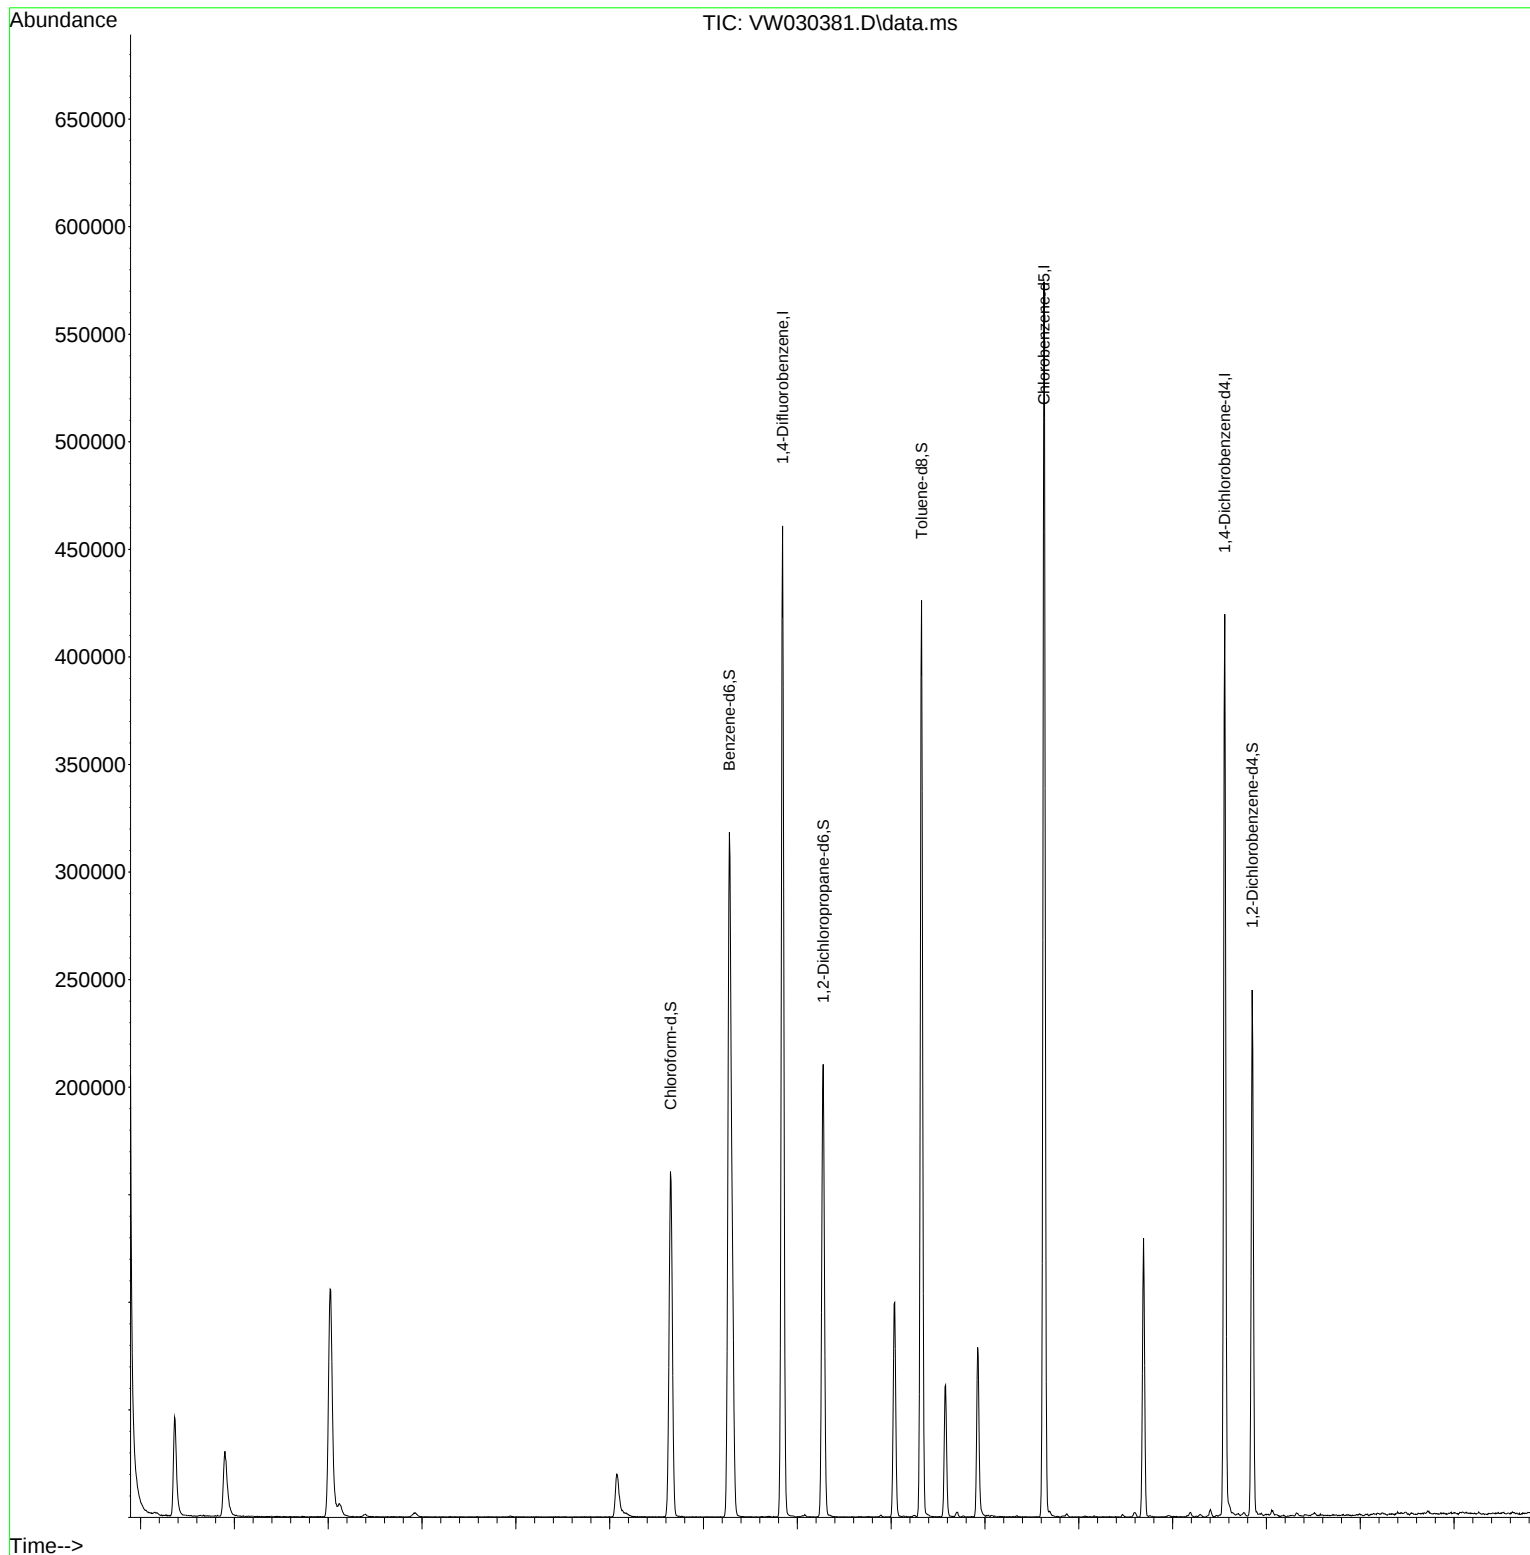

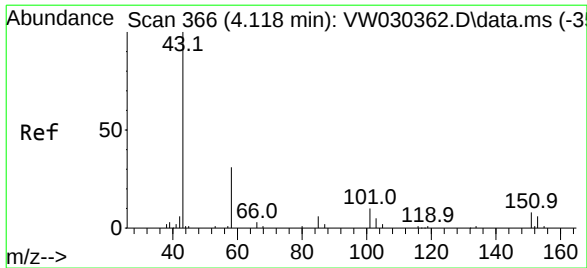

#13
 Acetone
 Concen: 6.028 ug/L
 RT: 4.118 min Scan# 36
 Delta R.T. -0.000 min
 Lab File: VW030381.D
 Acq: 03 Oct 2024 19:09

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ3

Tgt Ion: 43 Resp: 7277
 Ion Ratio Lower Upper
 43 100
 58 29.5 0.0 64.0

