

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030383.D
 Acq On : 03 Oct 2024 19:57
 Operator : SY/MD
 Sample : P4284-04
 Misc : 5.08g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ5

Quant Time: Oct 04 01:11:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	376087	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	340841	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	147987	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	70577	24.015	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.080%
7) Chloroethane-d5	2.899	69	52080	24.356	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.440%
11) 1,1-Dichloroethene-d2	4.021	65	42254	19.697	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.800%
21) 2-Butanone-d5	7.075	46	36118	30.561	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.120%
24) Chloroform-d	7.648	84	187849	18.592	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.360%
26) 1,2-Dichloroethane-d4	8.307	65	92746	17.587	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	70.360%
32) Benzene-d6	8.276	84	369857	19.361	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.440%
36) 1,2-Dichloropropane-d6	9.276	67	112041	19.500	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.000%
41) Toluene-d8	10.325	98	325003	18.554	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.200%
43) trans-1,3-Dichloroprop...	10.574	79	40354	16.886	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.560%
47) 2-Hexanone-d5	10.922	63	27716	29.213	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.420%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	71878	16.742	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	66.960%
66) 1,2-Dichlorobenzene-d4	13.848	152	91764	18.677	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.720%#
Target Compounds					Qvalue	
13) Acetone	4.124	43	11413	9.104	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030383.D
Acq On : 03 Oct 2024 19:57
Operator : SY/MD
Sample : P4284-04
Misc : 5.08g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EQ5

Quant Time: Oct 04 01:11:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 04 01:05:34 2024
Response via : Initial Calibration

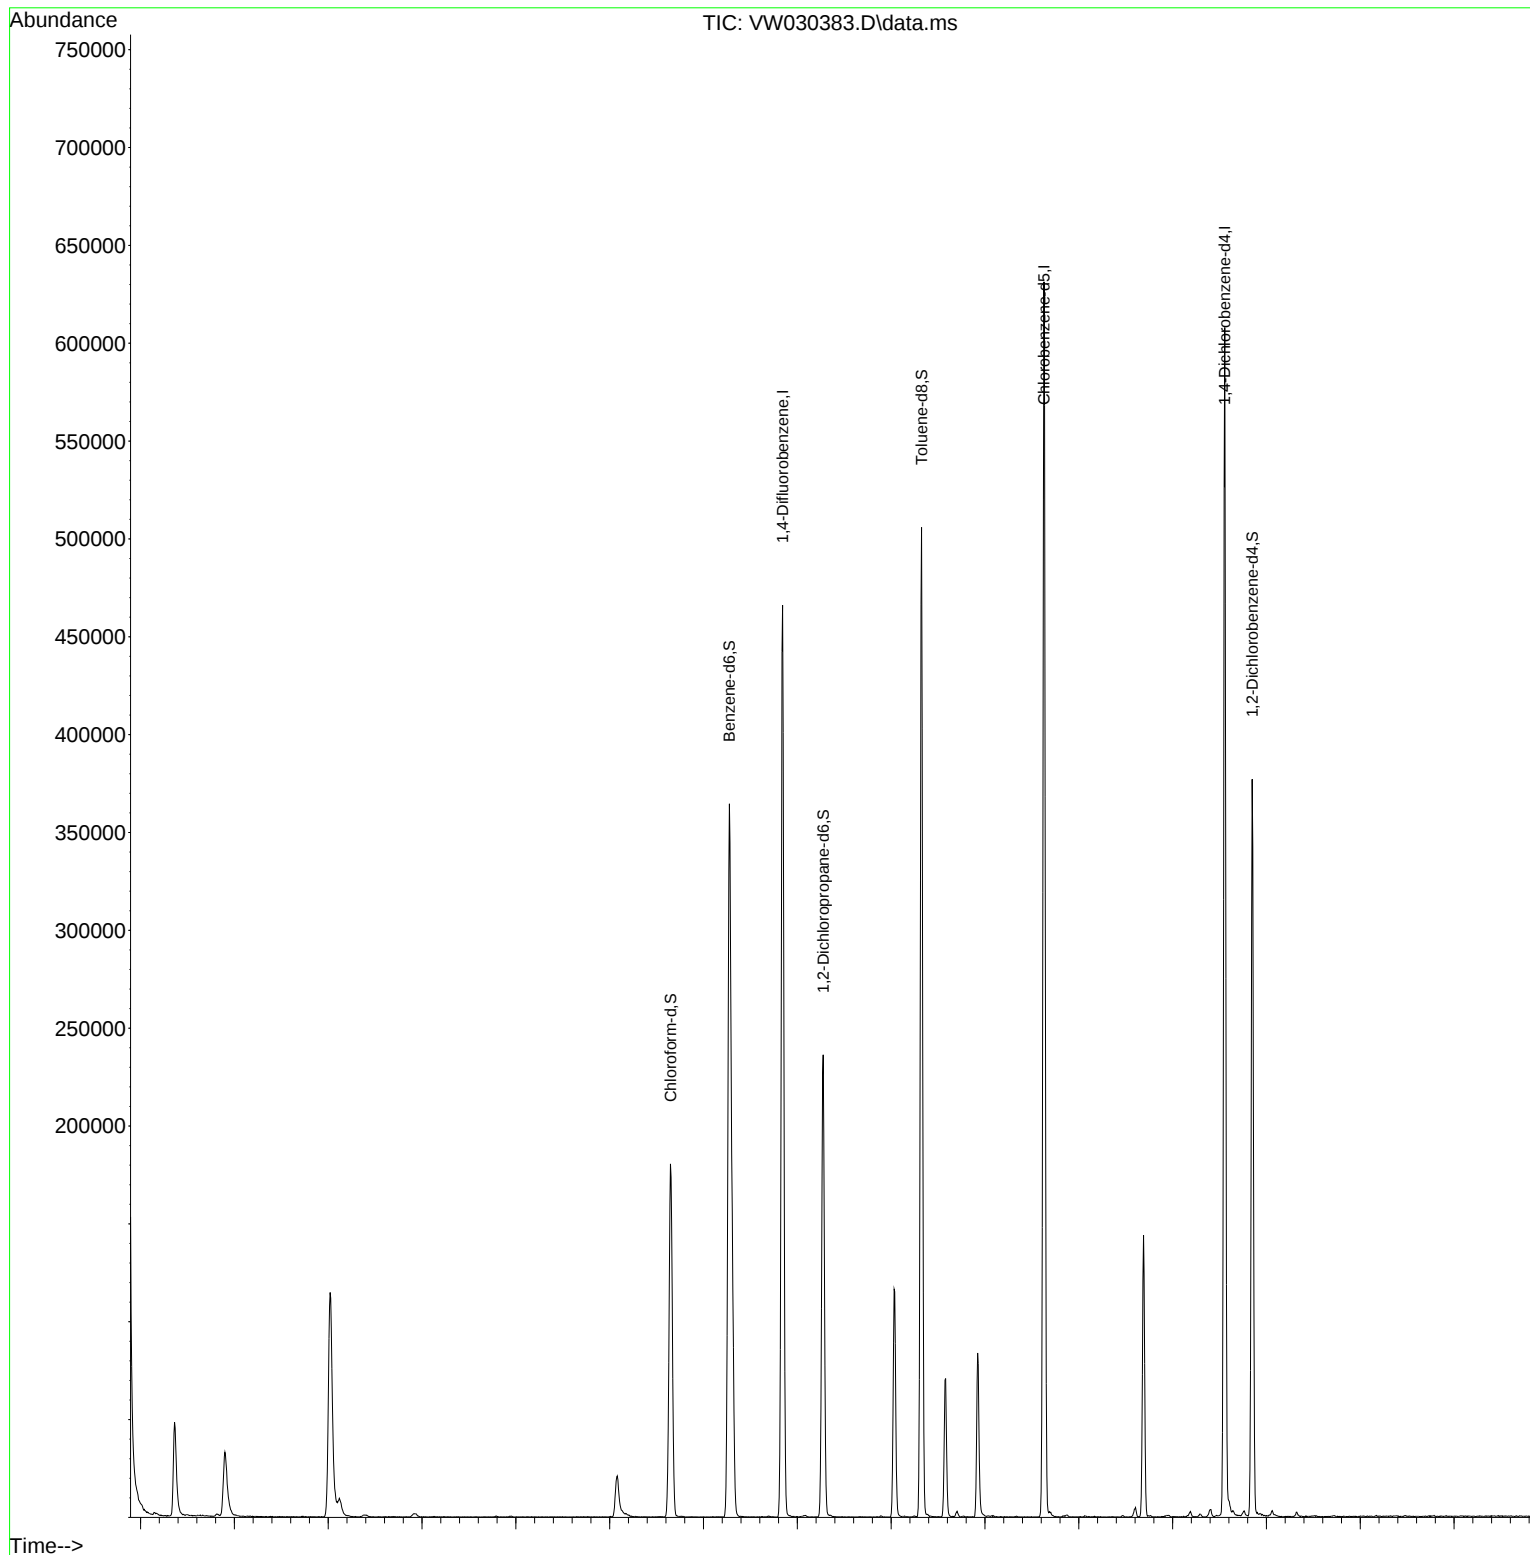

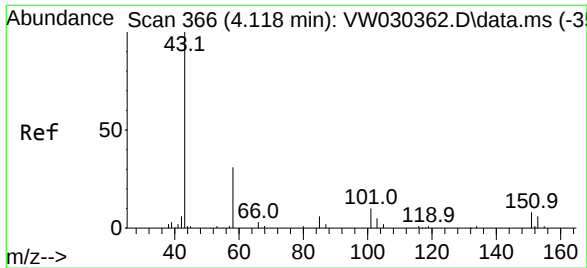

#13
 Acetone
 Concen: 9.104 ug/L
 RT: 4.124 min Scan# 36
 Delta R.T. 0.006 min
 Lab File: VW030383.D
 Acq: 03 Oct 2024 19:57

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ5

Tgt Ion: 43 Resp: 11413
 Ion Ratio Lower Upper
 43 100
 58 31.2 0.0 64.0

