
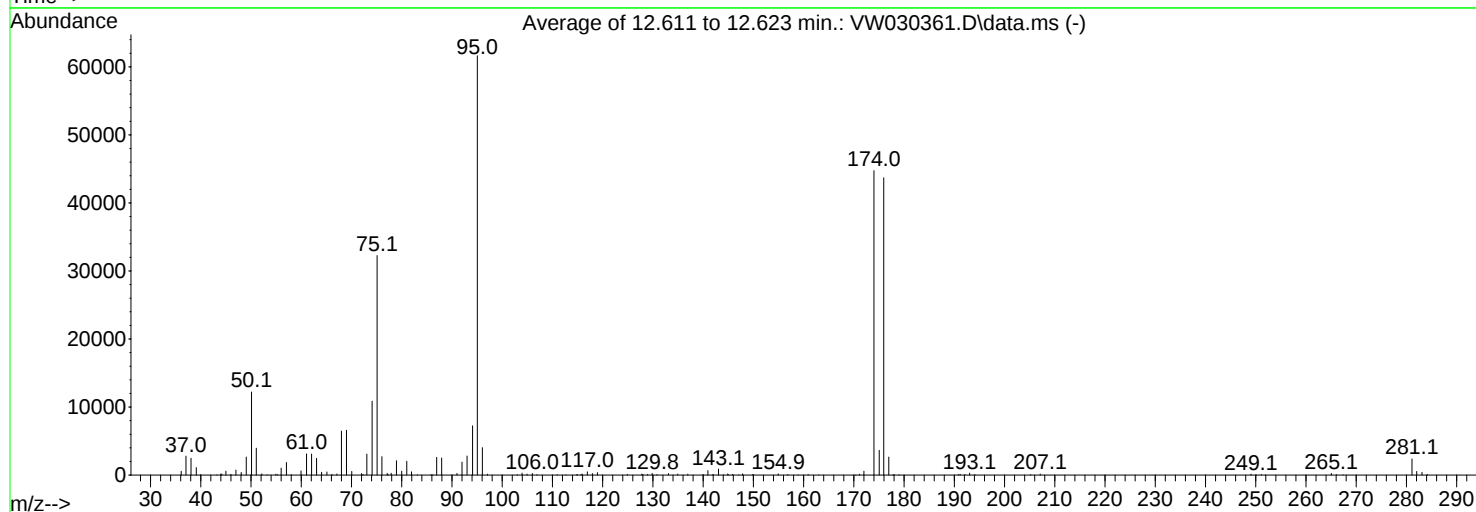


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030361.D
Acq On : 03 Oct 2024 09:09
Operator : SY/MD
Sample : BFB568
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB568

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Title : SFAM01.0
Last Update : Fri Oct 04 01:05:34 2024

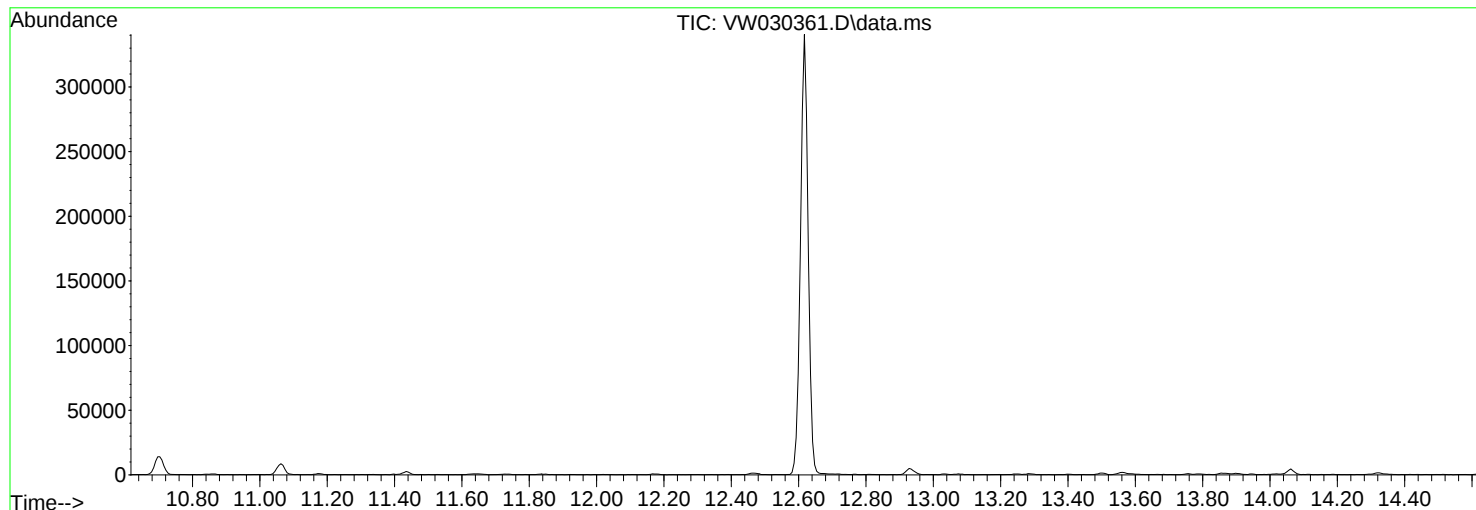

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	12212	PASS
75	95	30	80	52.4	32272	PASS
95	95	100	100	100.0	61637	PASS
96	95	5	9	6.5	4028	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.6	44747	PASS
175	174	5	9	8.1	3641	PASS
176	174	95	101	97.7	43699	PASS
177	176	5	9	6.1	2655	PASS

m/z	Abundance
40.00	134.0
44.00	134.0
281.10	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB568

m/z	Abundance
36.10	692.0
37.10	2707.0
38.10	2568.0
39.10	1009.0
40.00	242.0
44.00	489.0
45.00	623.0
46.10	113.0
47.00	767.0
48.00	333.0
49.10	2791.0
50.10	12175.0
51.10	3964.0
52.20	106.0
53.20	59.0
55.00	279.0
56.00	1108.0
57.00	1930.0
60.00	586.0
61.00	3444.0
62.10	3133.0
63.00	2662.0
64.00	473.0
65.00	614.0
67.20	145.0
68.00	6429.0
69.00	6206.0
70.10	588.0
72.30	300.0
73.10	2898.0
74.10	10402.0
75.10	31400.0
76.10	2485.0
77.10	365.0
78.00	305.0
78.90	2105.0
79.90	578.0
81.00	1898.0
81.90	359.0
83.10	54.0
85.80	102.0
86.20	129.0
86.90	2249.0
88.00	2423.0
91.10	217.0
92.00	1924.0
93.00	2697.0
94.10	6539.0
95.10	58448.0
96.00	3918.0
97.10	154.0
103.00	130.0
103.90	272.0
104.90	191.0
106.00	181.0
106.90	62.0
111.00	111.0
114.80	67.0
115.70	208.0
117.00	452.0
118.00	207.0
119.00	286.0
125.00	133.0
127.80	196.0
129.00	82.0
129.90	236.0
133.10	286.0
135.00	159.0
137.00	118.0
140.10	78.0
140.90	556.0
142.00	110.0
143.10	732.0
144.10	56.0
144.90	346.0
145.80	105.0
147.10	71.0
147.80	146.0
149.90	106.0
154.90	139.0
156.90	59.0
160.90	72.0
163.00	60.0
171.10	182.0
172.00	706.0
174.00	34848.0
175.00	3314.0
176.00	38024.0
177.00	2185.0
177.80	128.0
179.00	137.0
190.80	237.0

Instrument :
MSVOA_W
ClientSampleId :
BFB568

191.30	159.0
192.10	89.0
193.00	583.0
194.10	61.0
205.20	81.0
207.10	320.0
249.10	230.0
250.10	66.0
251.10	114.0
251.90	52.0
265.00	376.0
266.10	66.0
267.40	72.0
281.10	3759.0
282.10	854.0
283.10	471.0
284.20	156.0

Instrument :
MSVOA_W
ClientSampleId :
BFB568

m/z	Abundance
36.10	546.0
37.00	3257.0
38.00	2726.0
39.10	1363.0
39.90	148.0
43.20	56.0
44.00	425.0
45.00	570.0
45.90	109.0
47.00	862.0
48.00	440.0
49.00	2938.0
50.10	13396.0
51.00	4599.0
52.20	276.0
55.30	198.0
56.00	1167.0
57.10	1971.0
58.00	81.0
60.00	766.0
61.10	3104.0
62.00	3455.0
63.10	2537.0
64.10	408.0
65.10	433.0
66.00	53.0
67.10	160.0
68.00	7608.0
69.00	7256.0
70.00	571.0
72.00	329.0
73.00	3514.0
74.10	12224.0
75.10	36224.0
76.10	3165.0
77.10	413.0
77.80	320.0
79.00	2437.0
80.00	607.0
81.00	2339.0
82.00	750.0
83.10	62.0
85.90	70.0
87.00	2856.0
87.90	2520.0
90.90	258.0
92.00	2134.0
93.00	3076.0
94.10	8044.0
95.10	70704.0
96.10	4418.0
97.00	114.0
103.00	67.0
104.00	314.0
105.00	133.0
106.00	244.0
106.90	109.0
110.90	66.0
115.00	96.0
115.90	268.0
117.00	525.0
117.90	242.0
119.00	411.0
124.90	124.0
127.80	280.0
128.90	114.0
129.90	300.0
130.80	123.0
133.20	267.0
134.90	150.0
136.90	139.0
139.90	96.0
141.00	722.0
141.80	90.0
143.00	980.0
144.90	190.0
145.90	115.0
147.90	230.0
149.90	132.0
155.00	263.0
156.80	82.0
161.00	91.0
171.20	112.0
172.10	566.0
174.00	53464.0
175.10	3873.0
176.00	49224.0
177.00	3184.0
178.00	106.0
191.10	141.0
192.10	101.0
193.10	234.0

Instrument :
MSVOA_W
ClientSampleId :
BFB568

194.10	92.0
205.20	80.0
207.10	157.0
248.90	118.0
251.10	70.0
265.10	245.0
266.10	59.0
281.10	2526.0
282.00	526.0
283.10	521.0
284.20	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB568

m/z	Abundance
36.10	456.0
37.10	2390.0
38.00	2134.0
39.10	942.0
39.90	127.0
44.20	423.0
45.00	536.0
46.00	88.0
47.00	577.0
48.10	378.0
49.00	2233.0
50.10	11065.0
51.10	3284.0
52.00	154.0
54.90	152.0
56.00	800.0
57.00	1637.0
58.00	77.0
59.90	508.0
61.10	2795.0
62.10	2702.0
63.00	2189.0
64.10	353.0
65.20	340.0
66.20	53.0
67.00	211.0
68.00	5347.0
69.00	6291.0
70.00	452.0
72.00	345.0
73.10	2827.0
74.10	9975.0
75.10	29192.0
76.00	2489.0
77.30	159.0
77.80	204.0
79.00	1782.0
80.10	533.0
81.00	1877.0
82.00	358.0
86.90	2703.0
87.90	2600.0
91.00	278.0
92.00	1657.0
93.00	2649.0
94.10	7153.0
95.00	55760.0
96.10	3748.0
97.10	151.0
104.00	272.0
104.90	124.0
106.00	265.0
112.70	65.0
114.90	145.0
115.90	194.0
116.90	465.0
117.90	252.0
118.90	403.0
124.80	61.0
128.00	215.0
128.90	109.0
129.80	212.0
130.80	97.0
133.00	129.0
135.00	140.0
136.90	168.0
139.90	52.0
140.90	695.0
142.00	121.0
143.00	943.0
145.10	134.0
145.90	104.0
147.90	167.0
149.90	73.0
154.90	121.0
156.90	93.0
158.90	57.0
160.80	92.0
170.40	54.0
171.00	94.0
171.90	477.0
174.00	45928.0
175.00	3735.0
175.90	43848.0
176.90	2595.0
178.00	94.0
191.00	71.0
192.90	52.0
249.10	78.0
251.00	55.0
265.00	116.0
281.20	1030.0

Instrument :
MSVOA_W
ClientSampleId :
BFB568

282.10231.0

283.00212.0

Instrument :
MSVOA_W
ClientSampleId :
BFB568