

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100422\
 Data File : VW024722.D
 Acq On : 04 Oct 2022 18:20
 Operator : SY/VA
 Sample : N4973-02
 Misc : 6.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY197

Quant Time: Oct 05 07:19:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 22:12:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	219685	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	179805	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	55530	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	30796	13.398	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.600%
7) Chloroethane-d5	2.885	69	21621	16.187	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.760%
11) 1,1-Dichloroethene-d2	4.013	63	52158	9.804	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	39.200%#
21) 2-Butanone-d5	7.080	46	61615	74.562	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	149.120%#
24) Chloroform-d	7.647	84	128055	21.804	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.200%
26) 1,2-Dichloroethane-d4	8.305	65	74094	24.320	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.280%
32) Benzene-d6	8.275	84	208642	18.155	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	72.600%
36) 1,2-Dichloropropane-d6	9.275	67	82226	23.417	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.680%
41) Toluene-d8	10.323	98	141961	13.821	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	55.280%
43) trans-1,3-Dichloroprop...	10.573	79	24278	15.526	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	62.120%
47) 2-Hexanone-d5	10.927	63	40229	66.961	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	133.920%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	85673	34.243	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	136.960%#
66) 1,2-Dichlorobenzene-d4	13.847	152	43718	22.373	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.480%
Target Compounds					Qvalue	
13) Acetone	4.135	43	2685	4.453	ug/L	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100422\
Data File : VW024722.D
Acq On : 04 Oct 2022 18:20
Operator : SY/VA
Sample : N4973-02
Misc : 6.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY197

Quant Time: Oct 05 07:19:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 30 22:12:13 2022
Response via : Initial Calibration

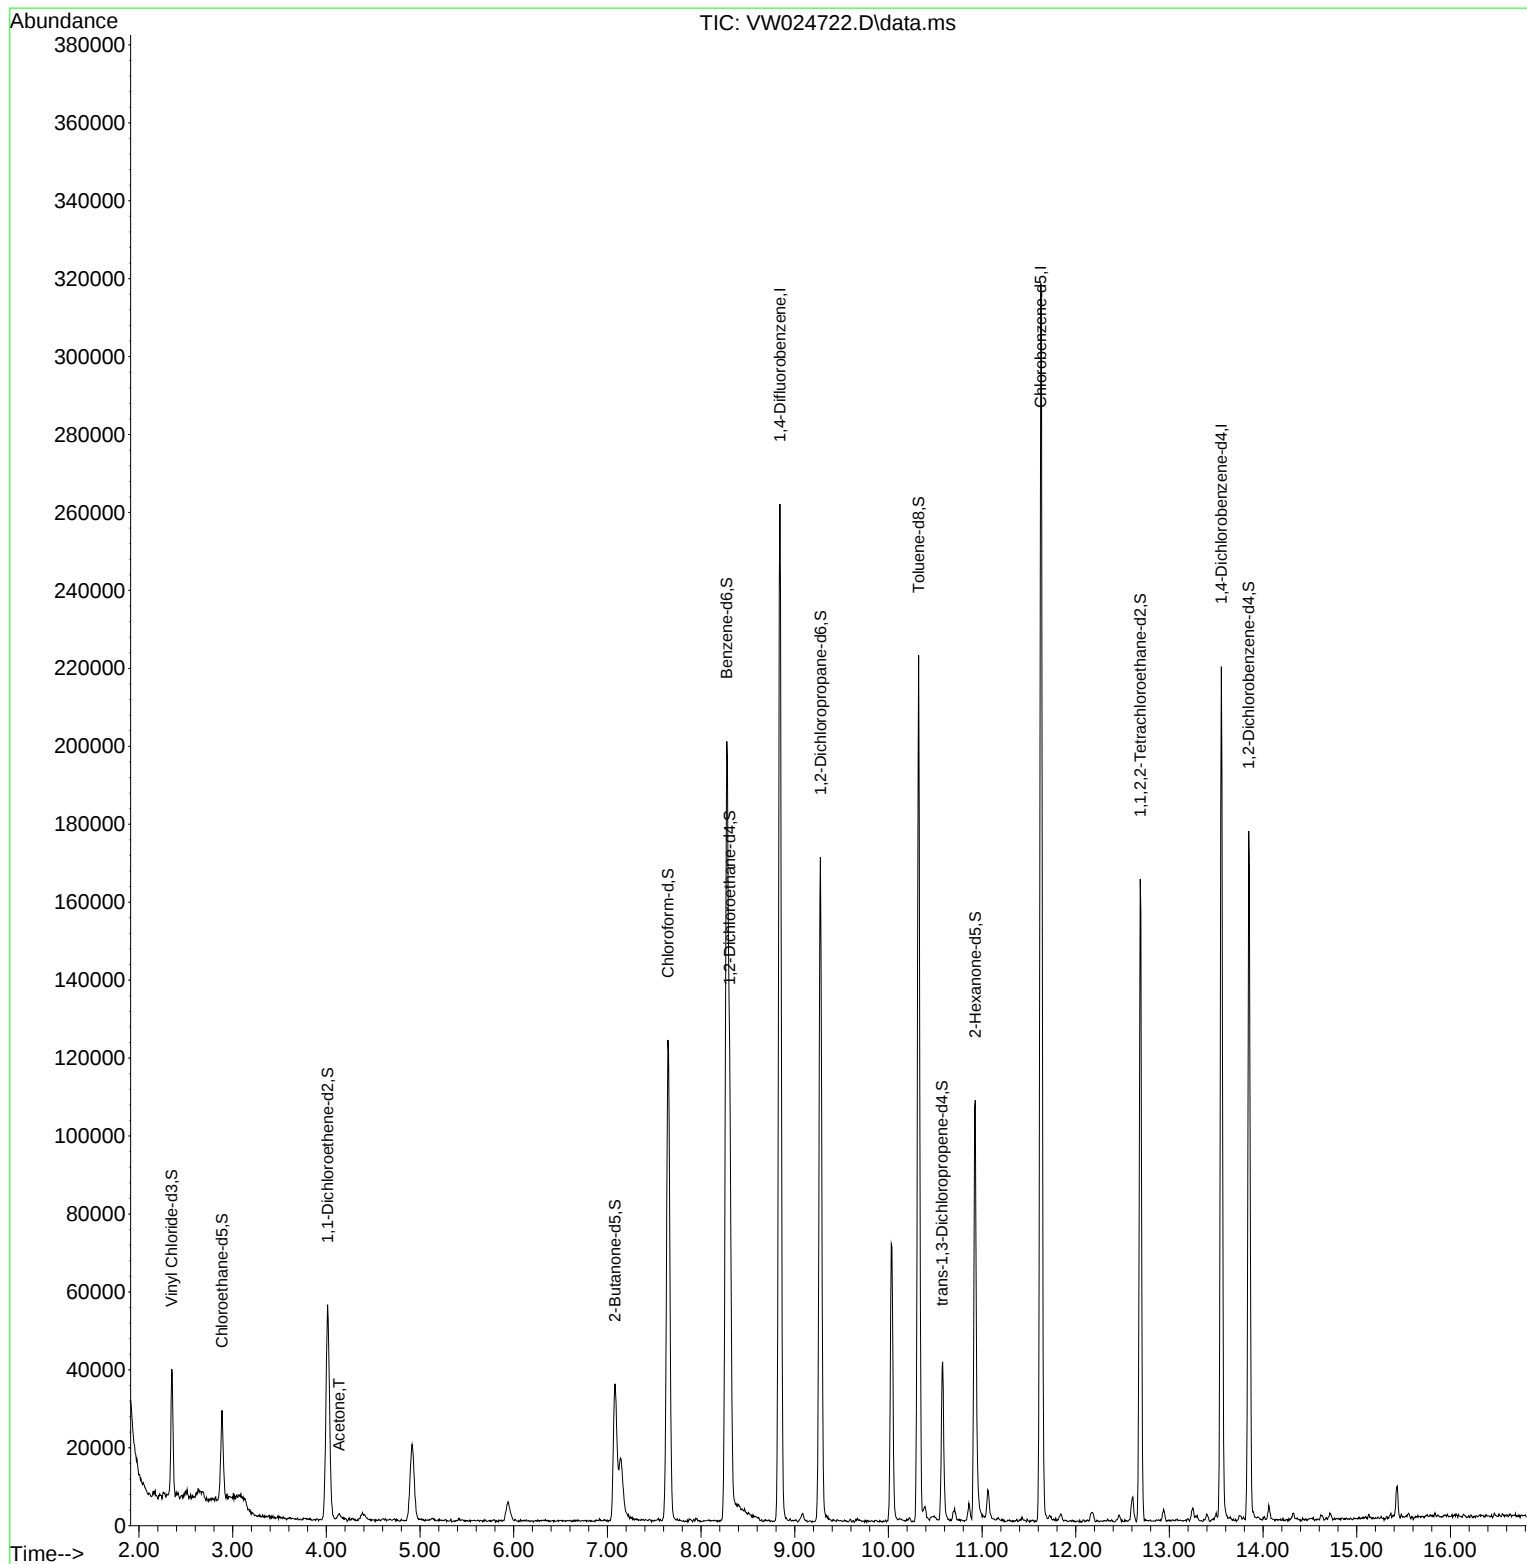

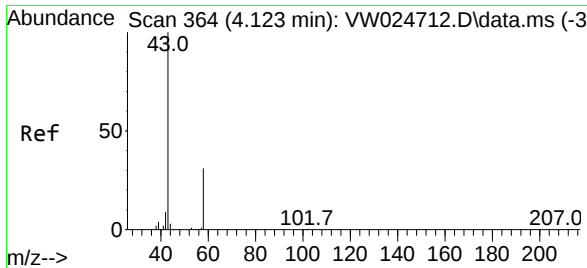

#13
 Acetone
 Concen: 4.453 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW024722.D
 Acq: 04 Oct 2022 18:20

Instrument :
 MSVOA_W
 ClientSampleId :
 EY197

Tgt Ion: 43 Resp: 2685
 Ion Ratio Lower Upper
 43 100
 58 7.0 0.0 67.6

