
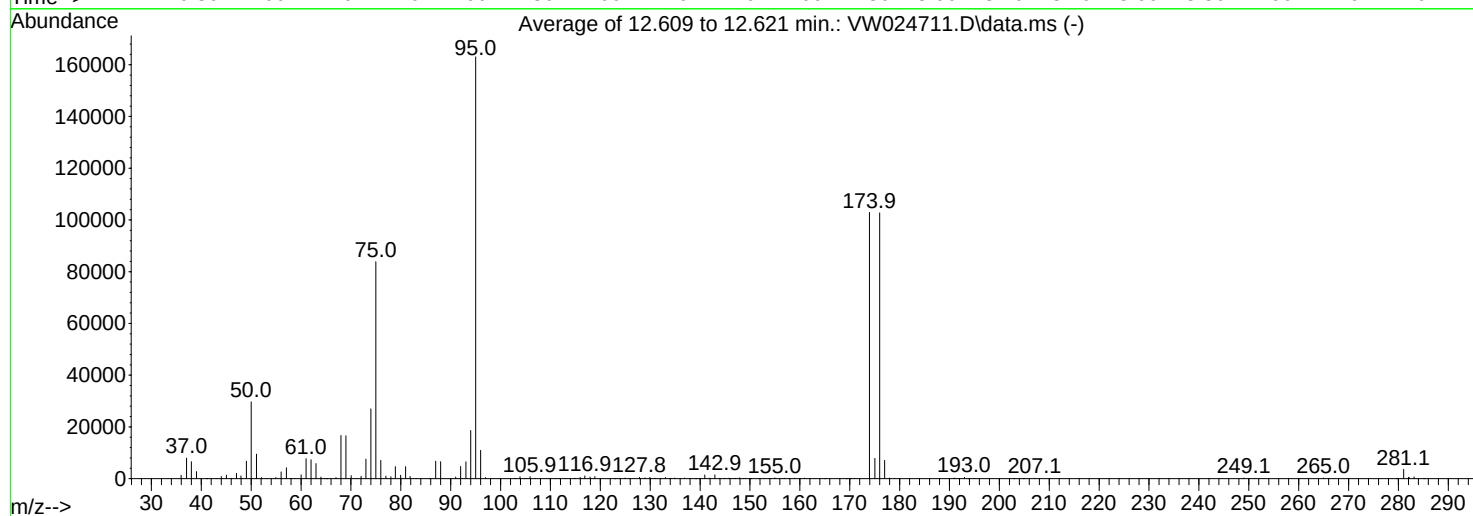


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100422\
 Data File : VW024711.D
 Acq On : 04 Oct 2022 07:59
 Operator : SY/VA
 Sample : BFB435
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB435

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Title : SFAM01.0
 Last Update : Fri Oct 07 03:04:02 2022

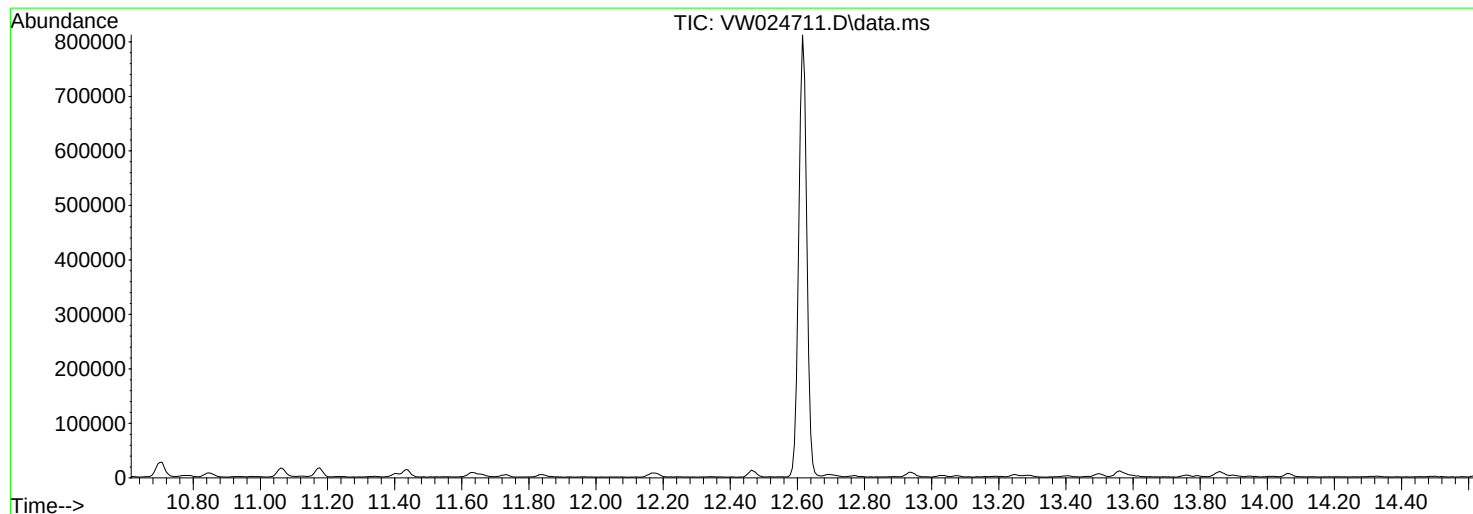

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	29675	PASS
75	95	30	80	51.4	83888	PASS
95	95	100	100	100.0	163051	PASS
96	95	5	9	6.7	10935	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	63.1	102915	PASS
175	174	5	9	7.6	7845	PASS
176	174	95	105	99.8	102739	PASS
177	176	5	10	6.9	7051	PASS

m/z	Abundance
35.90	100.0
39.90	633.0
43.00	75.0
44.00	712.0
56.80	55.0
207.00	100.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

m/z	Abundance
36.00	1515.0
37.10	7715.0
38.00	6448.0
39.10	2525.0
40.00	689.0
41.10	58.0
43.00	153.0
44.00	1584.0
45.10	1462.0
46.10	191.0
47.00	1887.0
48.00	973.0
49.00	7065.0
50.00	27424.0
51.00	9221.0
52.20	284.0
53.10	75.0
55.00	446.0
56.00	2169.0
57.00	4055.0
57.90	208.0
58.80	197.0
60.00	1320.0
61.00	7629.0
62.00	7188.0
63.00	5371.0
64.00	548.0
64.80	70.0
67.00	460.0
68.00	15767.0
69.00	15925.0
70.00	1071.0
71.10	126.0
72.10	837.0
73.00	7027.0
74.00	25728.0
75.00	79400.0
76.00	6979.0
77.00	1003.0
78.00	684.0
78.90	4142.0
80.00	1328.0
81.00	4296.0
81.90	736.0
83.30	78.0
85.80	114.0
87.00	6222.0
88.00	5656.0
91.00	683.0
92.00	4350.0
93.00	6021.0
94.00	17560.0
95.00	146176.0
96.00	10018.0
97.00	426.0
102.90	178.0
103.90	716.0
104.90	257.0
106.00	725.0
106.90	126.0
109.90	164.0
110.90	120.0
113.00	99.0
114.80	172.0
115.00	174.0
115.90	445.0
116.90	914.0
118.00	606.0
118.90	718.0
123.90	106.0
125.10	303.0
126.00	94.0
127.80	429.0
128.90	218.0
130.00	485.0
130.90	151.0
133.10	693.0
133.90	251.0
134.90	267.0
136.90	254.0
139.90	116.0
141.00	1443.0
141.90	271.0
143.00	1237.0
143.90	107.0
144.80	137.0
145.80	201.0
147.10	165.0
147.90	315.0
148.70	163.0
149.80	111.0
152.90	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

154.00	82.0
155.00	354.0
156.90	139.0
158.00	82.0
158.90	192.0
161.00	157.0
163.10	53.0
165.00	64.0
171.00	116.0
174.00	86016.0
175.00	6431.0
176.00	86856.0
177.00	6124.0
178.00	300.0
179.00	187.0
190.90	484.0
191.80	103.0
193.00	737.0
193.80	107.0
194.10	109.0
195.10	112.0
202.90	59.0
204.80	105.0
207.20	353.0
208.00	130.0
249.10	463.0
250.10	106.0
251.20	75.0
265.00	320.0
266.10	93.0
267.00	140.0
279.60	78.0
281.10	5327.0
282.00	1524.0
283.10	945.0
284.10	218.0
285.10	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

m/z	Abundance
36.00	1686.0
37.00	8439.0
38.00	6821.0
39.10	2955.0
40.00	839.0
43.00	230.0
44.10	1538.0
45.10	1442.0
46.20	109.0
47.00	2634.0
48.00	1128.0
49.10	6650.0
50.00	32600.0
51.10	9793.0
52.10	575.0
53.10	60.0
54.90	459.0
56.00	3043.0
57.00	4832.0
58.10	254.0
60.00	1792.0
61.00	8296.0
62.00	8297.0
63.00	6650.0
64.00	649.0
65.10	85.0
67.00	391.0
68.00	18320.0
69.00	18624.0
70.10	1542.0
71.20	72.0
71.90	1084.0
73.00	8747.0
74.00	29000.0
75.00	90576.0
76.00	8007.0
77.00	1191.0
77.90	842.0
78.90	5465.0
79.90	1341.0
81.00	5077.0
81.90	993.0
83.20	128.0
87.00	7182.0
88.00	7484.0
91.00	598.0
92.00	4924.0
93.00	6964.0
94.00	20192.0
95.00	188672.0
96.00	12302.0
97.00	358.0
103.10	147.0
103.90	724.0
104.80	185.0
105.80	904.0
107.00	126.0
109.70	68.0
110.10	110.0
110.90	170.0
111.80	90.0
112.80	145.0
114.80	155.0
116.00	449.0
116.90	940.0
117.90	702.0
118.90	953.0
122.90	55.0
124.00	199.0
124.90	243.0
125.90	56.0
127.90	492.0
129.00	336.0
130.00	638.0
131.00	267.0
132.00	57.0
133.00	454.0
134.10	169.0
134.90	246.0
136.90	263.0
139.90	190.0
140.90	1552.0
141.80	210.0
142.90	1549.0
144.00	154.0
145.00	111.0
145.80	147.0
147.10	126.0
148.00	325.0
149.10	196.0
149.90	171.0
151.80	132.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

152.80	118.0
153.80	89.0
155.00	300.0
156.90	272.0
158.90	181.0
160.90	228.0
162.90	69.0
171.00	126.0
174.00	110424.0
175.00	8301.0
176.00	110544.0
177.00	7341.0
178.00	240.0
178.90	139.0
191.10	389.0
191.80	64.0
193.10	479.0
194.00	108.0
195.10	89.0
205.10	140.0
207.10	275.0
249.00	303.0
249.90	107.0
251.10	57.0
264.90	237.0
266.10	124.0
267.10	65.0
281.00	3761.0
282.20	1005.0
283.20	706.0
284.00	148.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

m/z	Abundance
36.00	1084.0
37.00	7616.0
38.00	6316.0
39.00	2710.0
40.00	653.0
43.00	64.0
44.00	1380.0
45.00	1205.0
46.00	134.0
47.10	1683.0
47.90	978.0
49.00	6448.0
50.00	29000.0
51.00	9448.0
52.00	376.0
54.90	423.0
56.00	2590.0
57.10	3808.0
58.00	171.0
60.00	1366.0
61.00	7210.0
62.00	6457.0
63.00	5363.0
64.00	622.0
64.80	63.0
67.00	464.0
68.00	16046.0
69.00	15291.0
70.00	1030.0
71.20	83.0
72.10	868.0
73.00	6969.0
74.00	26240.0
75.00	81688.0
76.00	6124.0
77.00	828.0
78.10	704.0
78.90	4389.0
80.00	1200.0
80.90	4543.0
81.80	916.0
83.00	141.0
86.00	201.0
87.00	6800.0
88.00	6512.0
91.00	585.0
92.00	4784.0
93.10	6588.0
94.00	18136.0
95.00	154304.0
96.00	10485.0
97.00	485.0
102.70	148.0
103.90	759.0
105.10	234.0
105.90	709.0
106.90	167.0
110.00	61.0
111.00	175.0
111.80	125.0
112.90	198.0
114.90	149.0
116.00	583.0
116.90	1264.0
117.90	644.0
118.90	693.0
123.80	119.0
124.80	142.0
125.80	52.0
127.90	648.0
128.90	349.0
129.90	435.0
131.00	195.0
132.90	217.0
133.90	157.0
135.00	308.0
136.90	174.0
139.10	78.0
139.70	51.0
140.90	1247.0
142.00	189.0
142.90	1749.0
144.00	93.0
144.90	240.0
145.80	259.0
146.80	166.0
148.00	287.0
149.00	115.0
150.10	104.0
151.90	123.0
152.90	154.0
153.70	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435

155.00	306.0
156.70	182.0
157.80	98.0
159.00	187.0
161.00	164.0
169.30	62.0
170.10	80.0
170.90	111.0
172.00	283.0
173.90	112304.0
175.10	8803.0
176.00	110816.0
177.00	7688.0
177.90	197.0
178.90	116.0
191.20	93.0
192.90	282.0
194.00	62.0
195.10	52.0
205.00	54.0
207.20	204.0
248.80	191.0
249.90	65.0
265.10	185.0
267.10	53.0
281.10	1649.0
282.10	550.0
283.10	328.0
284.00	79.0

Instrument :
MSVOA_W
ClientSampleId :
BFB435