




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100423\
 Data File : VW027220.D
 Acq On : 04 Oct 2023 16:15
 Operator : SY/MD
 Sample : 04747-06
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EX841

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/05/2023
 Supervised By :Mahesh Dadoda 10/05/2023

Quant Time: Oct 04 22:52:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 22:49:04 2023
 Response via : Initial Calibration

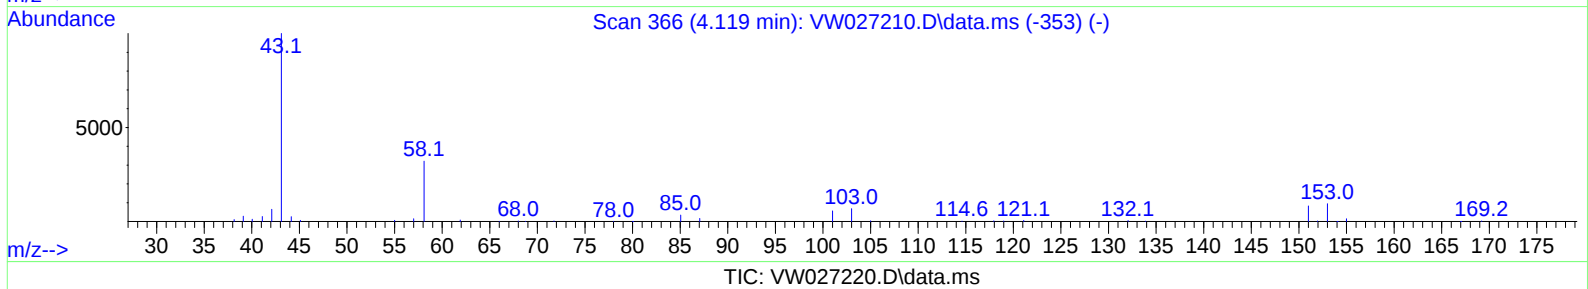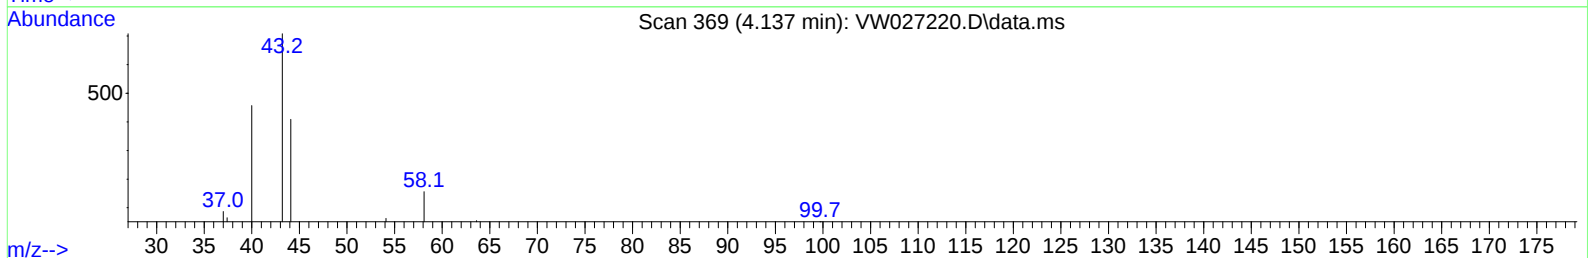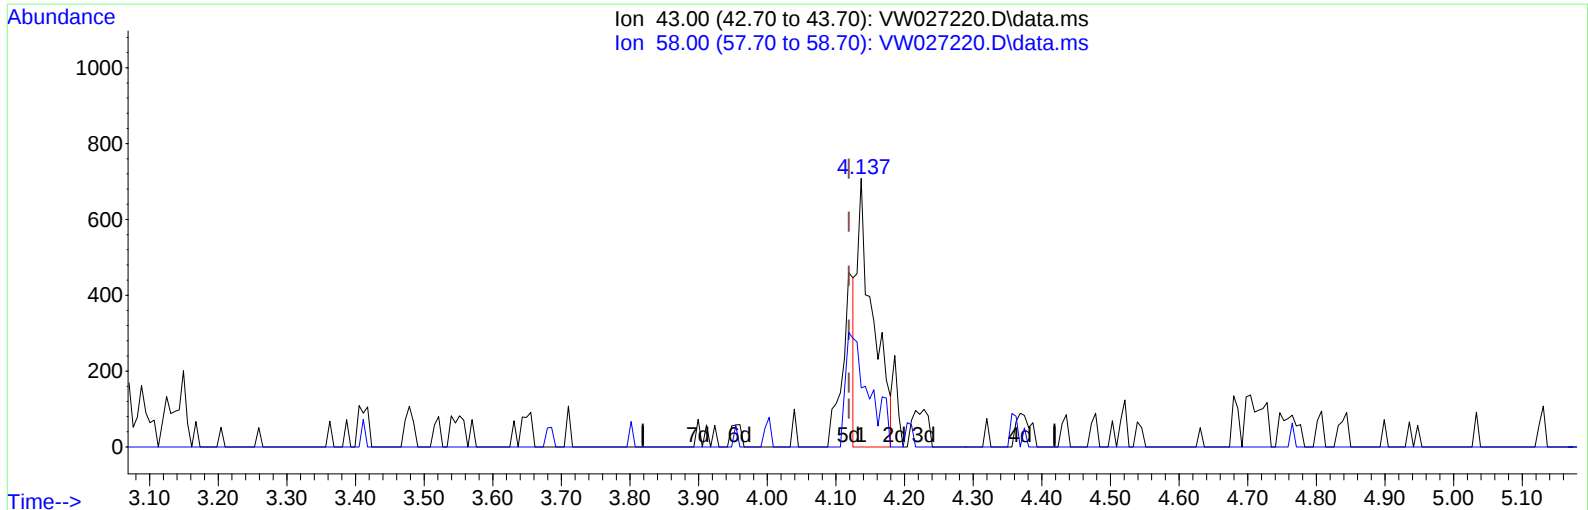

(13) Acetone (T)

4.137min (+ 0.018) 4.66 ug/L

response 1148

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	35.20	8.36
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100423\
 Data File : VW027220.D
 Acq On : 04 Oct 2023 16:15
 Operator : SY/MD
 Sample : 04747-06
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EX841

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/05/2023
 Supervised By :Mahesh Dadoda 10/05/2023

Quant Time: Oct 04 22:52:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 22:49:04 2023
 Response via : Initial Calibration

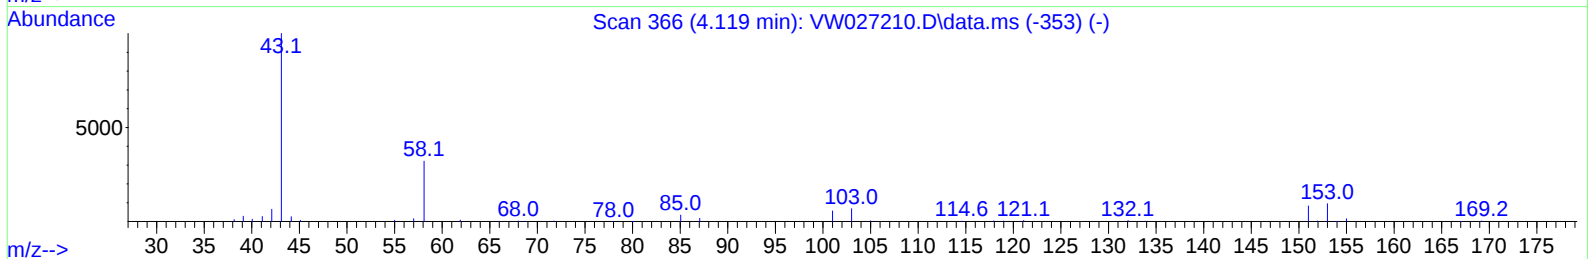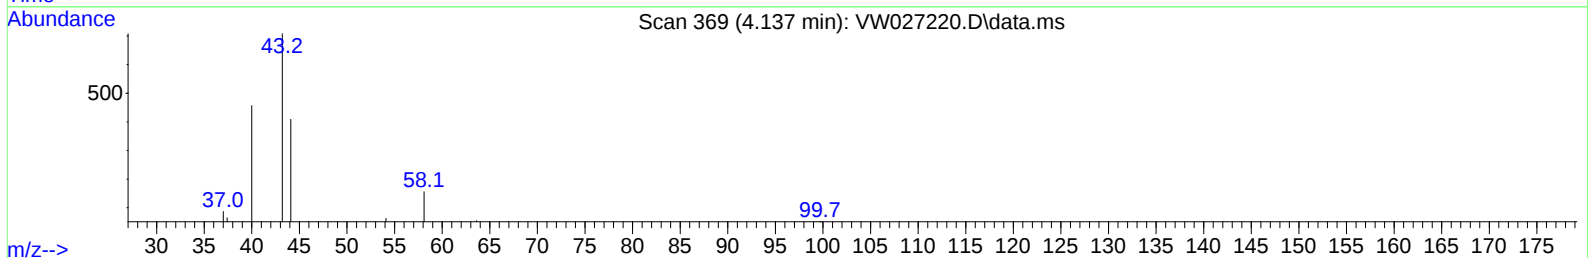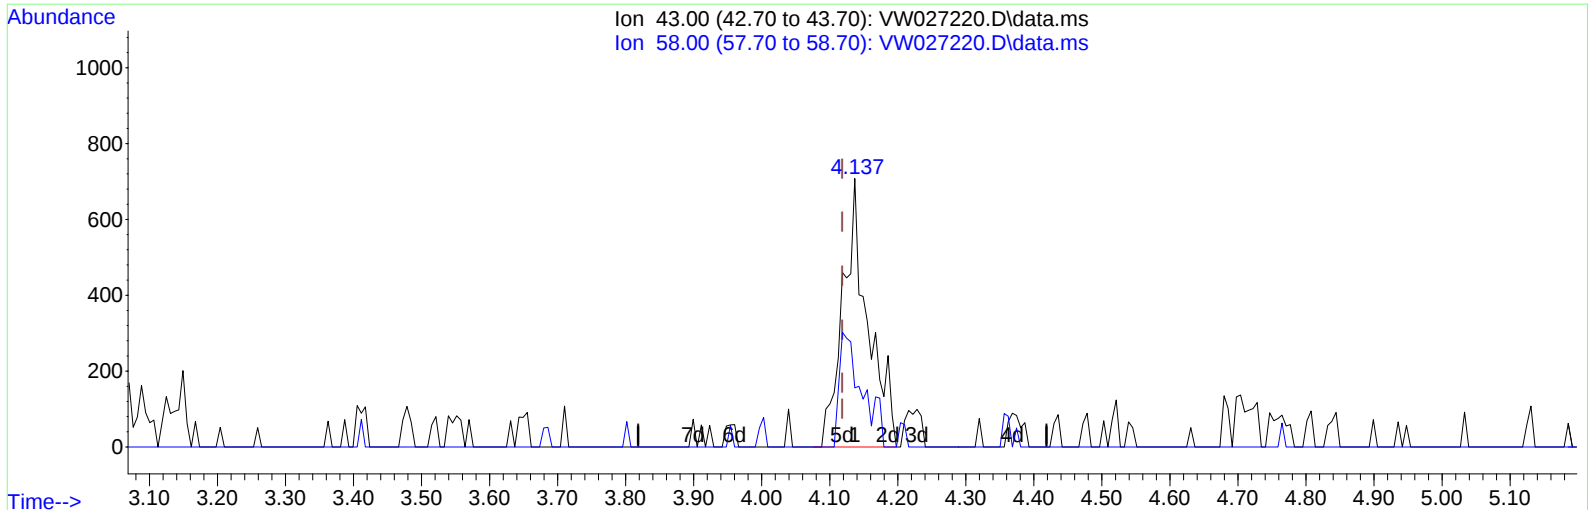

TIC: VW027220.D\data.ms

(13) Acetone (T)

4.137min (+ 0.018) 7.36 ug/L m

response 1814

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	35.20	5.29
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100423\
Data File : VW027220.D
Acq On : 04 Oct 2023 16:15
Operator : SY/MD
Sample : 04747-06
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX841

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/05/2023
Supervised By :Mahesh Dadoda 10/05/2023

Quant Time: Oct 04 22:52:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 22:49:04 2023
Response via : Initial Calibration

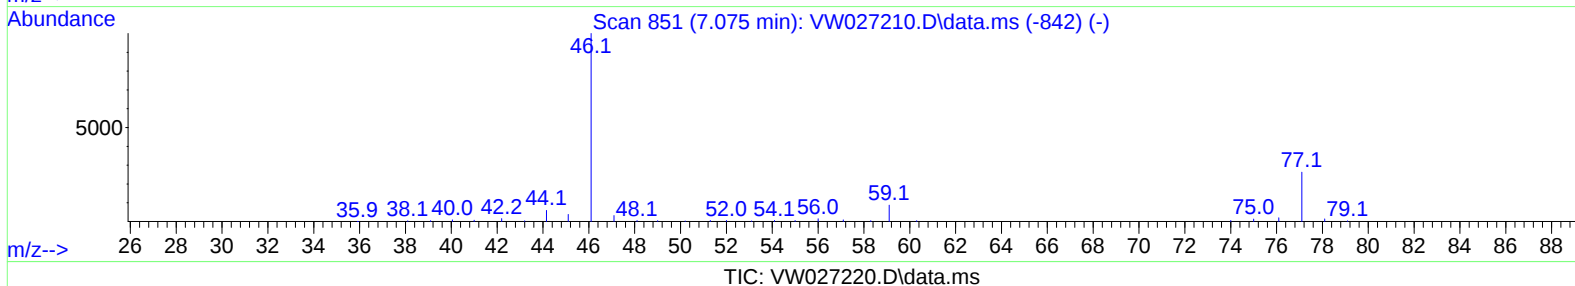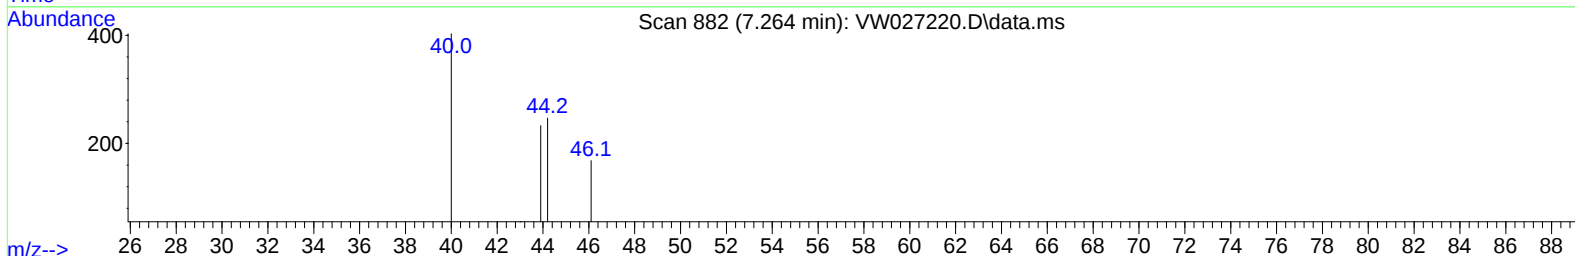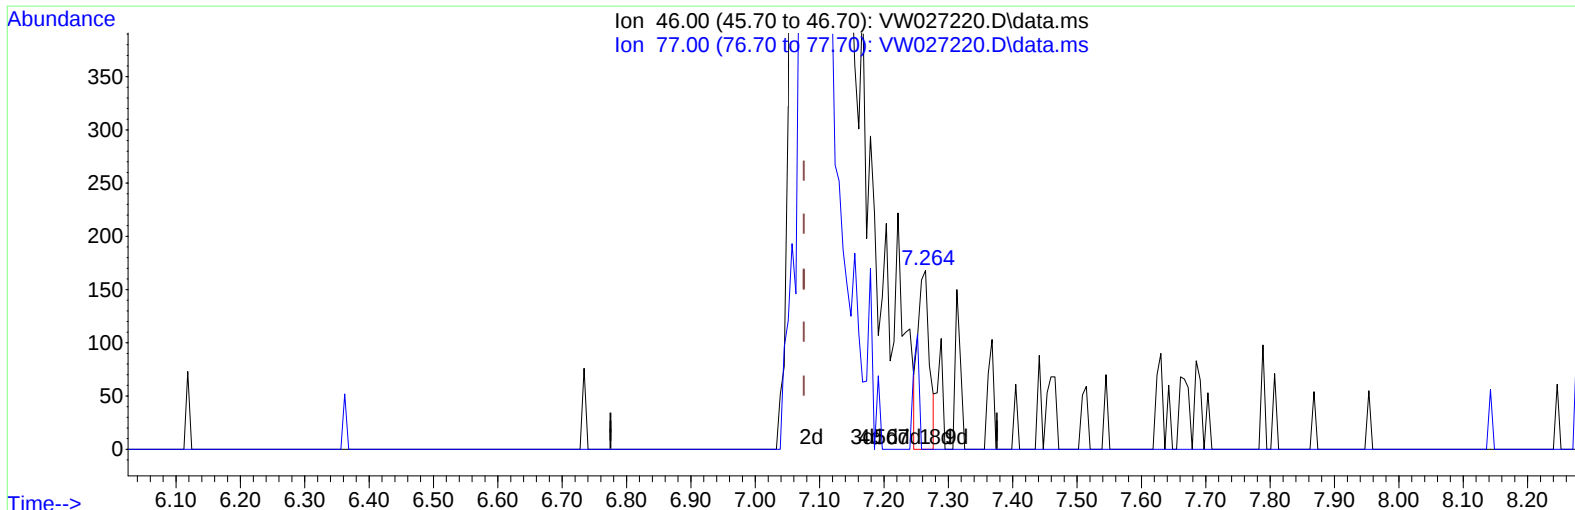

TIC: VW027220.D\data.ms

(21) 2-Butanone-d5 (S)

7.264min (+ 0.189) 1.03 ug/L

response 206

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	33.01
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100423\
Data File : VW027220.D
Acq On : 04 Oct 2023 16:15
Operator : SY/MD
Sample : 04747-06
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX841

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/05/2023
Supervised By :Mahesh Dadoda 10/05/2023

Quant Time: Oct 04 22:52:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 22:49:04 2023
Response via : Initial Calibration

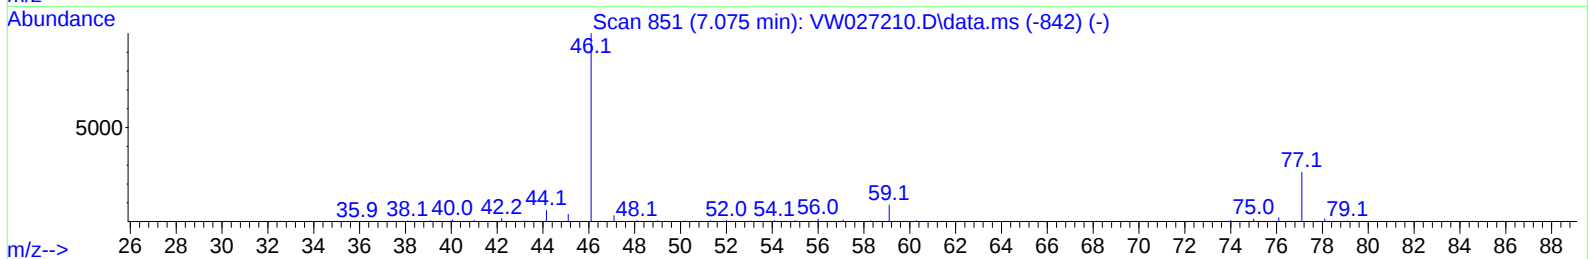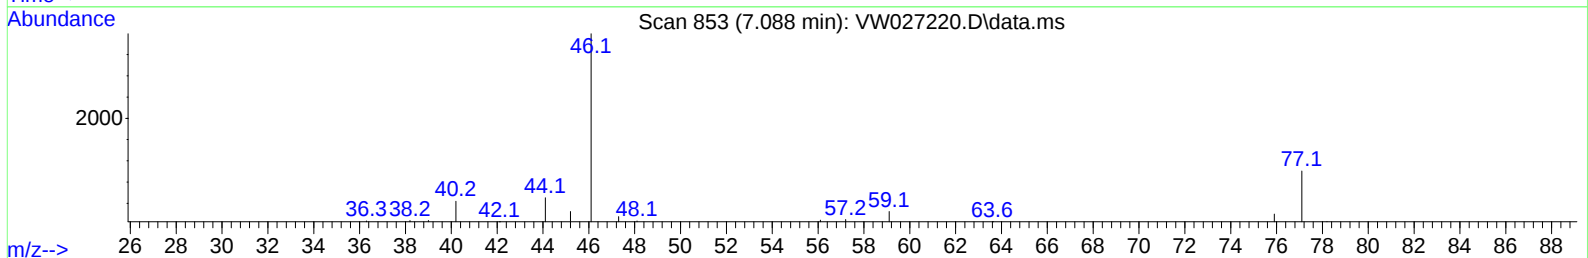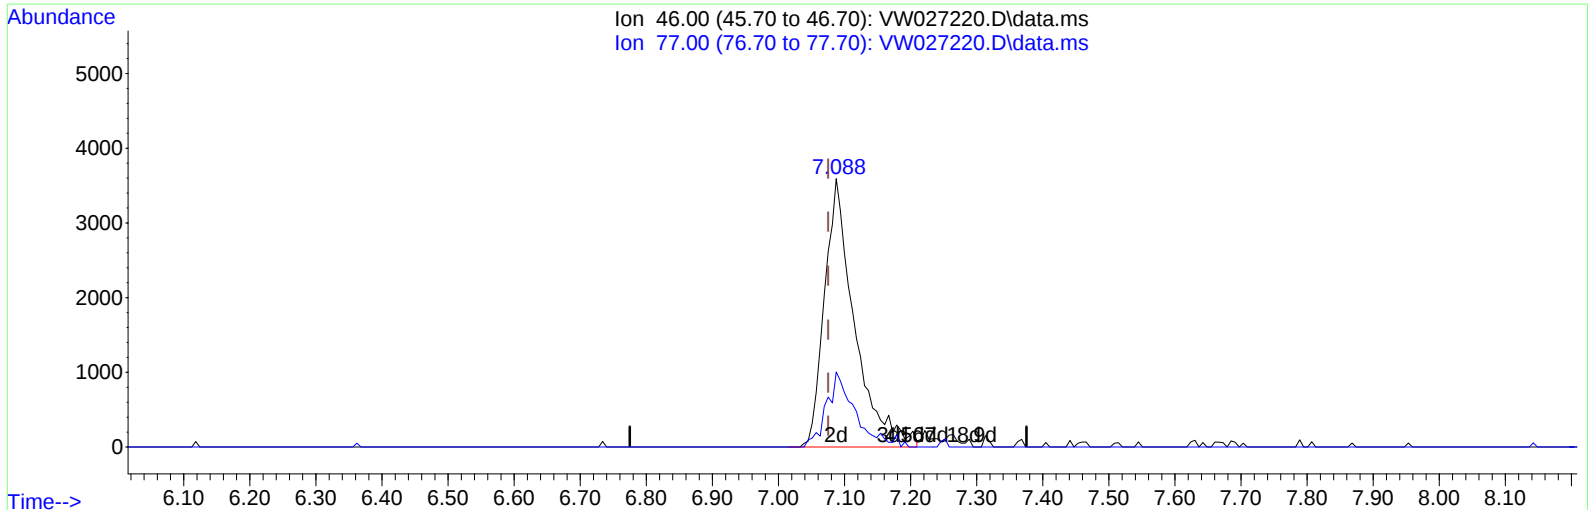

TIC: VW027220.D\data.ms

(21) 2-Butanone-d5 (S)

7.088min (+ 0.012) 57.06 ug/L m

response 11374

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.60#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100423\
 Data File : VW027220.D
 Acq On : 04 Oct 2023 16:15
 Operator : SY/MD
 Sample : 04747-06
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EX841

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/05/2023
 Supervised By :Mahesh Dadoda 10/05/2023

Quant Time: Oct 04 22:52:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 22:49:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.849	114	61367	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	60471	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	23377	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	29904	31.015	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	124.040%
7) Chloroethane-d5	2.893	69	29098	38.184	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	152.720%#
11) 1,1-Dichloroethene-d2	4.021	65	9820	24.514	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	98.040%
21) 2-Butanone-d5	7.088	46	11374m	57.063	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.120%
24) Chloroform-d	7.648	84	46482	25.880	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.520%
26) 1,2-Dichloroethane-d4	8.307	65	26514	30.804	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	123.200%
32) Benzene-d6	8.276	84	88608	23.909	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.640%
36) 1,2-Dichloropropane-d6	9.270	67	29110	26.236	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.960%
41) Toluene-d8	10.325	98	64942	19.858	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.440%
43) trans-1,3-Dichloroprop...	10.575	79	10364	23.802	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.200%
47) 2-Hexanone-d5	10.928	63	2584	15.224	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	30.440%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	24271	28.584	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.320%
66) 1,2-Dichlorobenzene-d4	13.849	152	19053	24.308	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.240%
Target Compounds					Qvalue	
13) Acetone	4.137	43	1814m	7.365	ug/L	
16) Methylene chloride	4.923	84	5510	4.587	ug/L	94
72) 1,2,3-Trichlorobenzene	15.556	180	470	0.656	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100423\
Data File : VW027220.D
Acq On : 04 Oct 2023 16:15
Operator : SY/MD
Sample : 04747-06
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EX841

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/05/2023
Supervised By :Mahesh Dadoda 10/05/2023

Quant Time: Oct 04 22:52:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 22:49:04 2023
Response via : Initial Calibration

