

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
 Data File : VW030388.D
 Acq On : 04 Oct 2024 13:11
 Operator : SY/MD
 Sample : P4237-18
 Misc : 5.33g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 05 01:26:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 05 01:25:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	198450	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	184719	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	80249	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	39546	25.501	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 102.000%			
7) Chloroethane-d5	2.899	69	30594	27.115	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 108.440%			
11) 1,1-Dichloroethene-d2	4.021	65	24498	21.642	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 86.560%			
21) 2-Butanone-d5	7.075	46	22749	36.479	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 72.960%			
24) Chloroform-d	7.654	84	116126	21.782	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 87.120%			
26) 1,2-Dichloroethane-d4	8.307	65	62134	22.328	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 89.320%			
32) Benzene-d6	8.276	84	226830	21.910	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 87.640%			
36) 1,2-Dichloropropane-d6	9.276	67	70733	22.716	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 90.880%			
41) Toluene-d8	10.325	98	203216	21.406	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 85.640%			
43) trans-1,3-Dichloroprop...	10.581	79	25594	19.761	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 79.040%			
47) 2-Hexanone-d5	10.922	63	18656	36.283	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 72.560%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	48130	20.685	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 82.760%			
66) 1,2-Dichlorobenzene-d4	13.848	152	66419	24.929	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 99.720%			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	1980	0.435	ug/L	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
Data File : VW030388.D
Acq On : 04 Oct 2024 13:11
Operator : SY/MD
Sample : P4237-18
Misc : 5.33g/10mL/MSVOA_W/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 05 01:26:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 05 01:25:07 2024
Response via : Initial Calibration

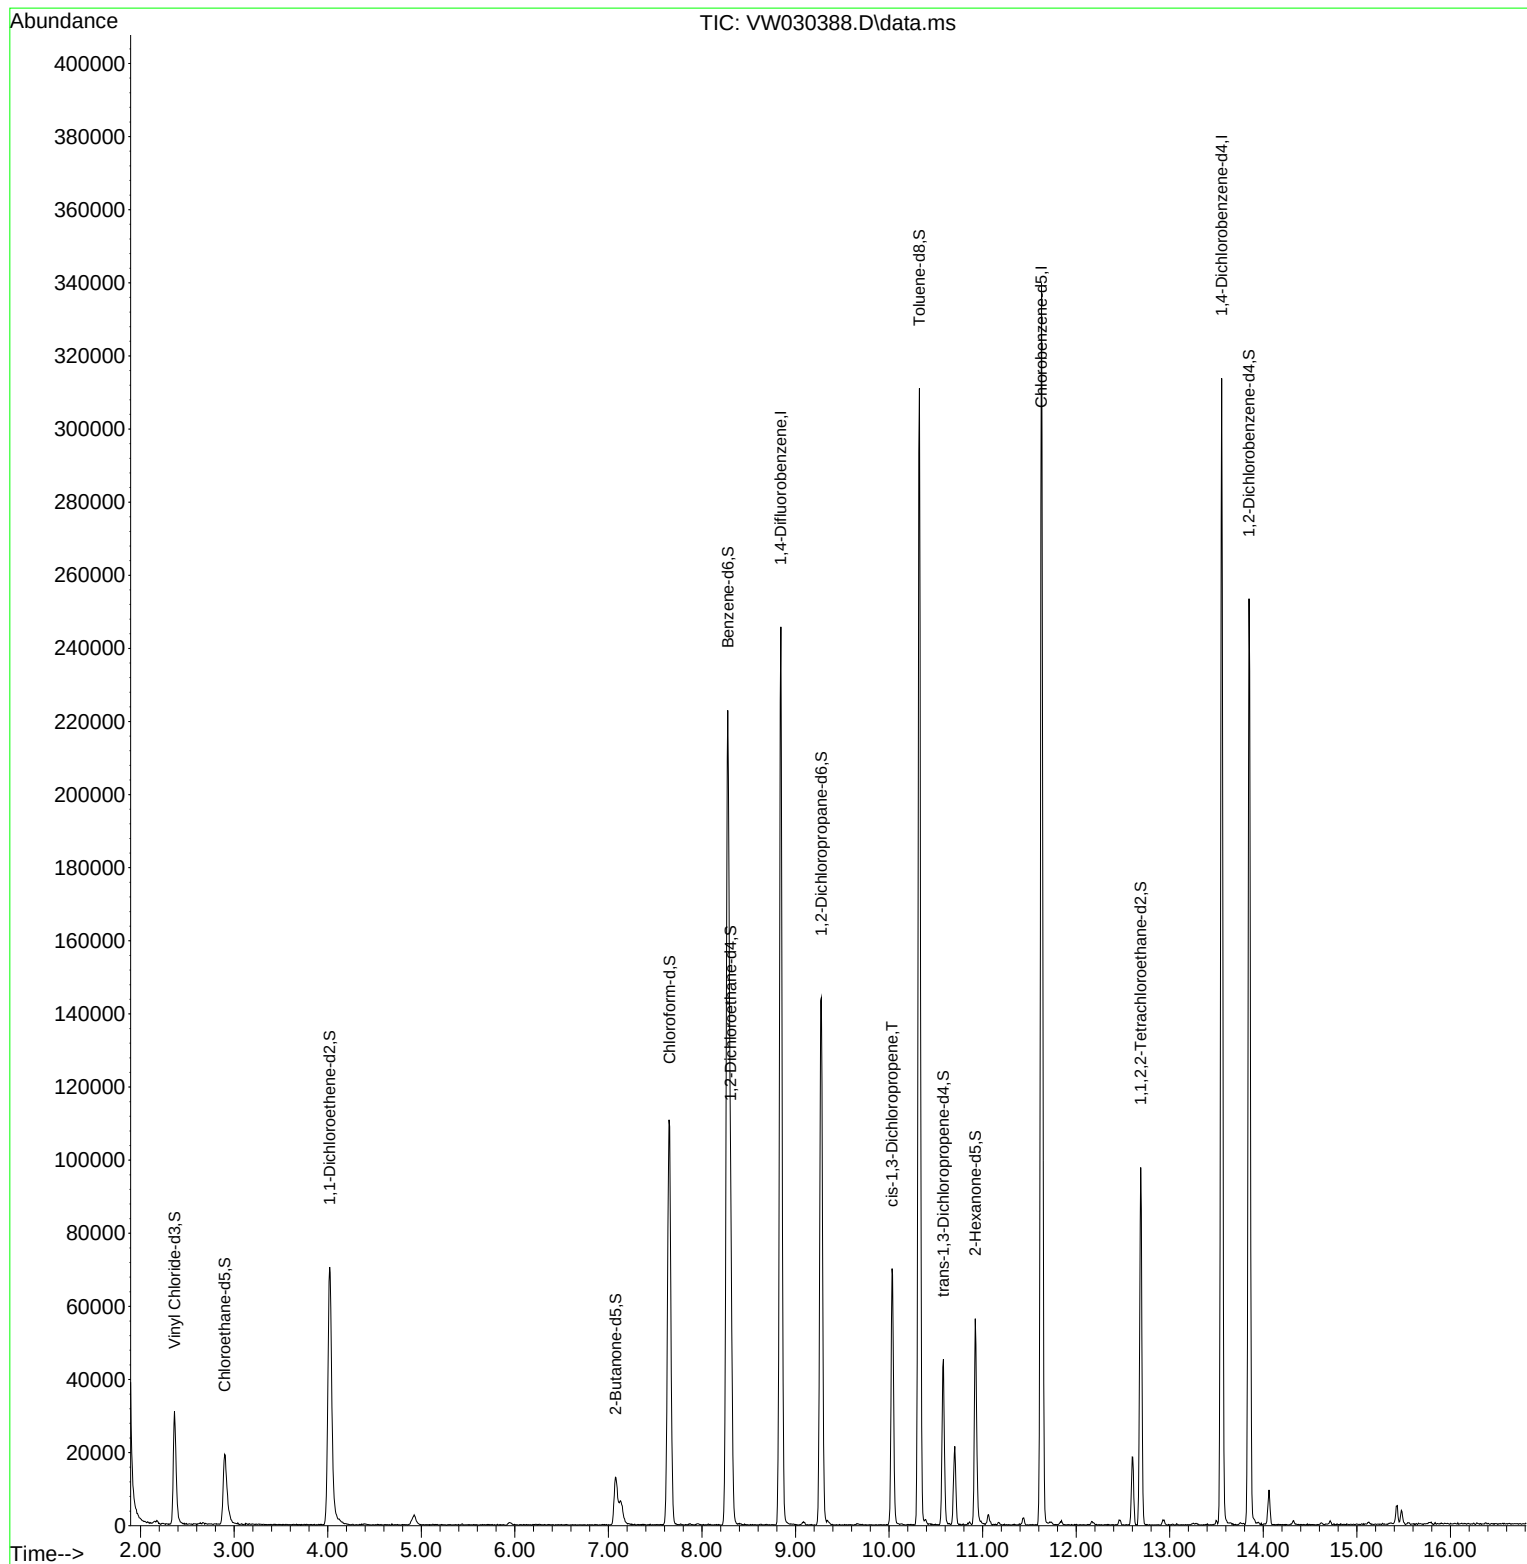

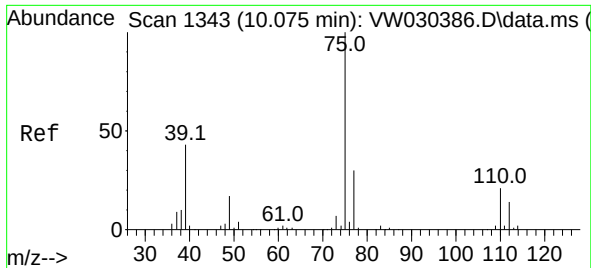

#39
 cis-1,3-Dichloropropene
 Concen: 0.435 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW030388.D
 Acq: 04 Oct 2024 13:11

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 1980
 Ion Ratio Lower Upper
 75 100
 77 41.6 22.0 40.8#

