

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
 Data File : VW030392.D
 Acq On : 04 Oct 2024 14:47
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 05 01:27:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 05 01:25:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	171444	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	165167	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	73939	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	33637	25.108	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.440%
7) Chloroethane-d5	2.905	69	27224	27.929	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.720%
11) 1,1-Dichloroethene-d2	4.027	65	21060	21.535	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.160%
21) 2-Butanone-d5	7.081	46	27427	50.908	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.820%
24) Chloroform-d	7.648	84	103258	22.419	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.680%
26) 1,2-Dichloroethane-d4	8.307	65	59048	24.562	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.240%
32) Benzene-d6	8.276	84	201406	21.757	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.040%
36) 1,2-Dichloropropane-d6	9.276	67	64343	23.110	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.440%
41) Toluene-d8	10.325	98	182153	21.459	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.840%
43) trans-1,3-Dichloroprop...	10.575	79	23698	20.463	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.840%
47) 2-Hexanone-d5	10.922	63	21679	47.153	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.300%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	51183	24.601	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.400%
66) 1,2-Dichlorobenzene-d4	13.849	152	61443	25.029	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.120%
Target Compounds						
					Qvalue	
39) cis-1,3-Dichloropropene	10.032	75	1839	0.452	ug/L #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
Data File : VW030392.D
Acq On : 04 Oct 2024 14:47
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 05 01:27:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 05 01:25:07 2024
Response via : Initial Calibration

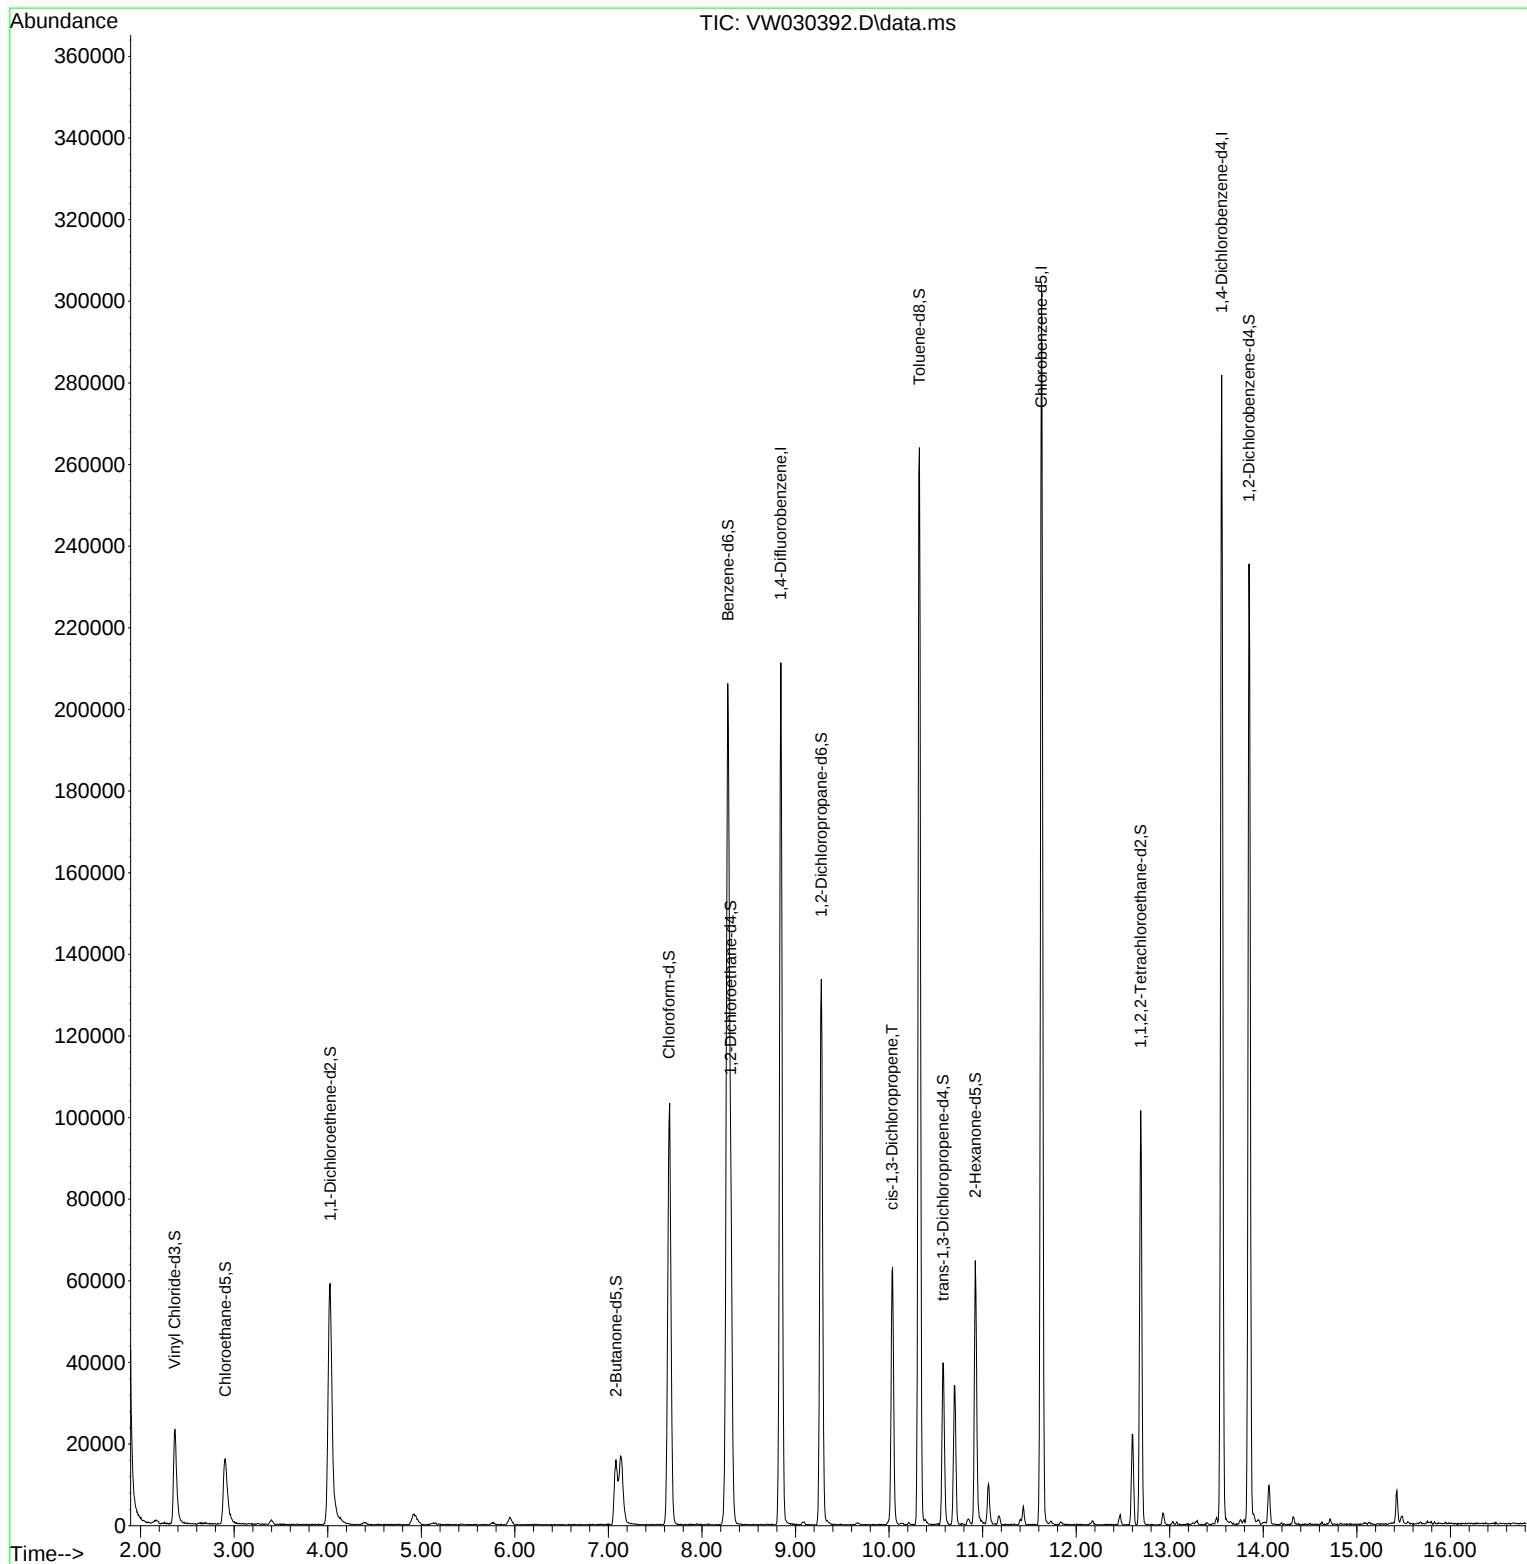

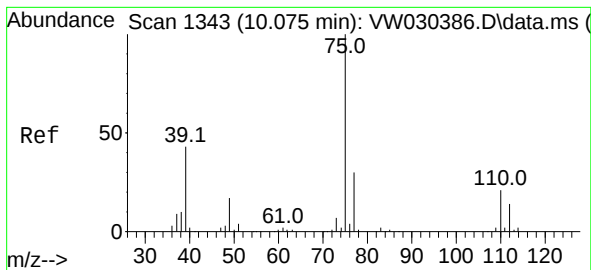

#39
 cis-1,3-Dichloropropene
 Concen: 0.452 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW030392.D
 Acq: 04 Oct 2024 14:47

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 1839
 Ion Ratio Lower Upper
 75 100
 77 46.5 22.0 40.8#

