




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
Data File : VW030400.D
Acq On : 04 Oct 2024 17:59
Operator : SY/MD
Sample : P4239-11 RE
Misc : 5.09g/10mL/MSVOA_W/SOIL/B
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4ET5RE

Manual IntegrationsAPPROVED

Quant Time: Oct 05 01:29:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 05 01:25:07 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/07/2024
Supervised By :Semsettin Yesilyurt 10/07/2024

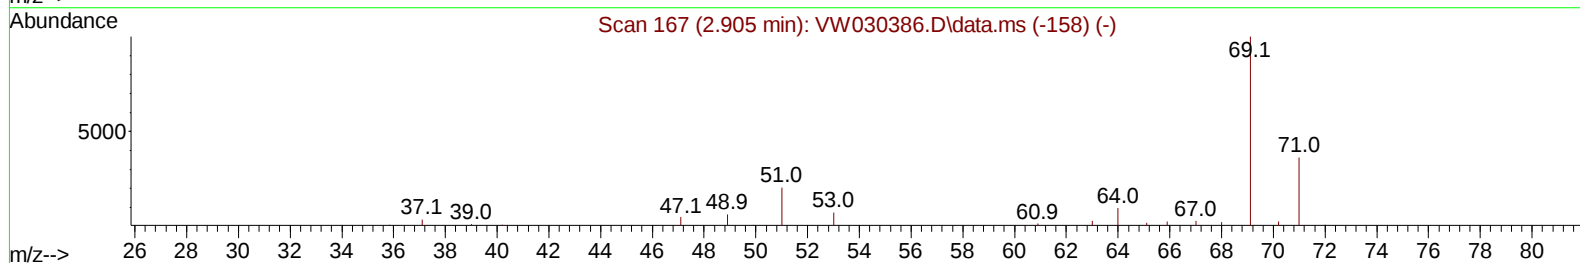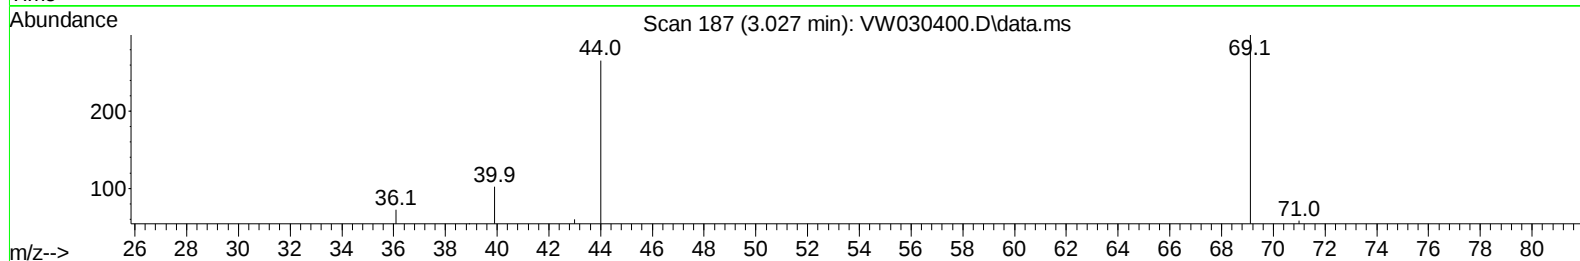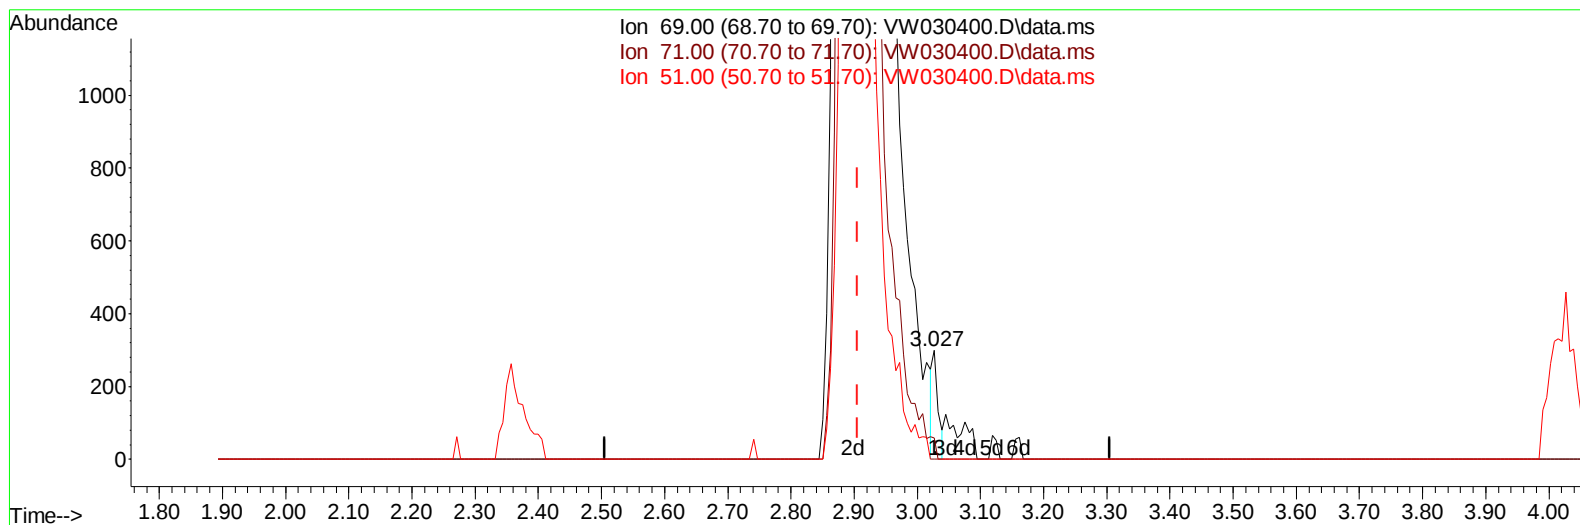

TIC: VW030400.D\data.ms

(7) Chloroethane-d5 (S)

3.027min (+ 0.122) 0.08 ug/L

response 186

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	23.66
51.00	28.00	24.19
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
 Data File : VW030400.D
 Acq On : 04 Oct 2024 17:59
 Operator : SY/MD
 Sample : P4239-11 RE
 Misc : 5.09g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4ET5RE

Manual IntegrationsAPPROVED

Quant Time: Oct 05 01:29:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 05 01:25:07 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/07/2024
 Supervised By :Semsettin Yesilyurt 10/07/2024

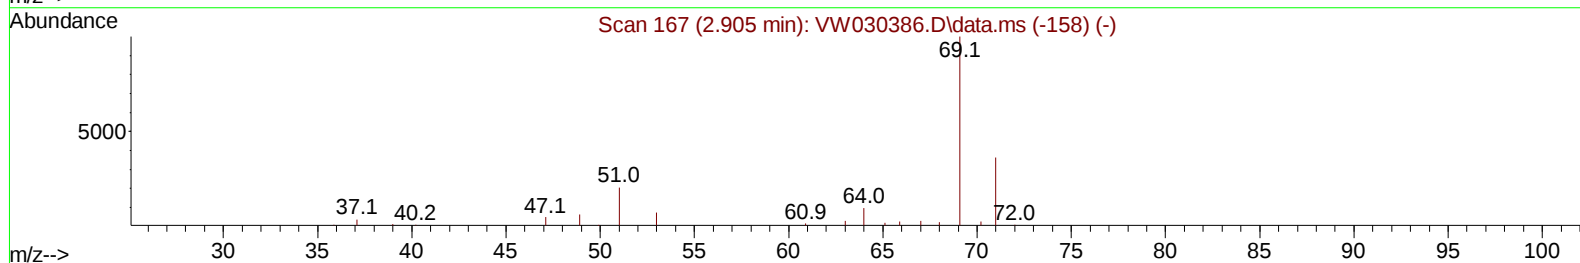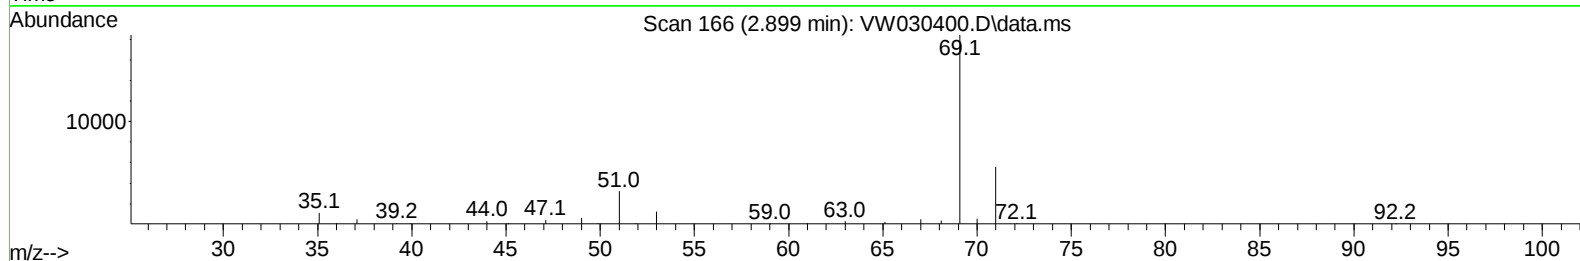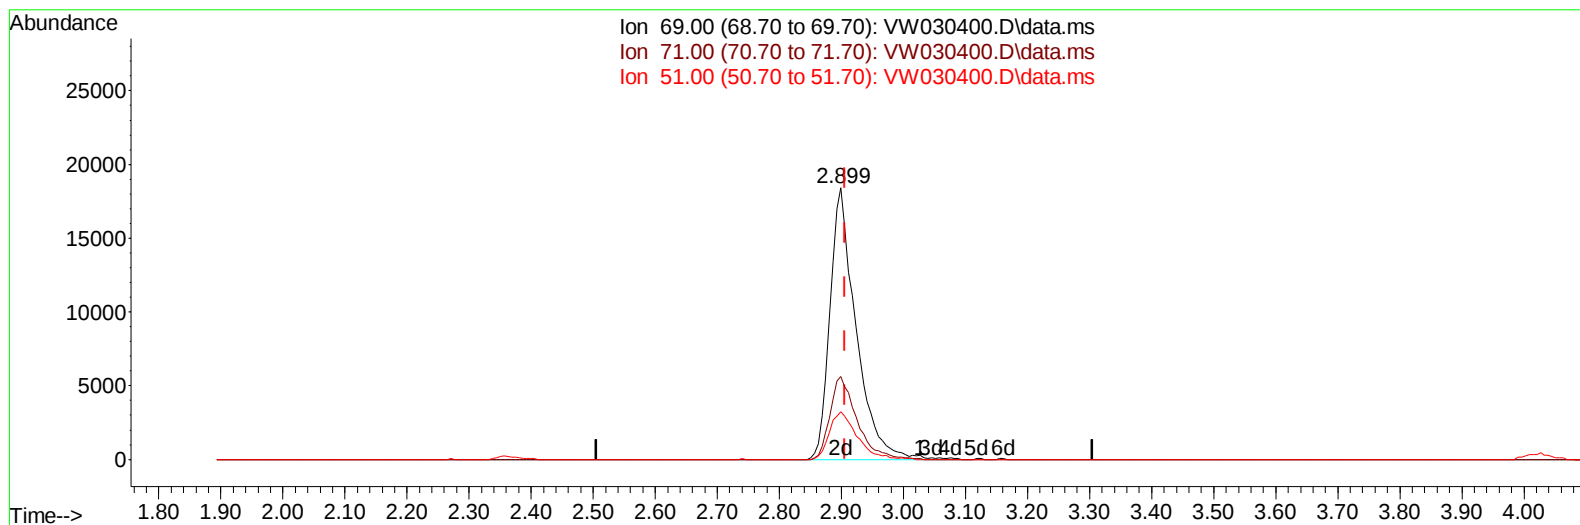

TIC: VW030400.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (-0.006) 22.51 ug/L m

response 53573

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	0.08#
51.00	28.00	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
 Data File : VW030400.D
 Acq On : 04 Oct 2024 17:59
 Operator : SY/MD
 Sample : P4239-11 RE
 Misc : 5.09g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4ET5RE

Manual IntegrationsAPPROVED

Quant Time: Oct 05 01:29:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 05 01:25:07 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/07/2024
 Supervised By :Semsettin Yesilyurt 10/07/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		418643	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		377424	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		162908	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		68539	20.951	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	83.800%		
7) Chloroethane-d5	2.899	69		53573m	22.507	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	90.040%		
11) 1,1-Dichloroethene-d2	4.021	65		42279	17.705	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	70.800%		
21) 2-Butanone-d5	7.081	46		40106	30.485	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	60.980%		
24) Chloroform-d	7.648	84		205309	18.255	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	73.000%		
26) 1,2-Dichloroethane-d4	8.307	65		103728	17.670	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	70.680%		
32) Benzene-d6	8.276	84		399874	18.903	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	75.600%		
36) 1,2-Dichloropropane-d6	9.270	67		124863	19.626	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	78.520%		
41) Toluene-d8	10.325	98		349925	18.040	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	72.160%		
43) trans-1,3-Dichloroprop...	10.581	79		45963	17.369	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	69.480%		
47) 2-Hexanone-d5	10.922	63		32333	30.776	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	61.560%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		84955	17.870	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	71.480%		
66) 1,2-Dichlorobenzene-d4	13.848	152		110958	20.515	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	82.040%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
Data File : VW030400.D
Acq On : 04 Oct 2024 17:59
Operator : SY/MD
Sample : P4239-11 RE
Misc : 5.09g/10mL/MSVOA_W/SOIL/B
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4ET5RE

Manual IntegrationsAPPROVED

Quant Time: Oct 05 01:29:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 05 01:25:07 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/07/2024
Supervised By :Semsettin Yesilyurt 10/07/2024

