

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
 Data File : VW030409.D
 Acq On : 04 Oct 2024 21:35
 Operator : SY/MD
 Sample : P4284-19
 Misc : 4.86g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EZ4

Quant Time: Oct 05 01:31:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 05 01:25:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	293017	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	198904	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	54884	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	60031	26.218	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.880%
7) Chloroethane-d5	2.899	69	47796	28.689	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	114.760%
11) 1,1-Dichloroethene-d2	4.027	65	32217	19.276	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.120%
21) 2-Butanone-d5	7.075	46	26790	29.094	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.180%
24) Chloroform-d	7.648	84	159294	20.236	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.960%
26) 1,2-Dichloroethane-d4	8.307	65	90394	22.000	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.000%
32) Benzene-d6	8.276	84	277275	24.872	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.480%
36) 1,2-Dichloropropane-d6	9.276	67	97605	29.110	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	116.440%
41) Toluene-d8	10.325	98	201018	19.665	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.640%
43) trans-1,3-Dichloroprop...	10.581	79	18159	13.021	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	52.080%
47) 2-Hexanone-d5	10.928	63	11897	21.488	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	42.980%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	61566	24.573	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.280%
66) 1,2-Dichlorobenzene-d4	13.849	152	34801	19.098	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	76.400%
Target Compounds						
13) Acetone	4.125	43	5654	5.788	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
Data File : VW030409.D
Acq On : 04 Oct 2024 21:35
Operator : SY/MD
Sample : P4284-19
Misc : 4.86g/10mL/MSVOA_W/SOIL/A
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EZ4

Quant Time: Oct 05 01:31:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 05 01:25:07 2024
Response via : Initial Calibration

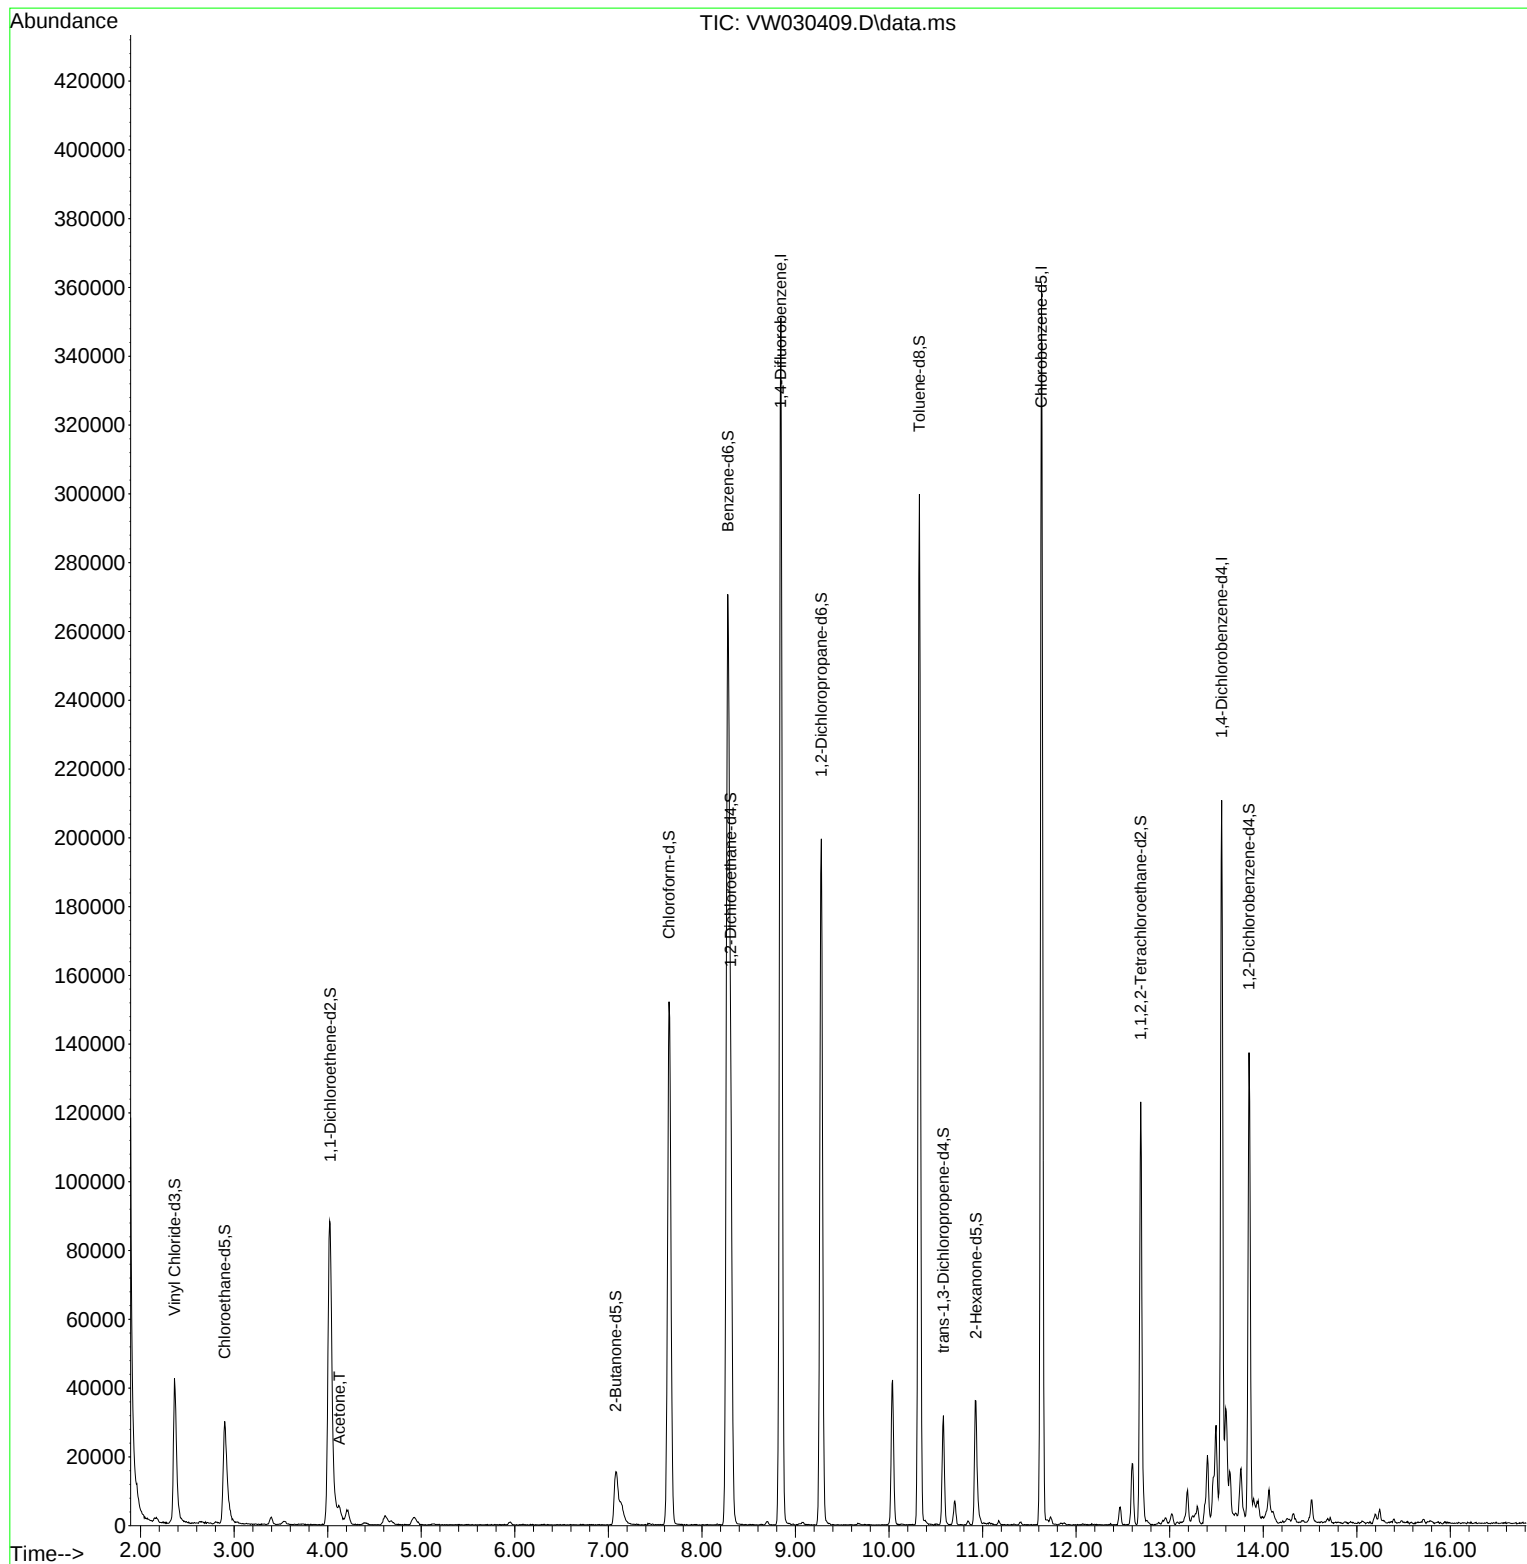

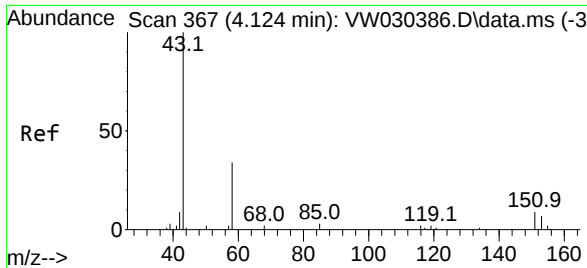

#13
 Acetone
 Concen: 5.788 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW030409.D
 Acq: 04 Oct 2024 21:35

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EZ4

Tgt Ion: 43 Resp: 5654
 Ion Ratio Lower Upper
 43 100
 58 28.6 0.0 64.0

