
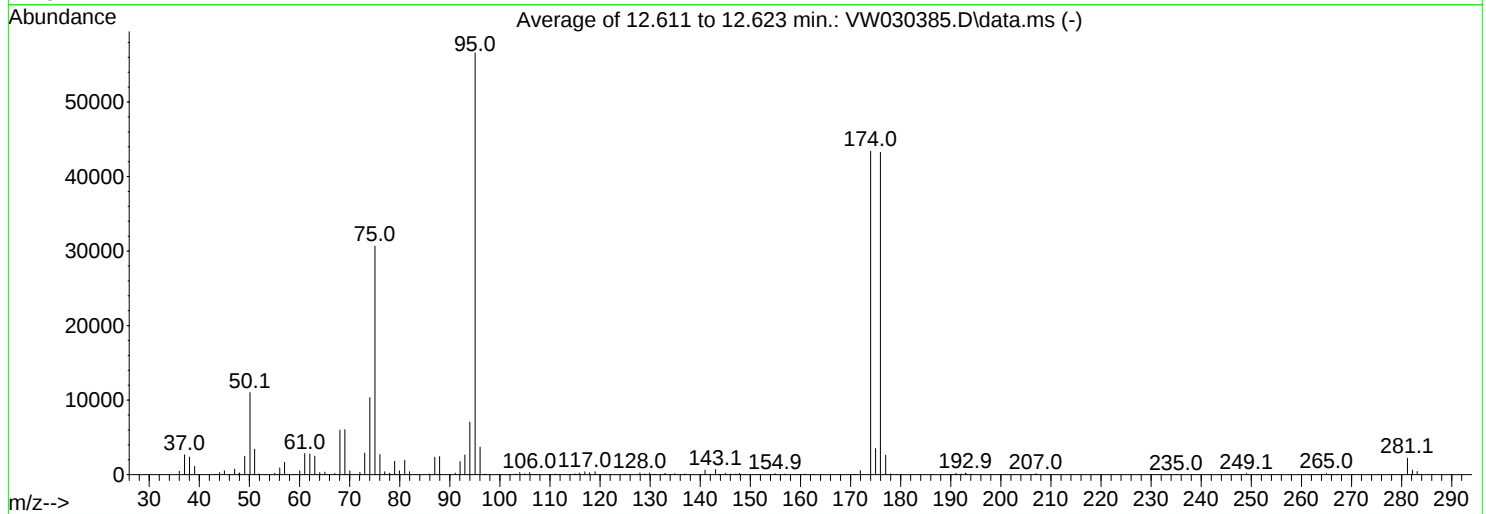


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100424\
Data File : VW030385.D
Acq On : 04 Oct 2024 11:14
Operator : SY/MD
Sample : BFB569
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB569

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Title : SFAM01.0
Last Update : Sat Oct 05 01:25:07 2024

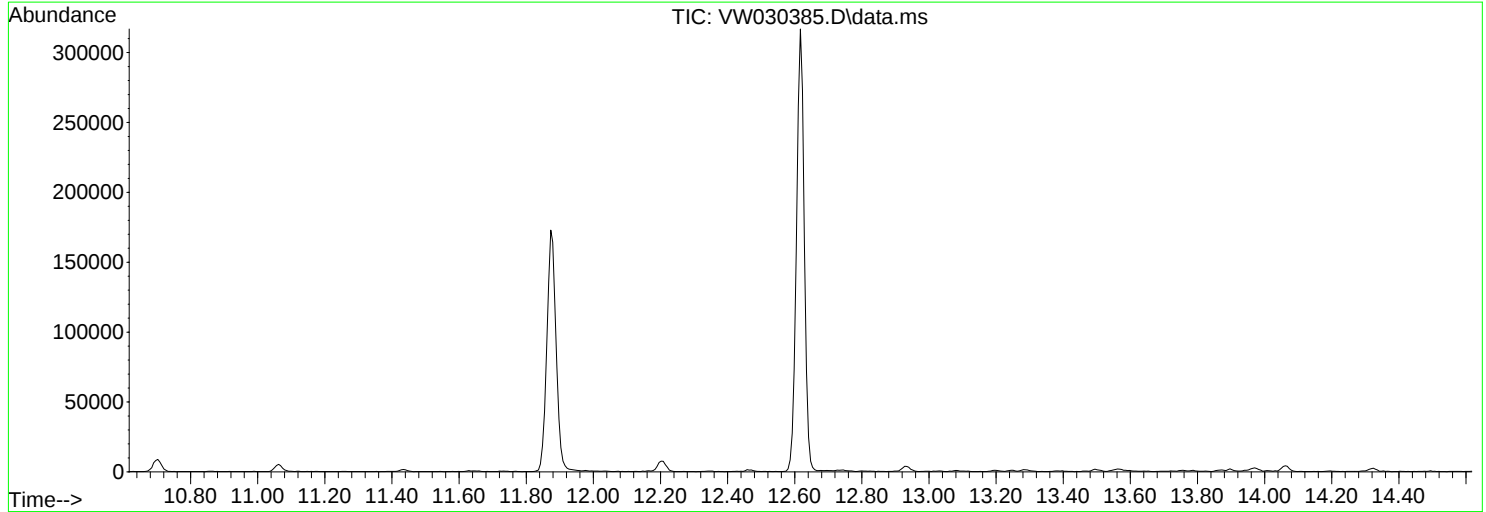

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	11007	PASS
75	95	30	80	54.2	30656	PASS
95	95	100	100	100.0	56600	PASS
96	95	5	9	6.5	3705	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.7	43397	PASS
175	174	5	9	8.0	3491	PASS
176	174	95	101	99.6	43237	PASS
177	176	5	9	6.0	2610	PASS

m/z	Abundance
39.90	137.0
43.90	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB569

m/z	Abundance
36.00	364.0
37.00	2757.0
38.00	2344.0
39.00	1124.0
40.00	91.0
43.90	356.0
45.00	442.0
47.00	762.0
48.00	324.0
49.10	2477.0
50.10	10634.0
51.10	3418.0
51.90	128.0
53.00	53.0
55.00	183.0
56.10	903.0
57.00	1483.0
58.90	80.0
60.00	606.0
61.10	2647.0
62.10	2638.0
63.00	2319.0
64.20	314.0
65.00	391.0
65.90	89.0
67.00	201.0
68.00	5786.0
69.00	5796.0
70.00	560.0
72.10	362.0
73.00	2818.0
74.10	9157.0
75.10	28584.0
76.10	2720.0
77.00	329.0
78.00	353.0
79.00	1780.0
79.90	547.0
81.00	1734.0
82.00	342.0
83.20	83.0
85.90	117.0
87.00	2132.0
88.00	2319.0
91.10	228.0
92.00	1788.0
93.00	2548.0
94.00	6069.0
95.00	53472.0
96.10	3784.0
97.00	62.0
103.10	84.0
104.00	247.0
105.00	125.0
105.90	249.0
107.00	80.0
111.10	68.0
113.00	53.0
115.00	102.0
115.80	230.0
116.90	334.0
117.80	238.0
119.00	379.0
125.10	96.0
128.00	232.0
129.10	61.0
129.80	207.0
131.00	102.0
132.90	377.0
134.00	67.0
135.00	130.0
136.90	94.0
141.00	432.0
142.00	74.0
143.10	642.0
145.00	206.0
146.10	66.0
147.10	115.0
147.80	108.0
149.10	53.0
154.90	140.0
156.80	57.0
157.20	66.0
161.00	62.0
162.80	61.0
170.80	90.0
172.00	595.0
174.00	36800.0
175.00	2818.0
175.90	34896.0
177.00	2268.0
178.00	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB569

179.10	146.0
191.00	344.0
192.10	129.0
192.90	298.0
193.20	297.0
194.10	94.0
207.00	275.0
235.00	53.0
249.00	311.0
251.00	76.0
265.00	277.0
266.20	66.0
267.00	96.0
281.10	3628.0
282.20	978.0
283.10	591.0
284.00	175.0

Instrument :
MSVOA_W
ClientSampleId :
BFB569

m/z	Abundance
36.00	535.0
37.10	3055.0
38.00	2679.0
39.00	1273.0
40.00	110.0
43.10	81.0
44.10	387.0
45.00	642.0
46.10	80.0
47.10	719.0
48.10	397.0
49.00	2801.0
50.10	12399.0
51.10	3513.0
51.90	166.0
55.10	266.0
56.00	886.0
57.00	1732.0
58.00	56.0
60.10	533.0
61.00	3234.0
62.00	3191.0
63.10	2785.0
64.00	349.0
65.10	388.0
67.10	180.0
68.10	6806.0
69.00	6776.0
70.00	534.0
72.00	327.0
73.00	3240.0
74.00	11605.0
75.00	34360.0
76.10	3061.0
77.00	399.0
77.90	235.0
79.00	1977.0
80.00	541.0
81.00	2113.0
82.00	417.0
83.00	72.0
85.90	85.0
87.00	2717.0
88.00	2650.0
91.10	205.0
92.00	1875.0
93.00	2796.0
94.00	7944.0
95.00	63128.0
96.00	3752.0
97.00	118.0
103.10	89.0
103.90	296.0
105.00	97.0
105.90	339.0
109.80	58.0
111.00	138.0
115.00	154.0
115.90	236.0
116.90	508.0
117.90	237.0
119.00	367.0
125.00	106.0
127.90	249.0
128.90	129.0
129.90	236.0
130.90	116.0
133.10	193.0
134.80	150.0
137.00	140.0
141.00	692.0
142.00	115.0
143.00	769.0
143.80	53.0
145.00	163.0
146.00	112.0
147.10	72.0
147.90	203.0
149.00	52.0
155.00	190.0
156.80	134.0
160.90	117.0
171.90	521.0
174.00	49824.0
175.00	3808.0
176.00	49312.0
177.00	2722.0
177.90	153.0
191.10	162.0
192.10	57.0
193.00	253.0
194.00	79.0

Instrument :
MSVOA_W
ClientSampleId :
BFB569

207.00	157.0
249.10	104.0
265.00	175.0
267.10	63.0
281.20	1801.0
282.10	583.0
283.10	419.0

Instrument :
MSVOA_W
ClientSampleId :
BFB569

m/z	Abundance
36.00	443.0
37.00	2207.0
38.10	2036.0
39.10	958.0
40.00	147.0
43.10	67.0
44.00	425.0
45.00	446.0
46.10	55.0
47.10	793.0
47.80	271.0
49.10	2115.0
50.10	9988.0
51.00	3284.0
52.10	166.0
55.10	151.0
56.10	911.0
57.00	1716.0
58.00	86.0
60.00	434.0
61.00	2640.0
62.00	2471.0
63.10	2397.0
63.90	192.0
65.00	257.0
67.10	161.0
68.10	5347.0
69.10	5529.0
70.10	472.0
72.00	300.0
73.00	2647.0
74.00	10207.0
75.10	29024.0
76.00	2329.0
77.00	457.0
78.20	220.0
79.00	1622.0
80.00	458.0
81.00	1978.0
81.90	397.0
85.90	52.0
87.00	2162.0
87.90	2310.0
91.10	224.0
92.10	1621.0
93.00	2555.0
94.00	7097.0
95.10	53200.0
96.10	3580.0
97.20	120.0
103.00	66.0
104.00	266.0
105.00	82.0
106.00	225.0
111.00	72.0
111.80	54.0
114.90	84.0
115.90	174.0
117.00	342.0
118.00	247.0
119.00	397.0
127.90	210.0
128.90	114.0
129.90	224.0
133.10	133.0
134.90	131.0
137.00	119.0
140.90	747.0
142.00	60.0
143.00	641.0
143.80	71.0
145.00	209.0
146.20	57.0
147.10	71.0
147.80	187.0
154.90	129.0
157.00	149.0
158.90	103.0
160.80	101.0
171.00	82.0
172.00	517.0
174.00	43568.0
175.00	3847.0
176.00	45504.0
177.00	2840.0
177.90	83.0
191.00	71.0
193.00	100.0
249.10	88.0
264.90	70.0
281.10	1238.0
282.10	266.0

Instrument :
MSVOA_W
ClientSampleId :
BFB569

283.00

293.0

Instrument :
MSVOA_W
ClientSampleId :
BFB569