

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100518\
 Data File : VW005861.D
 Acq On : 04 Oct 2018 17:45
 Operator : SY/AP
 Sample : J5251-04
 Misc : 4.09G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H2TS4

Manual Integrations
 APPROVED

MMDadoda
 10/5/2018 12:28:50 PM

Quant Time: Oct 05 03:49:06 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 05 01:16:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	286645	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	293350	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	134948	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	43970	12.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	48.12%
7) Chloroethane-d5	2.90	69	38501	13.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.00%
10) 1,1-Dichloroethene-d2	4.01	63	78662	9.86	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	39.44%#
20) 2-Butanone-d5	7.08	46	44606	38.02	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.04%
24) Chloroform-d	7.65	84	134640	18.28	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.12%
26) 1,2-Dichloroethane-d4	8.31	65	83510	18.72	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	74.88%
29) Benzene-d6	8.28	84	226467	15.59	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	62.36%
33) 1,2-Dichloropropane-d6	9.28	67	70961	16.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	67.64%#
37) Toluene-d8	10.33	98	222349	15.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	62.04%
38) trans-1,3-Dichloropropene-	10.58	79	37042	16.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.20%
39) 2-Hexanone-d5	10.93	63	33706	34.29	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.58%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	80089	19.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	78.56%
61) 1,2-Dichlorobenzene-d4	13.86	152	87140	18.25	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	73.00%#

Target Compounds					Ovalue
13) Acetone	4.12	43	3357	2.748 ug/L	89
16) Methylene chloride	4.92	84	9406m	1.990 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW100518\
Data File : VW005861.D
Acq On : 04 Oct 2018 17:45
Operator : SY/AP
Sample : J5251-04
Misc : 4.09G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
H2TS4

Manual Integrations
APPROVED

MMDadoda
10/5/2018 12:28:50 PM

Quant Time: Oct 05 03:49:06 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 05 01:16:24 2018
Response via : Initial Calibration

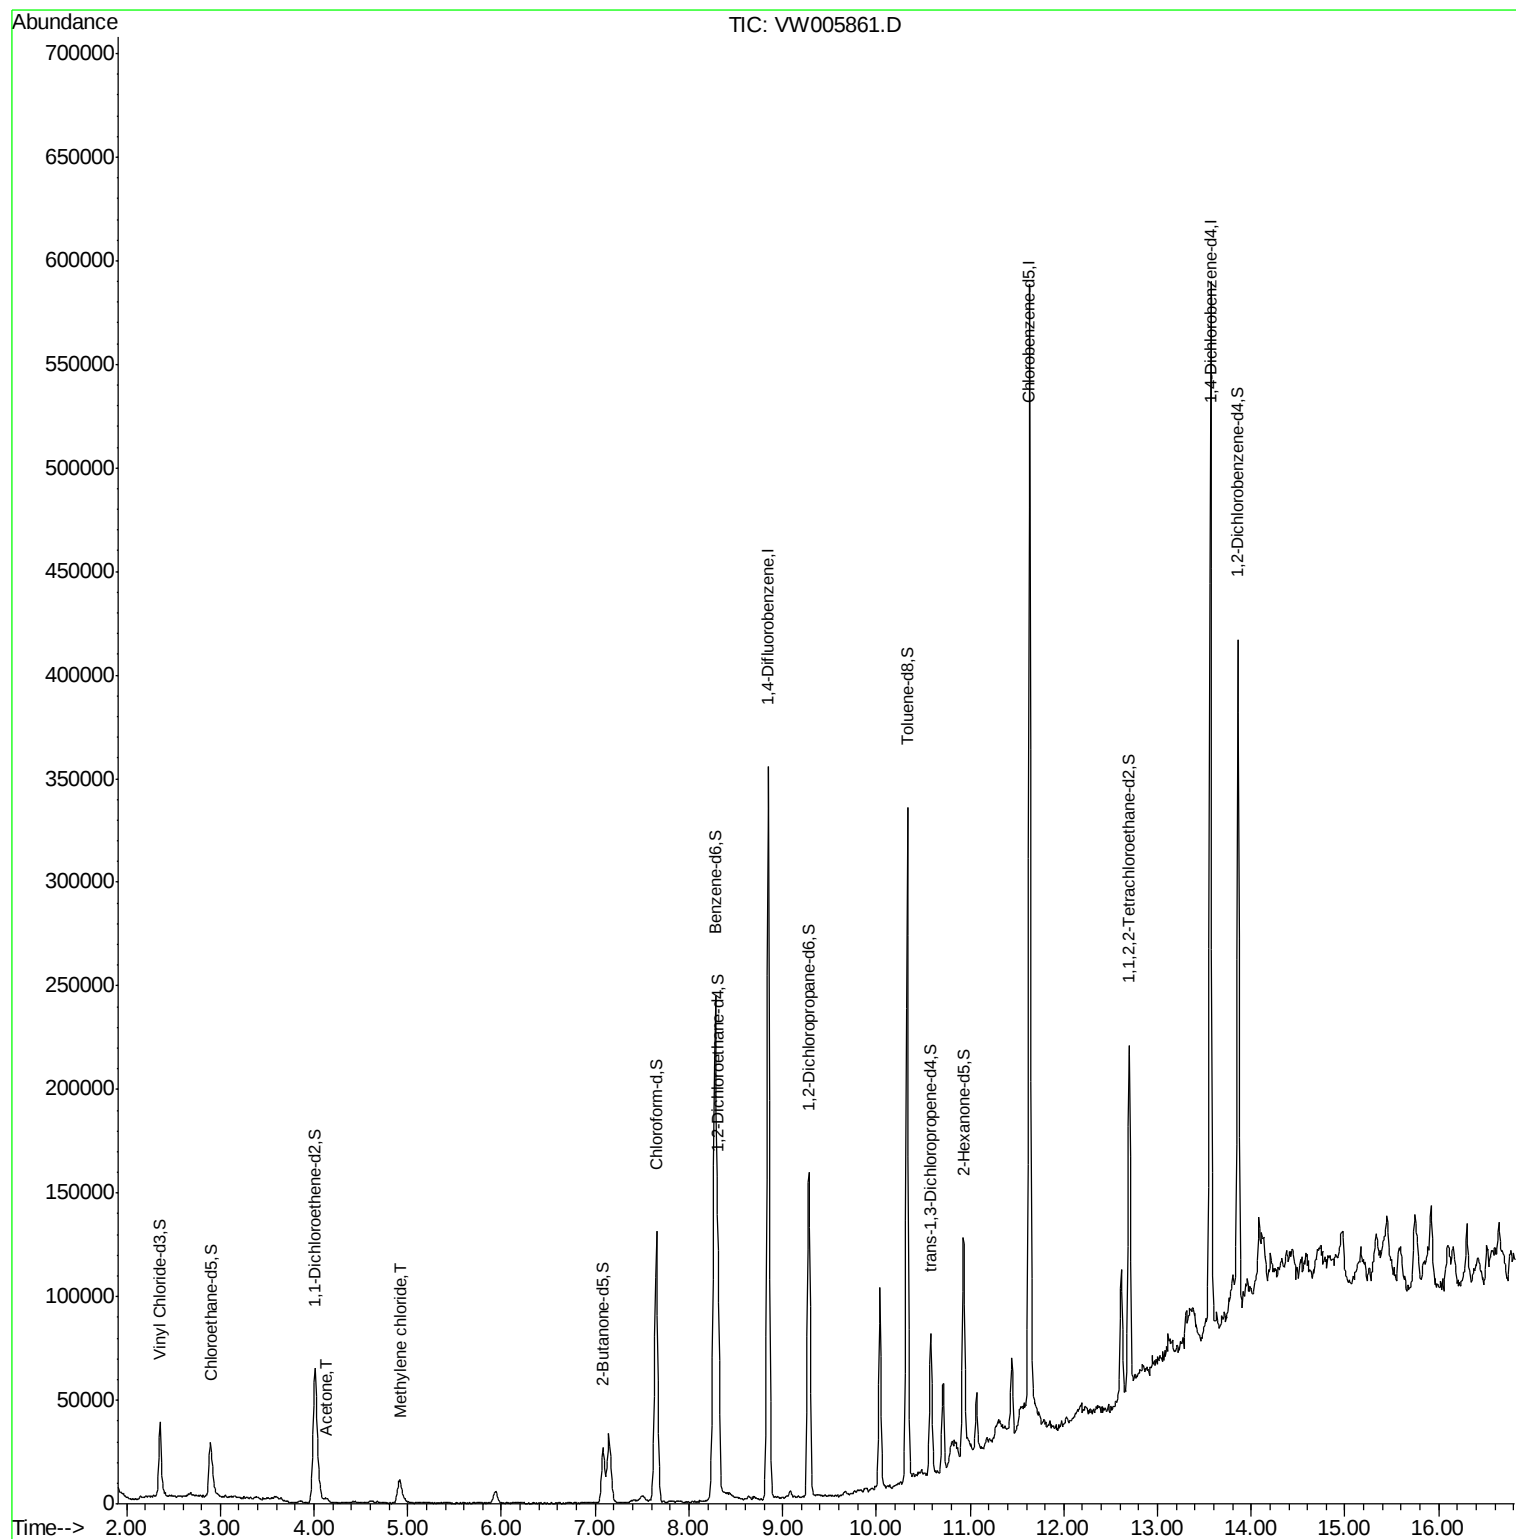

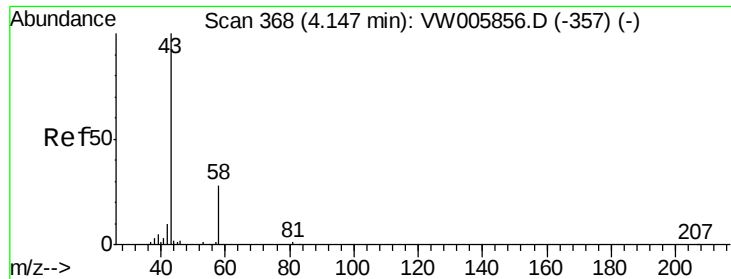





#13
Acetone
Concen: 2.748 ug/L
RT: 4.12 min Scan# 364
Delta R.T. -0.02 min
Lab File: VW005861.D
Acq: 04 Oct 2018 17:45

Instrument :
MSVOA_W
ClientSampleId :
H2TS4

Tot Ion	Ratio	Lower	Upper
43	100		
58	20.5	0.0	31.8

Manual Integrations
APPROVED

MMDadoda
10/5/2018 12:28:50 PM

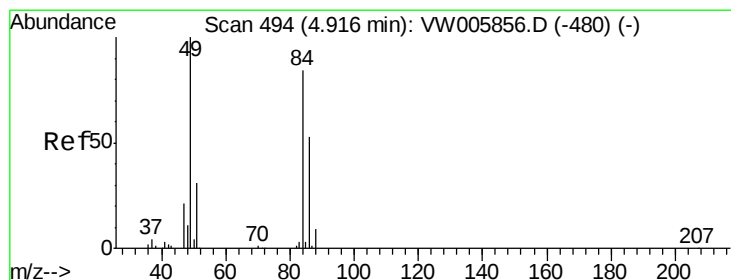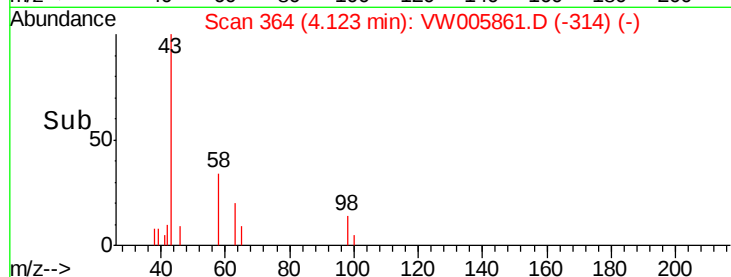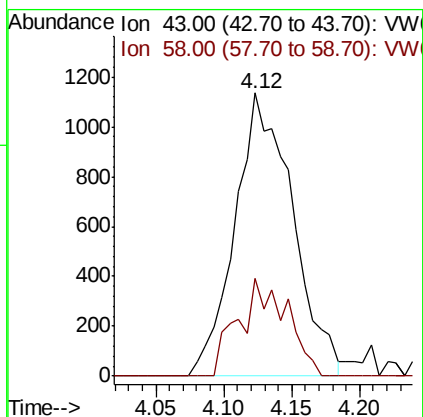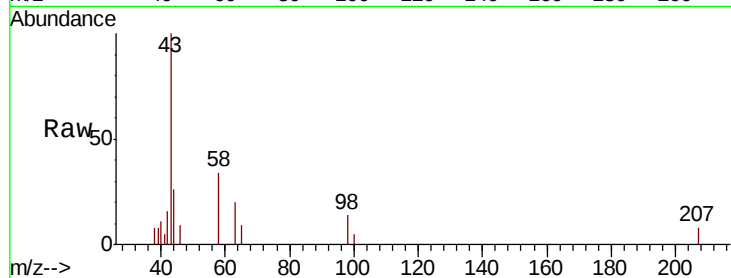

#16
Methylene chloride
Concen: 1.990 ug/L m
RT: 4.92 min Scan# 494
Delta R.T. -0.00 min
Lab File: VW005861.D
Acq: 04 Oct 2018 17:45

Tgt Ion	Ratio	Lower	Upper
84	100		
49	117.1	87.2	162.0
86	53.9	43.2	80.2

