


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW100518\
 Data File : VW005855.D
 Acq On : 04 Oct 2018 14:21
 Operator : SY/AP
 Sample : BFB89
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB89

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
 Title : VOC Analysis
 Last Update : Fri Oct 05 01:16:24 2018

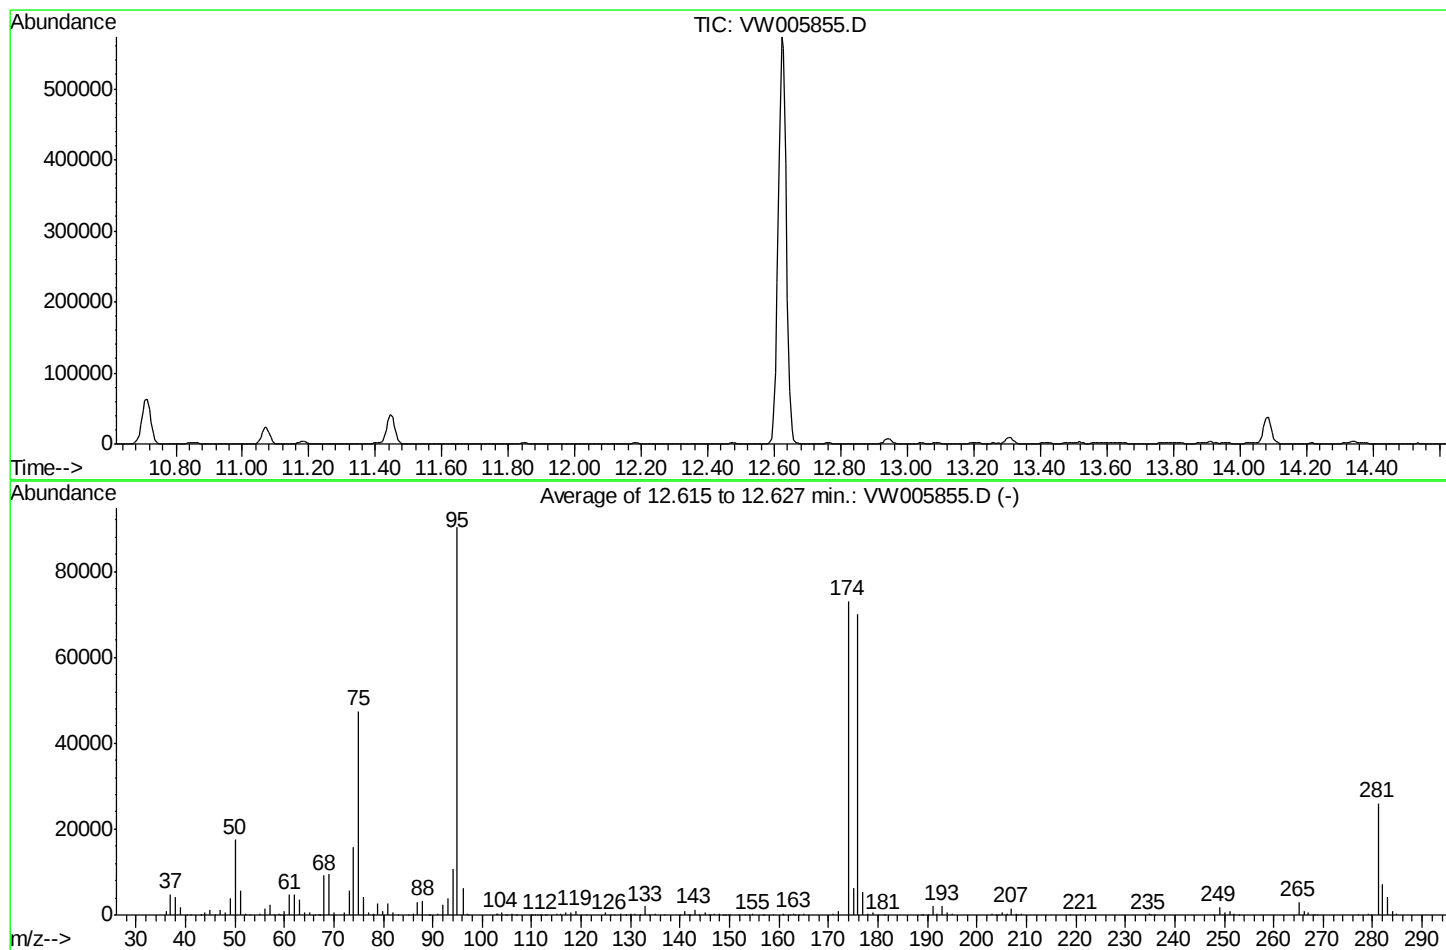

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	17563	PASS
75	95	30	80	52.7	47514	PASS
95	95	100	100	100.0	90242	PASS
96	95	5	9	6.8	6168	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.9	73005	PASS
175	174	5	9	8.6	6247	PASS
176	174	95	101	96.0	70053	PASS
177	176	5	9	7.9	5516	PASS

Scan 1750 (12.573 min): VW005855.D
BFB89

m/z	Abundance
40.00	110.0
44.00	156.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

m/z	Abundance
36.00	833.0
37.00	4028.0
38.00	3533.0
39.00	1460.0
40.20	177.0
41.10	57.0
43.00	170.0
44.00	668.0
45.00	909.0
45.90	143.0
47.00	1141.0
48.00	612.0
49.10	3088.0
50.00	13730.0
51.00	4418.0
52.00	266.0
53.10	66.0
55.00	354.0
56.00	1275.0
57.00	2099.0
57.90	124.0
59.00	478.0
60.00	888.0
61.00	3847.0
62.00	3955.0
63.00	3225.0
64.00	494.0
65.10	568.0
66.80	156.0
68.00	7297.0
69.00	7655.0
69.90	516.0
72.00	416.0
73.00	5185.0
74.00	12747.0
75.00	37568.0
76.00	3206.0
77.20	535.0
77.70	351.0
78.90	2281.0
79.90	633.0
80.90	2398.0
81.90	476.0
85.10	83.0
85.90	137.0
86.90	2593.0
88.00	2433.0
89.10	103.0
91.00	333.0
92.10	1953.0
93.00	2770.0
94.00	8436.0
95.00	70280.0
96.00	5367.0
97.00	246.0
103.10	402.0
103.80	625.0
104.80	234.0
105.90	319.0
106.90	85.0
109.90	222.0
110.80	256.0
111.80	208.0
112.60	61.0
115.10	174.0
115.80	290.0
116.90	503.0
118.00	493.0
118.90	1098.0
119.90	71.0
120.90	58.0
125.00	863.0
126.80	99.0
127.90	291.0
128.90	128.0
130.00	250.0
130.90	176.0
133.00	2204.0
134.80	330.0
137.00	76.0
139.80	55.0
141.00	707.0
142.10	94.0
142.90	982.0
143.90	136.0
144.90	618.0
145.80	76.0
146.20	75.0
146.90	400.0
148.00	283.0
149.00	144.0
150.00	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

153.00	67.0
154.80	216.0
158.90	67.0
160.80	313.0
161.00	314.0
163.00	519.0
164.00	170.0
165.00	464.0
170.90	193.0
172.00	672.0
174.00	51280.0
175.00	4943.0
176.00	49904.0
177.00	4143.0
178.00	376.0
178.90	727.0
180.00	105.0
181.20	113.0
188.90	231.0
190.00	82.0
191.00	2244.0
192.00	439.0
193.00	2513.0
193.90	565.0
194.90	307.0
203.00	469.0
203.90	93.0
205.00	726.0
205.90	203.0
206.30	253.0
207.00	1765.0
208.00	337.0
209.20	228.0
219.00	68.0
221.00	200.0
234.90	326.0
235.90	82.0
247.80	81.0
249.00	2093.0
250.00	663.0
251.00	946.0
252.10	215.0
252.90	107.0
265.00	3529.0
266.10	1024.0
267.00	844.0
268.20	224.0
268.80	72.0
277.00	107.0
279.20	307.0
281.10	27376.0
282.00	7943.0
283.10	4304.0
284.10	974.0
284.80	335.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

m/z	Abundance
36.10	974.0
37.00	5383.0
38.00	4927.0
39.00	2039.0
40.20	109.0
43.20	230.0
44.10	517.0
45.00	1211.0
46.00	183.0
47.10	1323.0
48.10	748.0
49.10	4334.0
50.00	19384.0
51.10	6008.0
52.10	286.0
53.00	109.0
55.00	293.0
56.00	1562.0
57.10	2620.0
57.90	157.0
59.20	383.0
59.90	1073.0
61.00	5377.0
62.00	5364.0
63.00	3972.0
64.00	789.0
65.00	638.0
67.10	265.0
68.00	10585.0
69.00	10912.0
70.00	852.0
71.90	626.0
73.10	6801.0
74.00	17432.0
75.00	53144.0
76.00	4823.0
77.00	446.0
78.10	436.0
79.00	2870.0
79.90	855.0
80.90	3149.0
81.90	761.0
83.10	108.0
85.00	63.0
86.00	233.0
86.90	3586.0
87.90	3772.0
89.30	119.0
90.80	390.0
92.00	2623.0
93.00	4630.0
94.00	12264.0
95.00	100840.0
96.00	6854.0
97.00	319.0
102.80	415.0
103.20	374.0
103.90	596.0
105.00	253.0
106.00	372.0
106.90	161.0
109.70	133.0
110.20	200.0
111.10	250.0
112.00	187.0
112.90	122.0
115.10	215.0
115.90	292.0
116.90	791.0
117.90	697.0
118.90	889.0
119.80	113.0
121.00	186.0
124.90	652.0
125.90	332.0
127.90	401.0
129.10	208.0
129.90	441.0
131.00	184.0
132.00	109.0
133.00	2323.0
134.90	369.0
136.80	148.0
141.00	994.0
141.80	128.0
142.90	1395.0
143.90	94.0
144.90	728.0
145.80	230.0
146.80	321.0
147.80	344.0
148.70	167.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

149.20	122.0
149.60	112.0
151.90	52.0
153.10	103.0
153.80	118.0
154.80	274.0
157.00	224.0
158.70	106.0
158.90	106.0
160.90	304.0
162.10	89.0
162.90	351.0
164.00	115.0
164.90	331.0
170.90	336.0
172.10	986.0
174.00	81280.0
175.00	6664.0
175.90	76592.0
177.00	5779.0
177.90	319.0
179.00	623.0
179.90	136.0
181.20	71.0
189.20	228.0
191.10	2126.0
192.00	488.0
193.00	2142.0
194.00	404.0
195.00	209.0
202.90	292.0
204.30	73.0
205.00	593.0
206.10	285.0
207.00	1667.0
208.20	323.0
209.00	203.0
218.80	90.0
220.80	106.0
235.10	330.0
235.90	94.0
249.10	1942.0
250.10	658.0
251.10	942.0
252.00	315.0
253.00	114.0
265.10	3524.0
266.10	1080.0
267.10	919.0
267.90	269.0
268.90	67.0
279.00	239.0
281.10	28240.0
282.10	7958.0
283.10	4828.0
284.00	1074.0
284.90	459.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

m/z	Abundance
36.10	801.0
37.00	5163.0
38.00	4346.0
39.10	1849.0
39.90	136.0
40.90	58.0
43.00	181.0
44.10	749.0
45.00	1081.0
46.10	93.0
47.00	961.0
47.90	825.0
49.00	3951.0
50.00	19576.0
51.00	6160.0
52.10	235.0
53.00	118.0
54.90	418.0
56.00	1421.0
57.00	2308.0
57.90	92.0
59.00	228.0
60.10	1160.0
61.00	4922.0
62.00	4902.0
63.10	3559.0
64.00	664.0
65.10	489.0
66.20	132.0
66.90	282.0
68.00	9558.0
69.00	10382.0
69.90	714.0
72.10	731.0
73.00	5367.0
74.00	17320.0
75.00	51832.0
76.00	4566.0
77.00	696.0
77.90	316.0
78.90	2680.0
80.00	908.0
80.90	2752.0
81.90	578.0
83.00	91.0
85.90	190.0
87.00	3192.0
88.00	3713.0
89.40	54.0
91.00	411.0
92.10	3007.0
93.00	4681.0
94.10	11888.0
95.00	99608.0
96.10	6285.0
97.20	225.0
102.90	373.0
103.90	410.0
104.70	193.0
105.90	485.0
107.10	60.0
110.00	254.0
110.70	94.0
111.10	130.0
111.80	232.0
112.90	95.0
115.00	233.0
116.00	423.0
116.90	912.0
118.00	487.0
118.90	808.0
119.80	77.0
124.90	548.0
127.90	365.0
129.00	137.0
129.90	341.0
130.80	237.0
131.90	57.0
133.10	1348.0
133.80	390.0
134.80	337.0
136.80	187.0
140.90	899.0
142.00	122.0
143.00	1283.0
144.00	67.0
145.00	479.0
146.00	181.0
147.00	234.0
148.00	242.0
148.90	224.0
149.90	136.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89

153.10	130.0
153.90	99.0
154.70	281.0
156.70	229.0
157.10	204.0
158.90	200.0
161.00	326.0
162.10	87.0
162.80	165.0
163.20	162.0
163.90	64.0
165.00	183.0
170.90	280.0
171.90	730.0
174.00	86456.0
175.00	7134.0
176.00	83664.0
177.00	6627.0
177.90	250.0
179.00	454.0
180.10	93.0
189.10	152.0
191.00	1616.0
192.00	343.0
192.90	1749.0
194.00	455.0
195.00	213.0
202.90	185.0
205.10	395.0
206.10	133.0
207.00	1356.0
208.00	325.0
209.10	152.0
221.10	80.0
234.80	227.0
235.90	77.0
249.00	1485.0
250.00	411.0
251.00	653.0
252.00	200.0
252.80	60.0
265.00	2231.0
266.00	647.0
267.10	486.0
268.00	209.0
268.90	66.0
278.90	133.0
279.50	180.0
281.10	22376.0
282.10	5827.0
283.00	3458.0
284.20	649.0
285.00	212.0

Instrument :
MSVOA_W
ClientSampleId :
BFB89