

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100522\
 Data File : VW024737.D
 Acq On : 05 Oct 2022 15:35
 Operator : SY/VA
 Sample : N4991-08
 Misc : 4.15g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COBG0

Quant Time: Oct 06 01:39:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 06 01:37:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	222709	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	196147	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	73909	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	33447	14.354	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.400%
7) Chloroethane-d5	2.892	69	24346	17.980	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.920%
11) 1,1-Dichloroethene-d2	4.019	63	57129	10.593	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	42.360%#
21) 2-Butanone-d5	7.080	46	70635	84.316	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	168.640%#
24) Chloroform-d	7.653	84	136177	22.872	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.480%
26) 1,2-Dichloroethane-d4	8.305	65	79909	25.872	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.480%
32) Benzene-d6	8.275	84	197215	15.731	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	62.920%
36) 1,2-Dichloropropane-d6	9.275	67	86922	22.692	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.760%
41) Toluene-d8	10.323	98	139121	12.416	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	49.680%
43) trans-1,3-Dichloroprop...	10.579	79	27831	16.315	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.280%
47) 2-Hexanone-d5	10.927	63	45339	69.179	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	138.360%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	96895	35.501	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	142.000%#
66) 1,2-Dichlorobenzene-d4	13.853	152	49034	18.854	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.400%
Target Compounds					Qvalue	
13) Acetone	4.147	43	2966	4.853	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100522\
Data File : VW024737.D
Acq On : 05 Oct 2022 15:35
Operator : SY/VA
Sample : N4991-08
Misc : 4.15g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BG0

Quant Time: Oct 06 01:39:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 06 01:37:00 2022
Response via : Initial Calibration

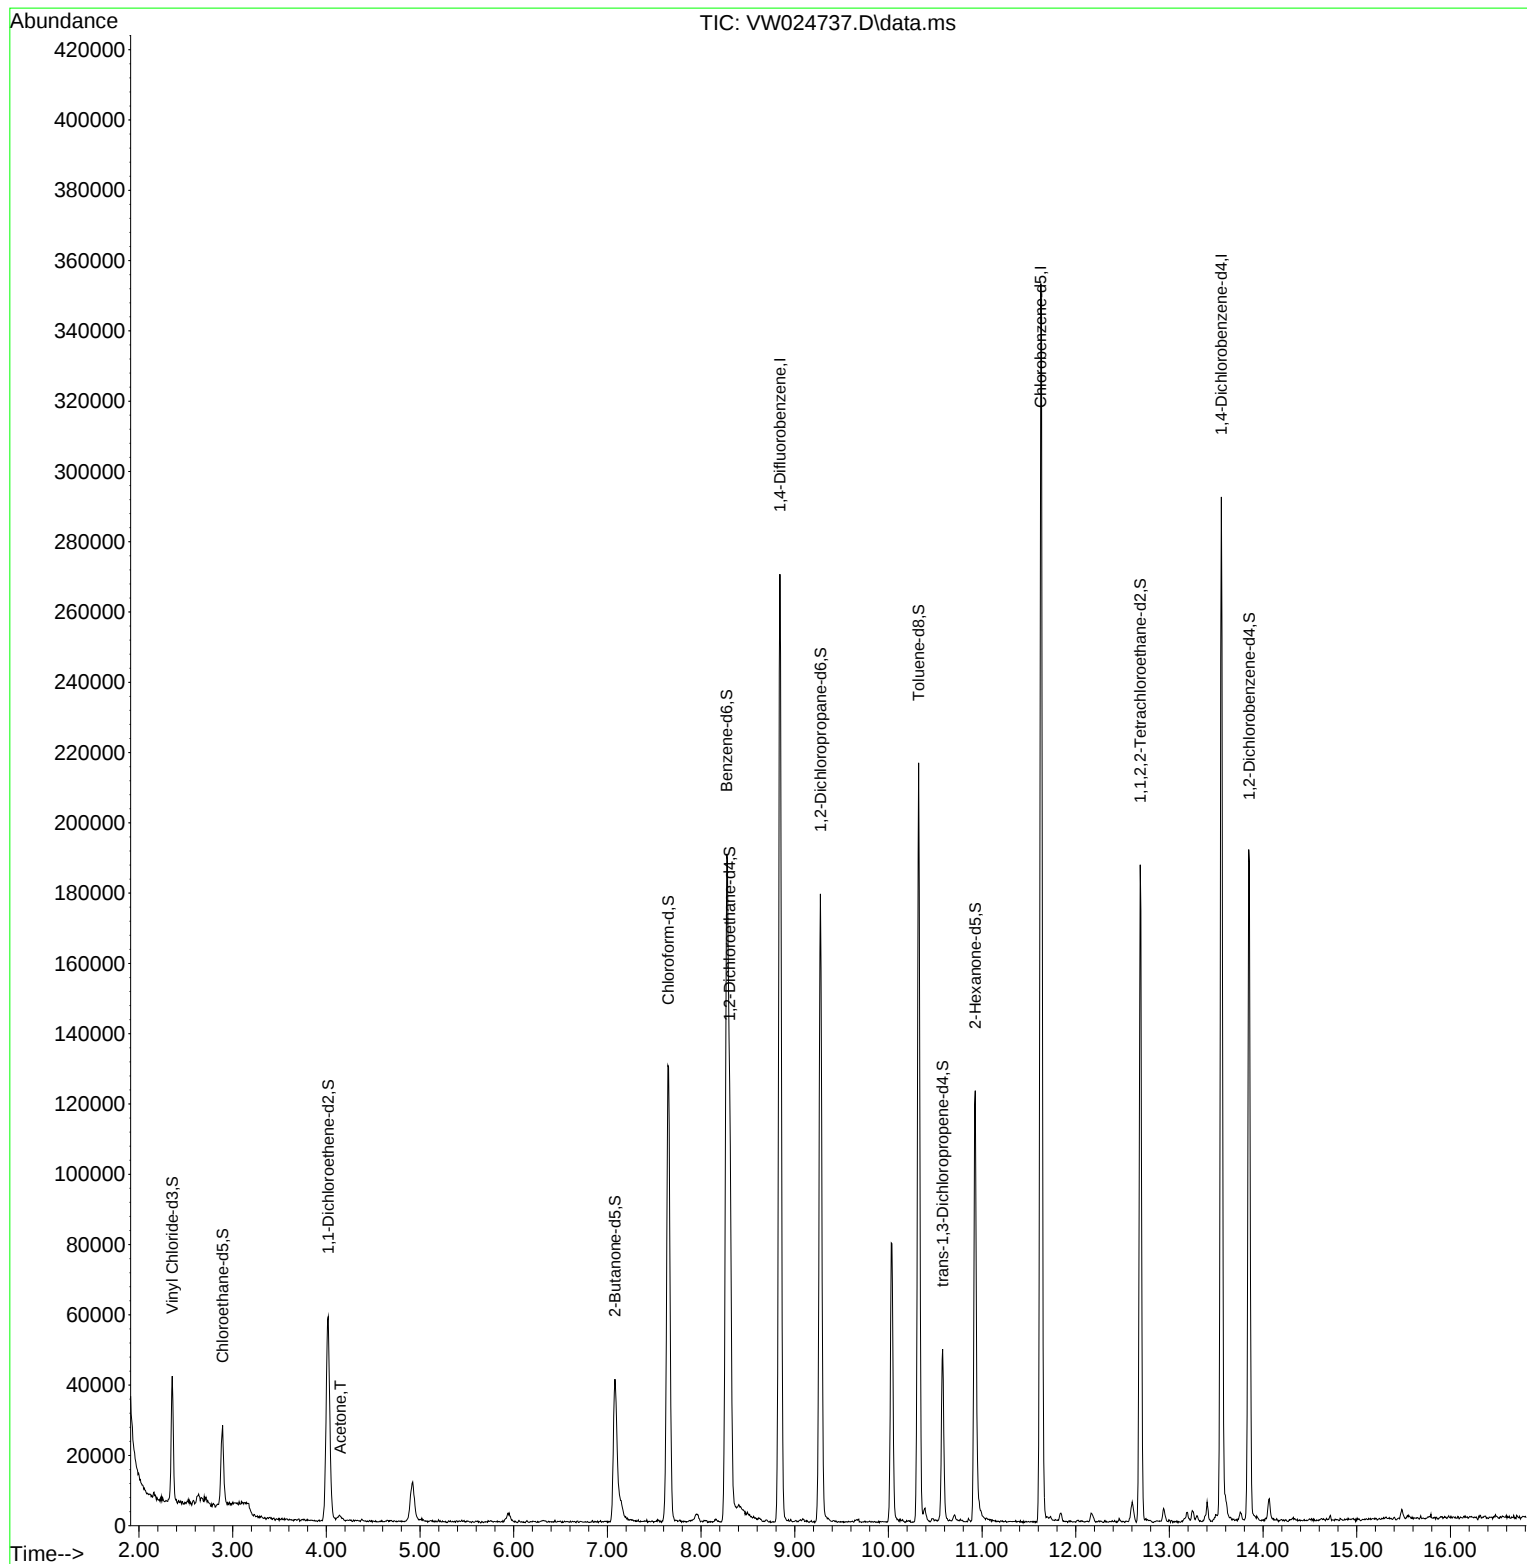

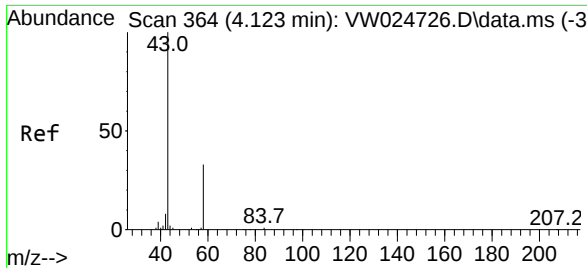

#13
 Acetone
 Concen: 4.853 ug/L
 RT: 4.147 min Scan# 30
 Delta R.T. 0.025 min
 Lab File: VW024737.D
 Acq: 05 Oct 2022 15:35

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BG0

Tgt Ion: 43 Resp: 2966
 Ion Ratio Lower Upper
 43 100
 58 32.7 0.0 67.6

