




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
 Data File : VW024757.D
 Acq On : 06 Oct 2022 14:18
 Operator : SY/VA
 Sample : N4991-10RE
 Misc : 4.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BG2RE

Manual IntegrationsAPPROVED

Quant Time: Oct 07 03:07:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/07/2022
 Supervised By :Mahesh Dadoda 10/07/2022

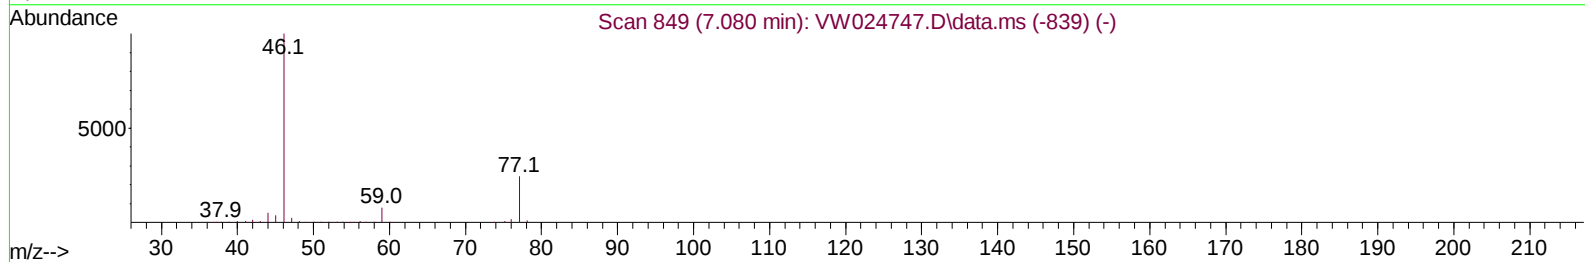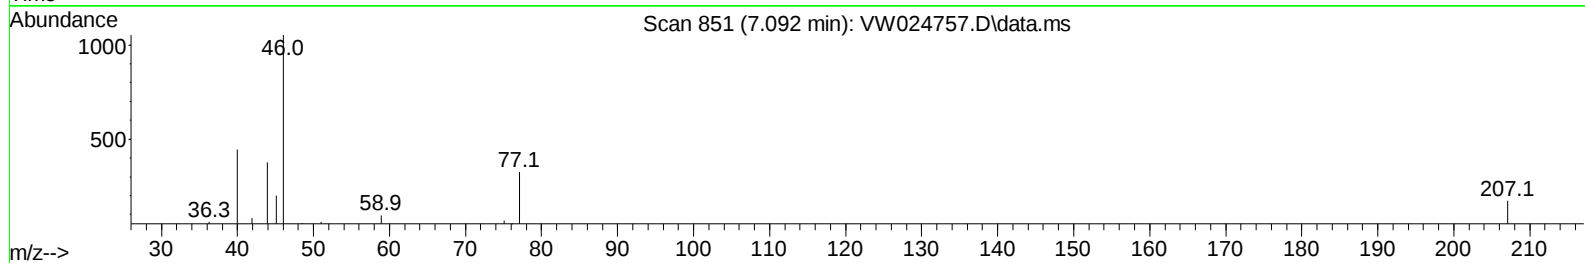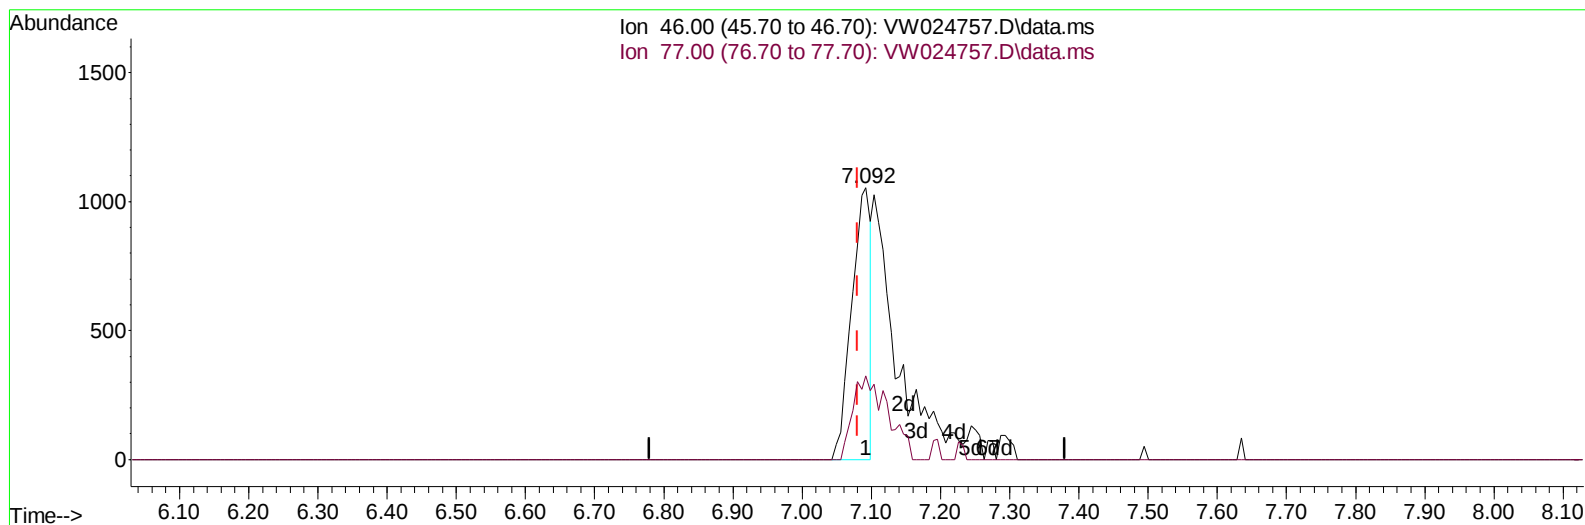

TIC: VW024757.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.012) 28.18 ug/L

response 1991

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.60	37.47#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
 Data File : VW024757.D
 Acq On : 06 Oct 2022 14:18
 Operator : SY/VA
 Sample : N4991-10RE
 Misc : 4.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BG2RE

Manual IntegrationsAPPROVED

Quant Time: Oct 07 03:07:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/07/2022
 Supervised By :Mahesh Dadoda 10/07/2022

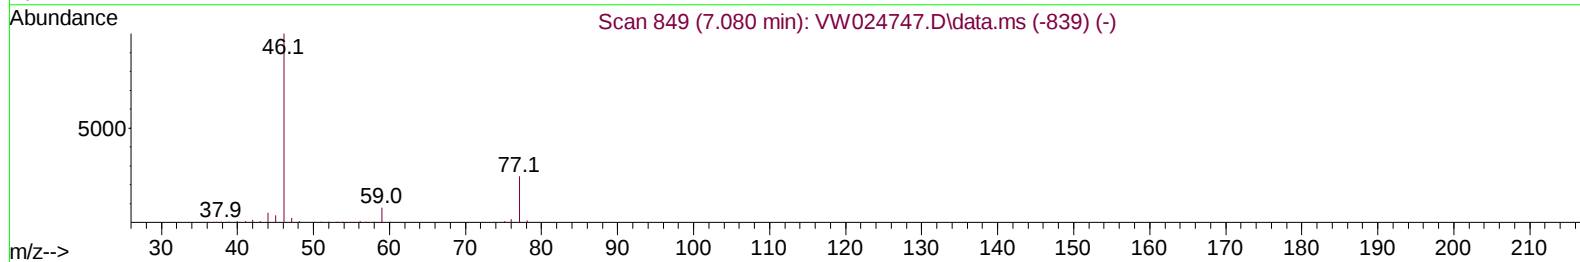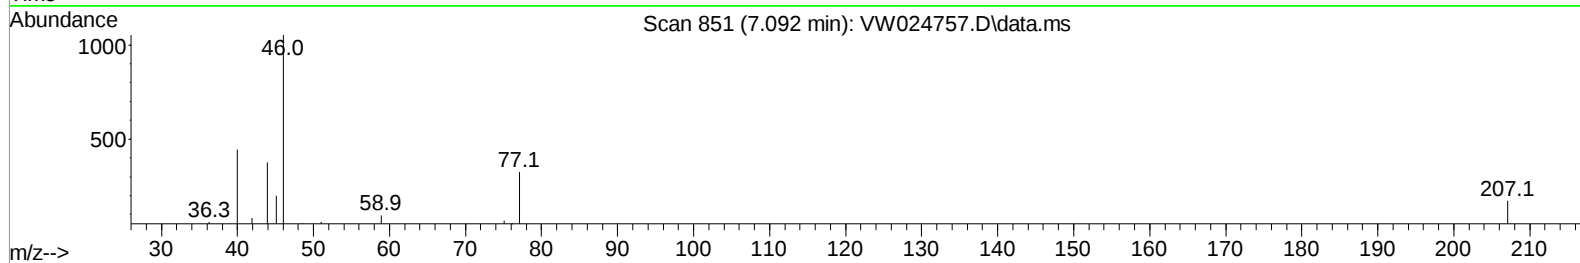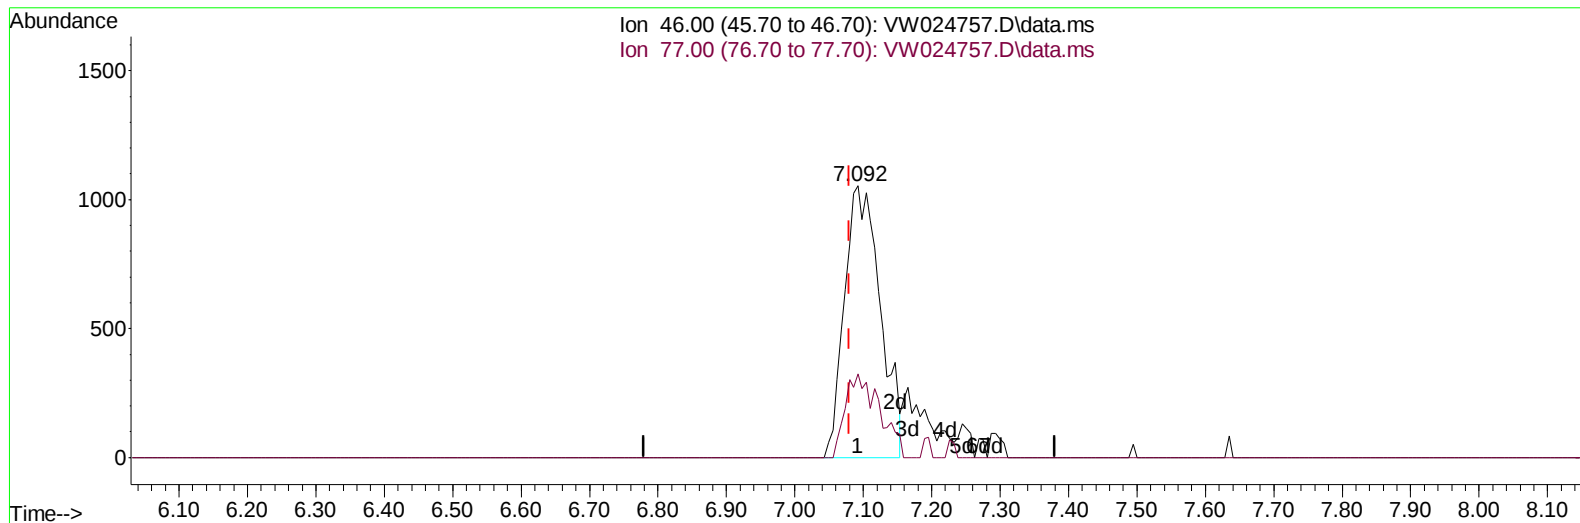

TIC: VW024757.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.012) 54.43 ug/L m

response 3845

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.60	19.40
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
Data File : VW024757.D
Acq On : 06 Oct 2022 14:18
Operator : SY/VA
Sample : N4991-10RE
Misc : 4.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BG2RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2022
Supervised By :Mahesh Dadoda 10/07/2022

Quant Time: Oct 07 03:07:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

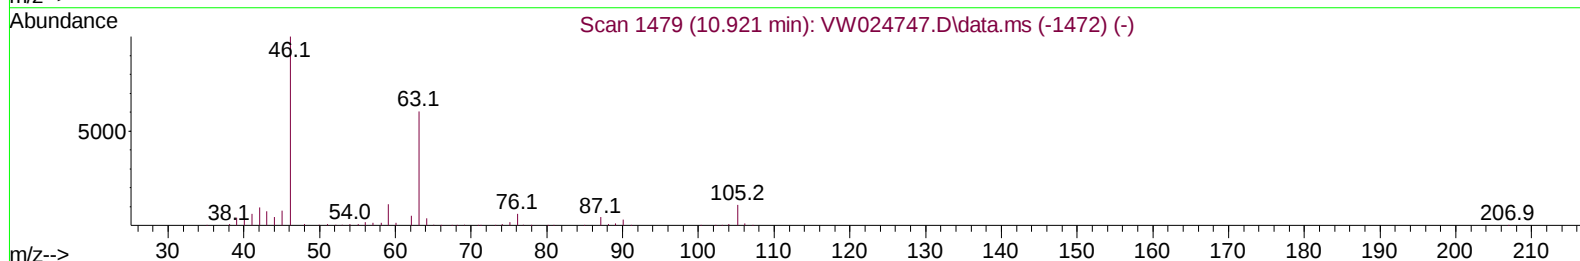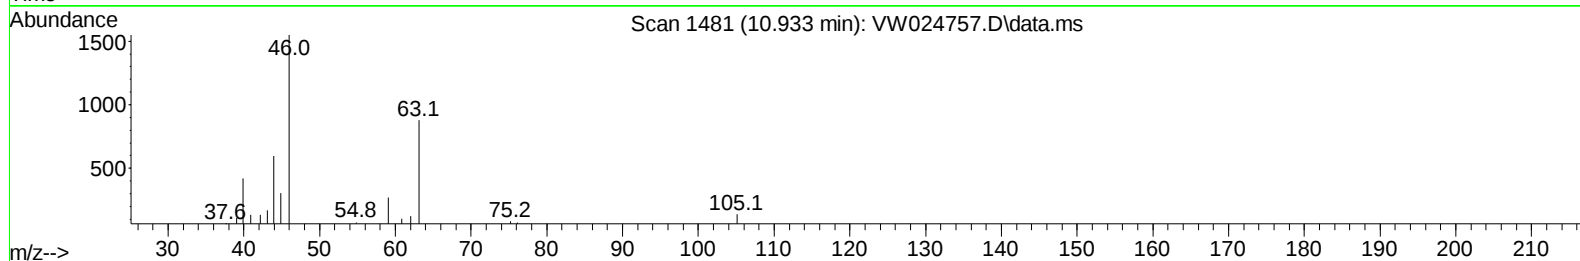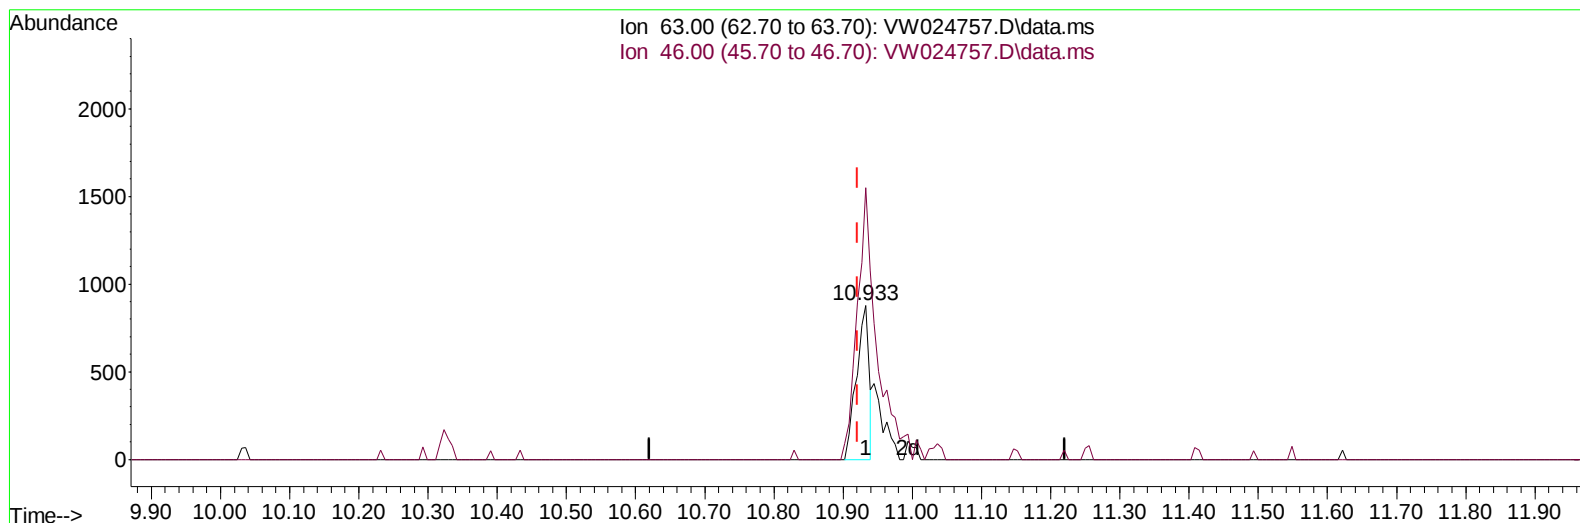

TIC: VW024757.D\data.ms

(47) 2-Hexanone-d5 (S)

10.933min (+ 0.012) 23.78 ug/L

response 1110

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	166.00	266.67#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
Data File : VW024757.D
Acq On : 06 Oct 2022 14:18
Operator : SY/VA
Sample : N4991-10RE
Misc : 4.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BG2RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2022
Supervised By :Mahesh Dadoda 10/07/2022

Quant Time: Oct 07 03:07:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

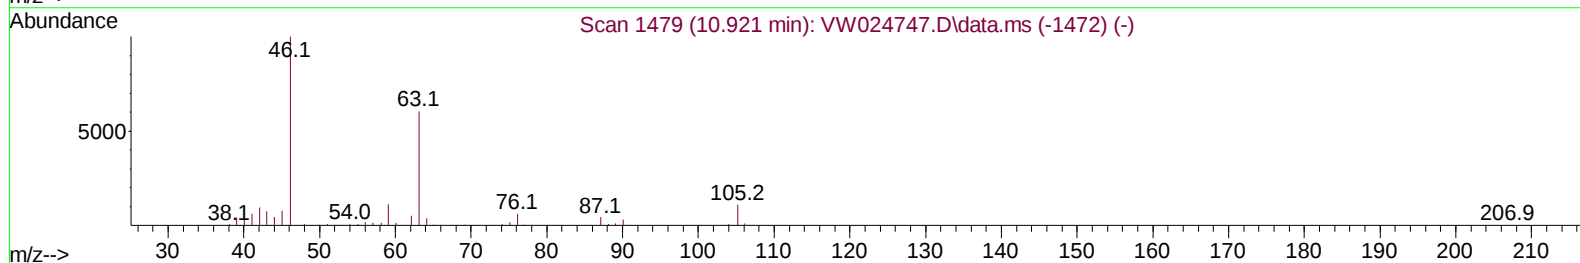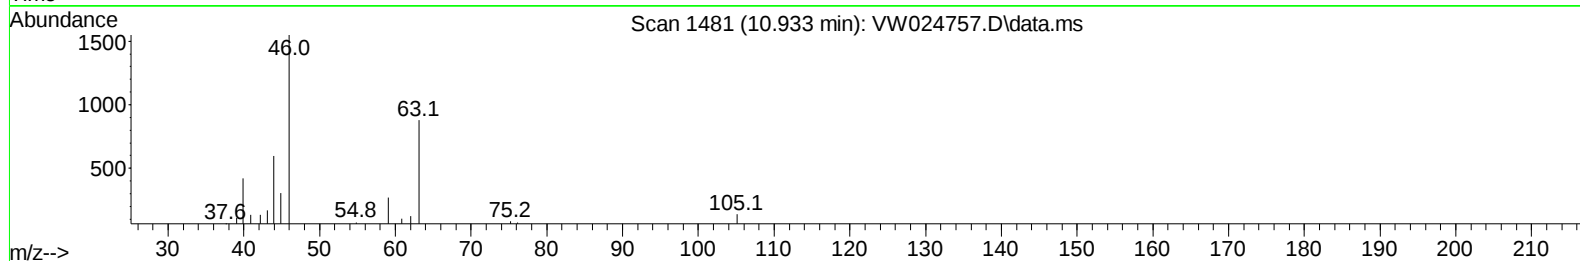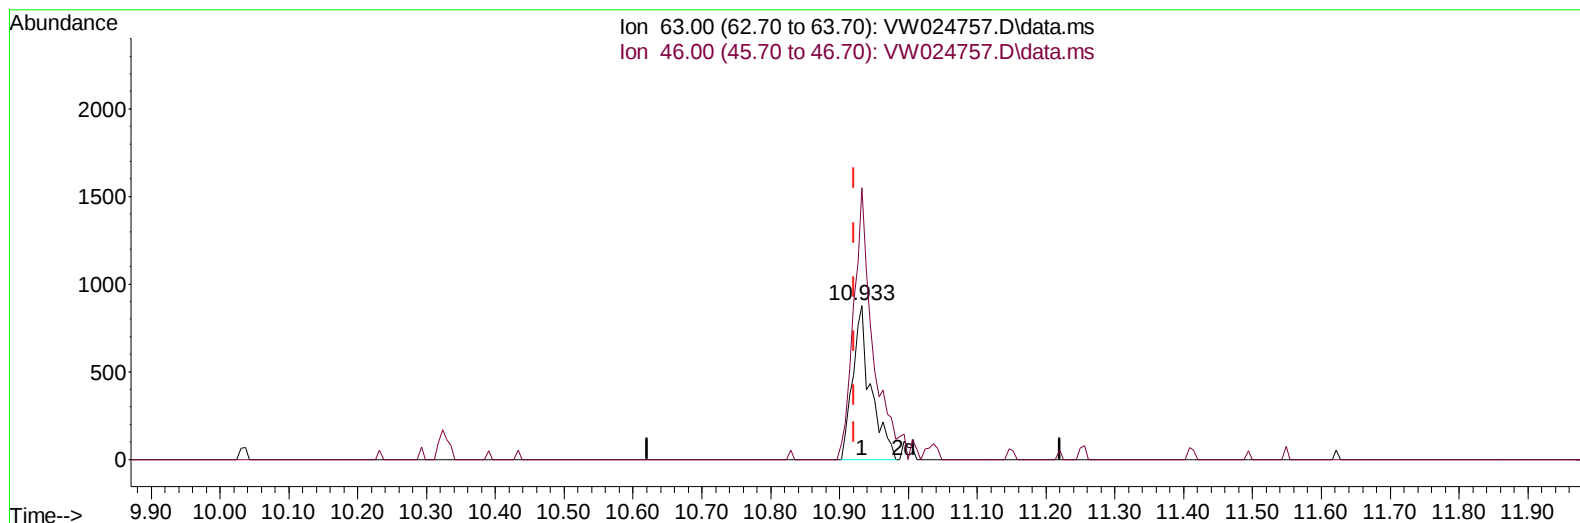

TIC: VW024757.D\data.ms

(47) 2-Hexanone-d5 (S)

10.933min (+ 0.012) 34.33 ug/L m

response 1602

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	166.00	184.77
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100622\
 Data File : VW024757.D
 Acq On : 06 Oct 2022 14:18
 Operator : SY/VA
 Sample : N4991-10RE
 Misc : 4.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BG2RE

Manual IntegrationsAPPROVED

Quant Time: Oct 07 03:07:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/07/2022
 Supervised By :Mahesh Dadoda 10/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	18781	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	13968	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	3209	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	3452	17.568	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	70.280%	
7) Chloroethane-d5	2.898	69	4899	42.903	ug/L	0.01
Spiked Amount 25.000	Range 30	- 150	Recovery	=	171.600%#	
11) 1,1-Dichloroethene-d2	4.038	63	5373	11.814	ug/L	0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	47.240%	
21) 2-Butanone-d5	7.092	46	3845m	54.426	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	108.860%	
24) Chloroform-d	7.653	84	13138	26.167	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	104.680%	
26) 1,2-Dichloroethane-d4	8.305	65	7175	27.548	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	110.200%	
32) Benzene-d6	8.281	84	18517	20.741	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.960%	
36) 1,2-Dichloropropane-d6	9.275	67	8280	30.354	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	121.400%#	
41) Toluene-d8	10.323	98	12094	15.156	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	60.640%	
43) trans-1,3-Dichloroprop...	10.585	79	1953	16.077	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	64.320%	
47) 2-Hexanone-d5	10.933	63	1602m	34.325	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	68.660%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	7706	39.648	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	158.600%#	
66) 1,2-Dichlorobenzene-d4	13.847	152	2758	24.424	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	97.680%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
Data File : VW024757.D
Acq On : 06 Oct 2022 14:18
Operator : SY/VA
Sample : N4991-10RE
Misc : 4.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BG2RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2022
Supervised By :Mahesh Dadoda 10/07/2022

Quant Time: Oct 07 03:07:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

