




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
 Data File : VW024765.D
 Acq On : 06 Oct 2022 17:31
 Operator : SY/VA
 Sample : N5023-06
 Misc : 6.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BD9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2022
 Supervised By :Mahesh Dadoda 10/07/2022

Quant Time: Oct 07 03:08:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

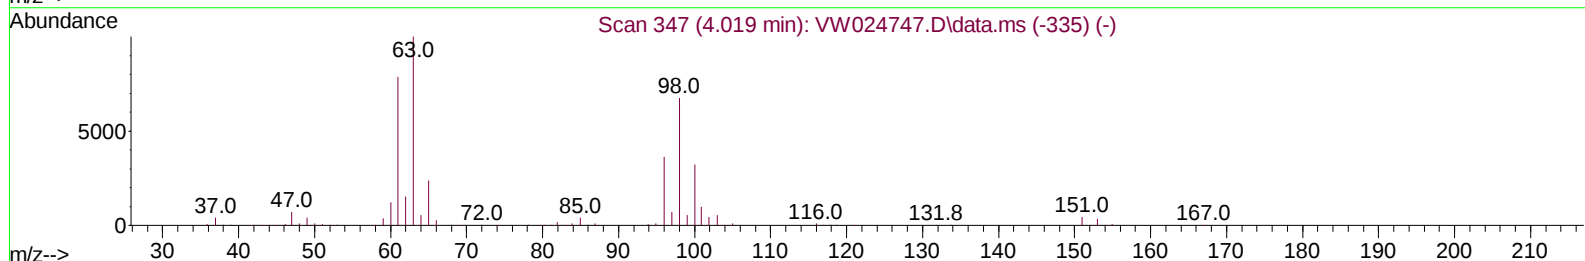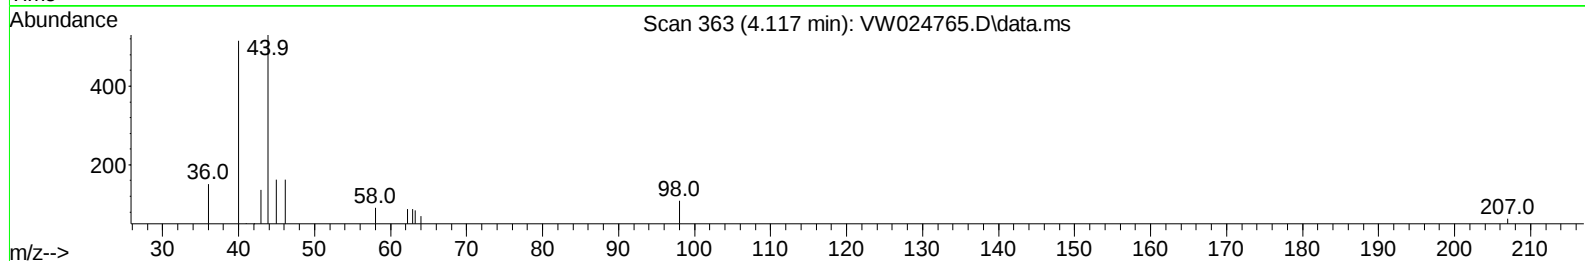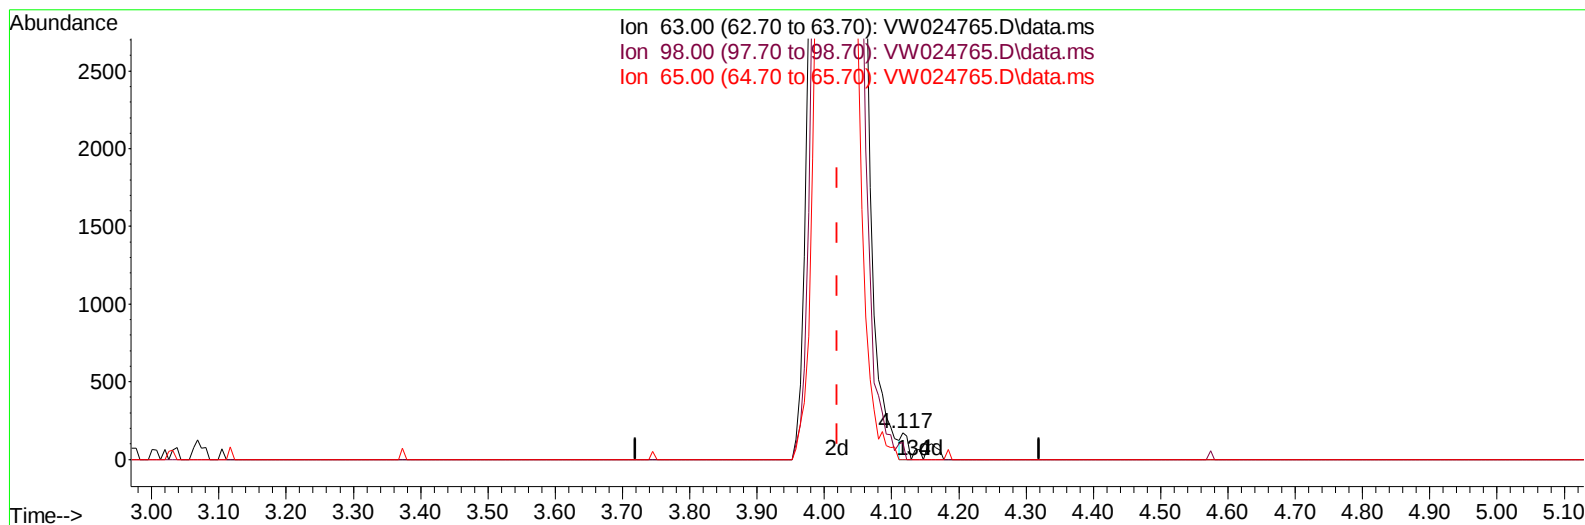

TIC: VW024765.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.117min (+ 0.097) 0.01 ug/L

response 119

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	74.00	64.71
65.00	22.40	25.21
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
 Data File : VW024765.D
 Acq On : 06 Oct 2022 17:31
 Operator : SY/VA
 Sample : N5023-06
 Misc : 6.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BD9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2022
 Supervised By :Mahesh Dadoda 10/07/2022

Quant Time: Oct 07 03:08:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

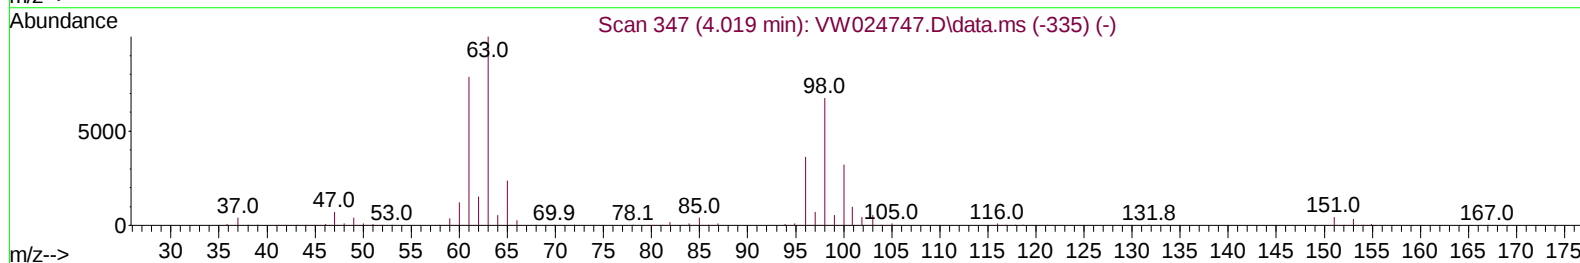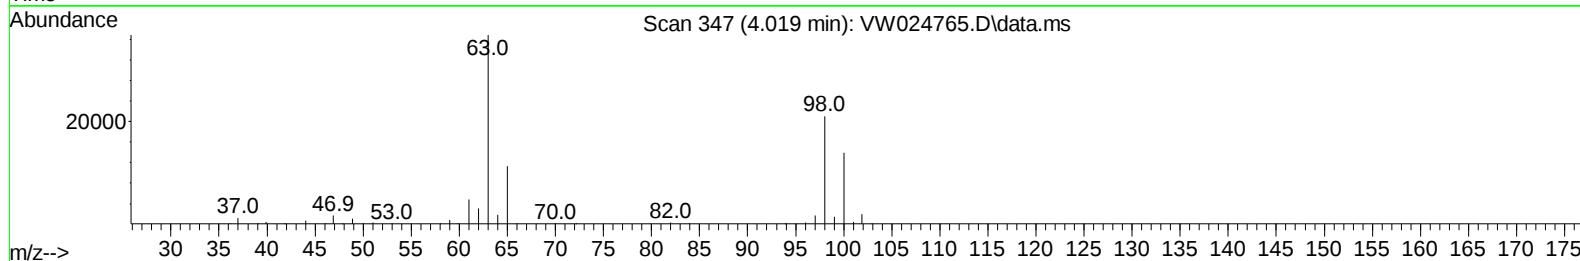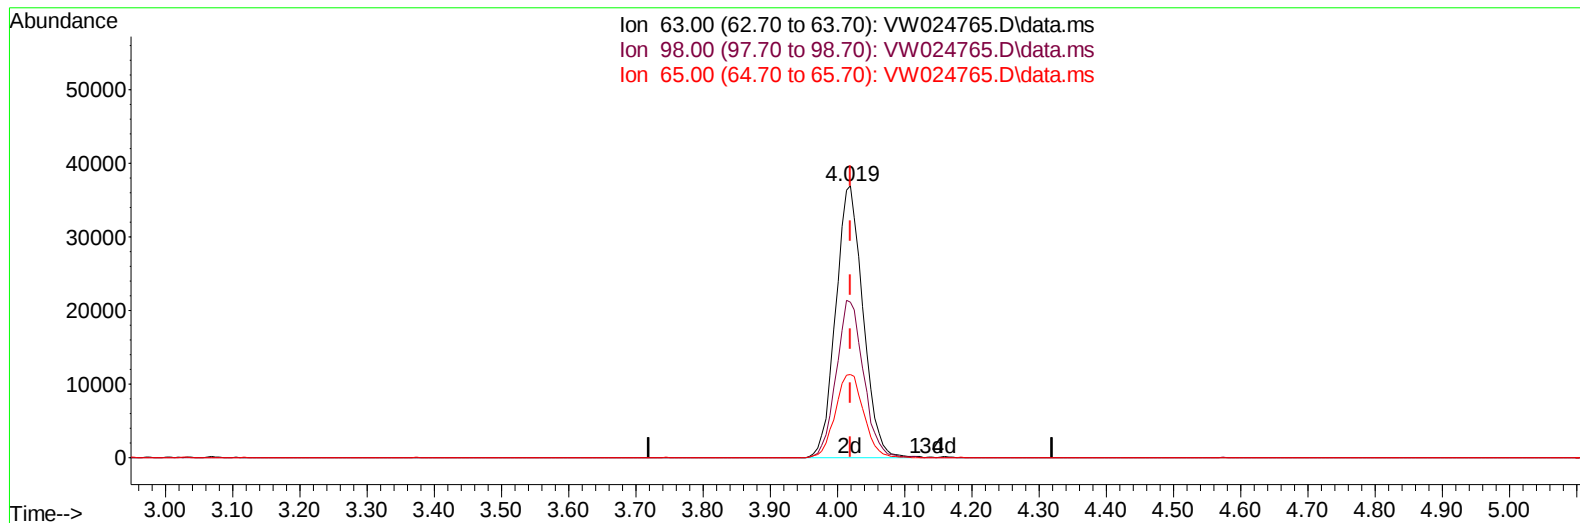

TIC: VW024765.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 7.53 ug/L m

response 103904

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	74.00	0.07#
65.00	22.40	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100622\
 Data File : VW024765.D
 Acq On : 06 Oct 2022 17:31
 Operator : SY/VA
 Sample : N5023-06
 Misc : 6.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BD9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2022
 Supervised By :Mahesh Dadoda 10/07/2022

Quant Time: Oct 07 03:08:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	570062	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	472834	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	181129	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	70087	11.751	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	47.000%	
7) Chloroethane-d5	2.885	69	49602	14.311	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	57.240%	
11) 1,1-Dichloroethene-d2	4.019	63	103904m	7.527	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	30.120%#	
21) 2-Butanone-d5	7.086	46	110947	51.740	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	103.480%	
24) Chloroform-d	7.647	84	281320	18.460	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	73.840%	
26) 1,2-Dichloroethane-d4	8.305	65	152673	19.312	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	77.240%	
32) Benzene-d6	8.275	84	448973	14.856	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	59.440%	
36) 1,2-Dichloropropane-d6	9.274	67	177668	19.241	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	76.960%	
41) Toluene-d8	10.323	98	328106	12.147	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	48.600%	
43) trans-1,3-Dichloroprop...	10.579	79	50837	12.363	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	49.440%	
47) 2-Hexanone-d5	10.920	63	80225	50.779	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.560%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	178572	27.141	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	108.560%	
66) 1,2-Dichlorobenzene-d4	13.847	152	111996	17.572	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	70.280%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
Data File : VW024765.D
Acq On : 06 Oct 2022 17:31
Operator : SY/VA
Sample : N5023-06
Misc : 6.72g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BD9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/07/2022
Supervised By :Mahesh Dadoda 10/07/2022

Quant Time: Oct 07 03:08:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

