
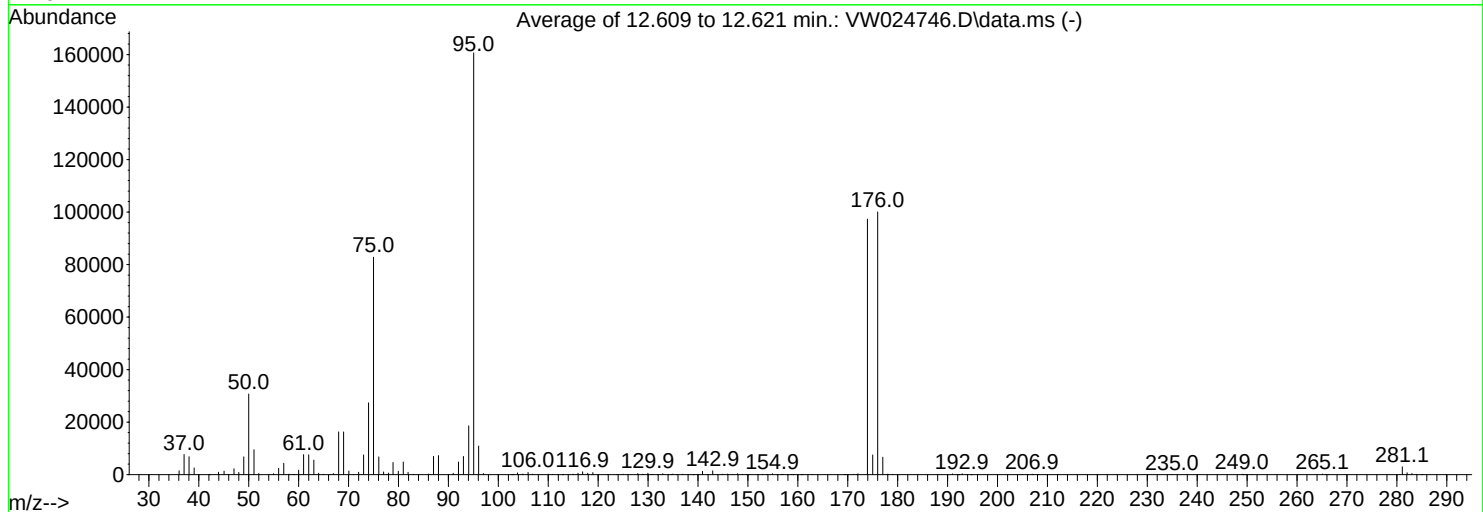


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100622\
 Data File : VW024746.D
 Acq On : 06 Oct 2022 08:07
 Operator : SY/VA
 Sample : BFB437
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB437

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Title : SFAM01.0
 Last Update : Fri Oct 07 03:04:02 2022

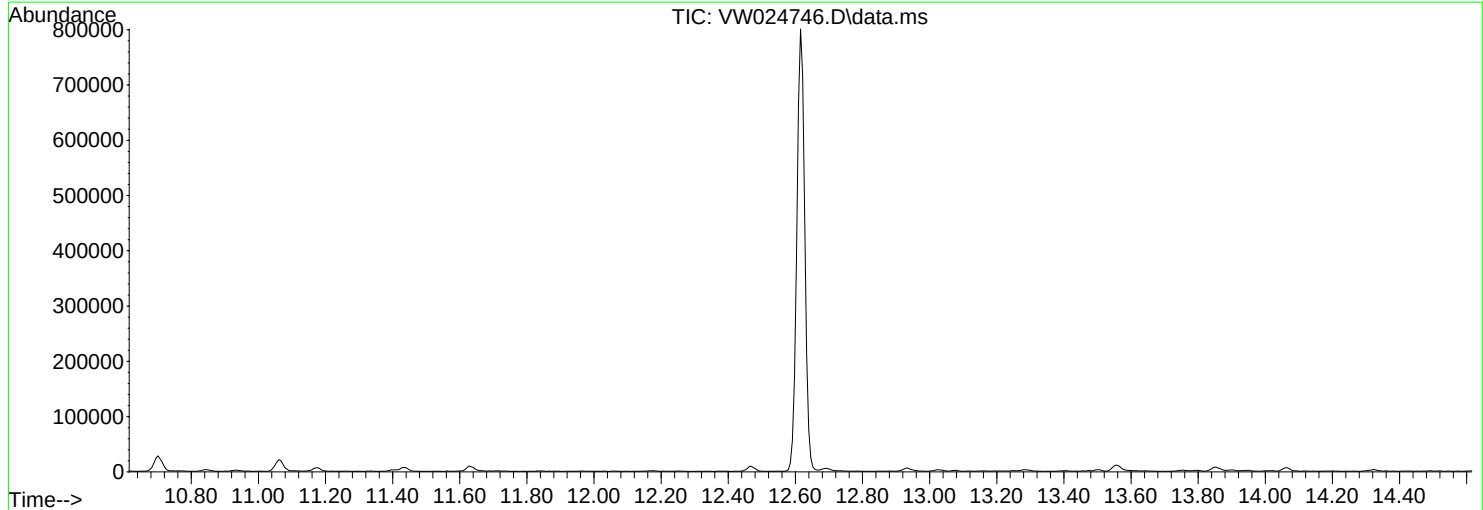

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	30701	PASS
75	95	30	80	51.5	82819	PASS
95	95	100	100	100.0	160661	PASS
96	95	5	9	6.8	10920	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	60.6	97325	PASS
175	174	5	9	7.7	7479	PASS
176	174	95	105	102.8	100088	PASS
177	176	5	10	6.6	6650	PASS

m/z	Abundance
40.00	294.0
41.10	69.0
43.10	148.0
43.90	388.0
55.00	103.0
57.20	127.0
69.10	60.0
75.00	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

m/z	Abundance
36.00	1469.0
37.10	7483.0
38.00	6481.0
39.00	2883.0
39.90	459.0
40.90	61.0
43.10	164.0
44.00	1287.0
45.00	1513.0
46.00	133.0
47.00	2099.0
48.10	735.0
49.00	6517.0
50.00	29800.0
51.10	9084.0
52.00	395.0
55.00	438.0
56.00	2408.0
57.00	4495.0
58.10	165.0
59.20	225.0
60.00	1741.0
61.00	7297.0
62.00	6761.0
63.10	5286.0
64.00	636.0
65.00	196.0
66.90	409.0
68.00	15540.0
69.00	16472.0
70.00	1416.0
71.00	90.0
72.00	690.0
73.00	6843.0
74.00	24936.0
75.00	76168.0
76.00	6998.0
77.00	1130.0
78.00	651.0
78.90	4094.0
79.90	1146.0
80.90	4546.0
81.90	916.0
83.00	95.0
86.10	238.0
87.00	6811.0
88.00	6374.0
91.00	382.0
92.00	4247.0
93.00	6934.0
94.10	16384.0
95.00	149376.0
96.10	10423.0
97.00	326.0
103.10	191.0
103.80	712.0
104.90	264.0
106.00	625.0
107.00	127.0
110.10	141.0
110.90	152.0
112.00	83.0
112.80	89.0
115.00	258.0
116.00	477.0
116.90	937.0
117.90	482.0
119.00	871.0
123.80	142.0
125.00	233.0
126.00	170.0
128.00	424.0
128.90	266.0
130.00	512.0
131.10	208.0
131.90	72.0
133.00	630.0
134.00	151.0
134.70	201.0
135.00	218.0
137.00	114.0
139.90	143.0
140.90	1121.0
141.90	212.0
142.90	1213.0
145.00	113.0
146.00	197.0
147.00	206.0
148.00	354.0
148.80	150.0
149.80	64.0
153.00	112.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

153.70	73.0
155.00	336.0
156.80	114.0
157.90	75.0
158.70	162.0
161.00	173.0
162.90	135.0
169.90	55.0
171.70	287.0
173.90	81968.0
175.00	6734.0
176.00	82056.0
177.00	5579.0
178.00	356.0
179.00	156.0
191.00	541.0
192.00	192.0
193.00	517.0
194.00	149.0
194.70	114.0
205.00	143.0
206.00	65.0
206.90	343.0
208.20	94.0
235.00	129.0
249.00	314.0
249.70	130.0
250.10	119.0
251.00	128.0
265.10	380.0
265.80	76.0
266.30	69.0
281.10	3856.0
282.00	1110.0
283.00	650.0
283.90	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

m/z	Abundance
36.00	1642.0
37.00	8538.0
38.00	7690.0
39.00	2606.0
39.90	465.0
42.90	108.0
44.00	1392.0
45.00	1421.0
45.90	72.0
47.00	2123.0
48.00	1153.0
49.00	7719.0
50.00	33568.0
51.00	10630.0
52.00	560.0
55.00	611.0
56.00	2653.0
57.00	4808.0
58.10	222.0
58.90	57.0
60.00	1788.0
61.00	8415.0
62.00	8558.0
63.00	5922.0
64.00	639.0
64.90	152.0
66.30	135.0
67.00	400.0
68.00	18808.0
69.00	17520.0
70.00	1580.0
71.00	95.0
72.00	1011.0
73.00	8740.0
74.00	31064.0
75.00	93808.0
76.10	7025.0
77.00	961.0
77.70	461.0
78.10	546.0
78.90	5347.0
80.00	1498.0
81.00	5417.0
81.90	984.0
83.00	175.0
85.90	331.0
87.00	7743.0
88.00	7808.0
90.90	730.0
92.00	5433.0
93.00	7456.0
94.00	21600.0
95.10	177088.0
96.10	11852.0
97.00	502.0
102.70	92.0
103.10	108.0
103.90	775.0
104.90	237.0
105.80	627.0
106.00	639.0
106.80	293.0
109.90	167.0
111.00	141.0
111.90	115.0
113.00	158.0
114.90	236.0
116.00	462.0
116.90	1175.0
117.80	533.0
118.90	728.0
121.90	82.0
123.70	99.0
125.10	154.0
125.80	117.0
127.90	441.0
128.90	285.0
129.80	543.0
130.70	262.0
132.90	381.0
134.20	115.0
135.00	356.0
135.70	74.0
136.90	306.0
139.00	55.0
140.00	143.0
140.80	1507.0
142.10	181.0
143.00	1747.0
143.80	158.0
145.00	159.0
145.90	302.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

147.00	163.0
147.90	382.0
148.90	170.0
149.70	177.0
152.10	88.0
153.00	116.0
153.80	99.0
154.80	446.0
155.80	78.0
156.80	216.0
159.00	103.0
161.10	133.0
162.90	64.0
171.00	113.0
172.10	380.0
173.90	104440.0
175.00	8105.0
176.00	106816.0
177.00	8567.0
178.10	142.0
179.10	107.0
191.00	298.0
192.20	58.0
192.80	387.0
193.90	140.0
204.90	99.0
207.20	219.0
208.00	54.0
249.00	263.0
250.90	126.0
265.10	179.0
266.30	50.0
281.10	3415.0
282.10	850.0
283.00	524.0
284.00	171.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

m/z	Abundance
36.10	1323.0
37.00	6986.0
38.10	6272.0
39.10	2267.0
39.90	402.0
42.10	73.0
43.00	114.0
44.00	1226.0
45.10	1129.0
45.80	108.0
47.10	2592.0
47.90	685.0
49.00	6151.0
50.00	28736.0
51.10	8881.0
52.00	310.0
54.90	377.0
56.00	2218.0
57.00	4078.0
57.90	220.0
58.90	70.0
60.00	1595.0
61.00	7104.0
62.00	7351.0
63.10	5461.0
64.00	440.0
64.90	119.0
67.00	390.0
68.00	14538.0
69.00	14949.0
70.10	1197.0
72.00	1039.0
73.00	6948.0
74.00	26184.0
75.00	78664.0
76.10	6226.0
77.00	1056.0
77.90	593.0
78.90	4394.0
80.00	1189.0
80.90	4568.0
81.90	790.0
83.10	102.0
86.00	171.0
87.00	6230.0
88.00	7670.0
90.90	539.0
92.00	4857.0
93.00	6413.0
94.00	17872.0
95.10	155520.0
96.00	10486.0
97.00	423.0
103.10	88.0
103.90	594.0
104.90	308.0
106.00	701.0
106.80	206.0
110.00	179.0
110.80	160.0
111.90	115.0
113.10	106.0
114.90	136.0
115.90	622.0
116.90	1205.0
118.00	559.0
119.00	763.0
123.80	60.0
124.90	128.0
125.90	147.0
127.90	450.0
129.10	268.0
130.00	545.0
130.90	176.0
132.80	155.0
134.10	87.0
134.90	233.0
135.70	66.0
136.90	193.0
140.00	167.0
141.00	1218.0
141.90	204.0
142.90	1454.0
143.90	66.0
144.90	211.0
146.00	171.0
146.80	106.0
148.00	346.0
148.80	67.0
150.00	116.0
151.90	81.0
152.90	135.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437

154.90	349.0
157.00	299.0
158.80	156.0
160.70	109.0
161.10	125.0
169.40	67.0
170.00	59.0
171.10	194.0
172.00	490.0
174.00	105568.0
175.00	7599.0
176.00	111392.0
177.00	5803.0
178.10	218.0
178.90	70.0
190.90	138.0
192.70	120.0
193.00	120.0
207.00	189.0
249.20	65.0
265.10	106.0
281.10	1793.0
282.00	317.0
283.10	183.0
285.00	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB437