
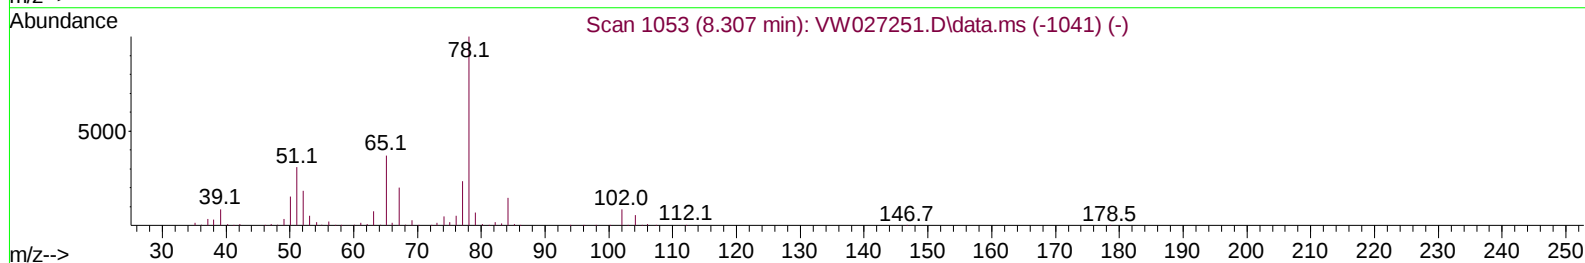
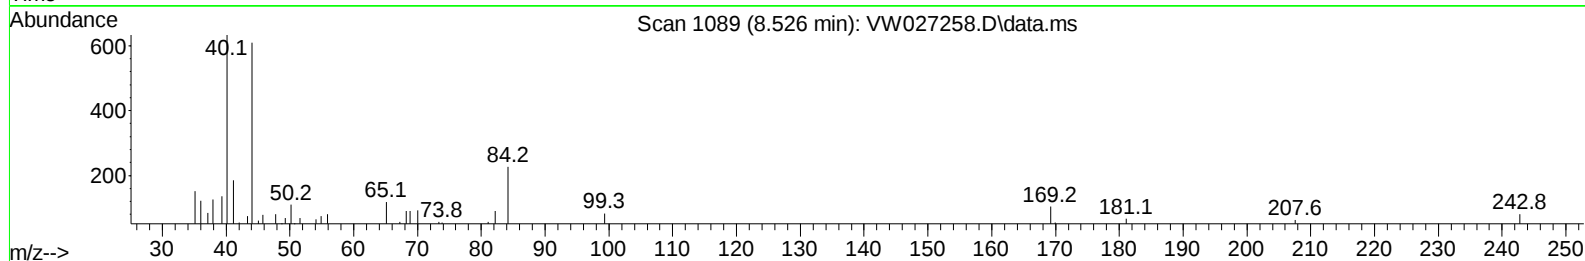


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100623\
Data File : VW027258.D
Acq On : 06 Oct 2023 13:22
Operator : SY/MD
Sample : 04771-04
Misc : 4.23g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:24:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 07 00:22:13 2023
Response via : Initial Calibration

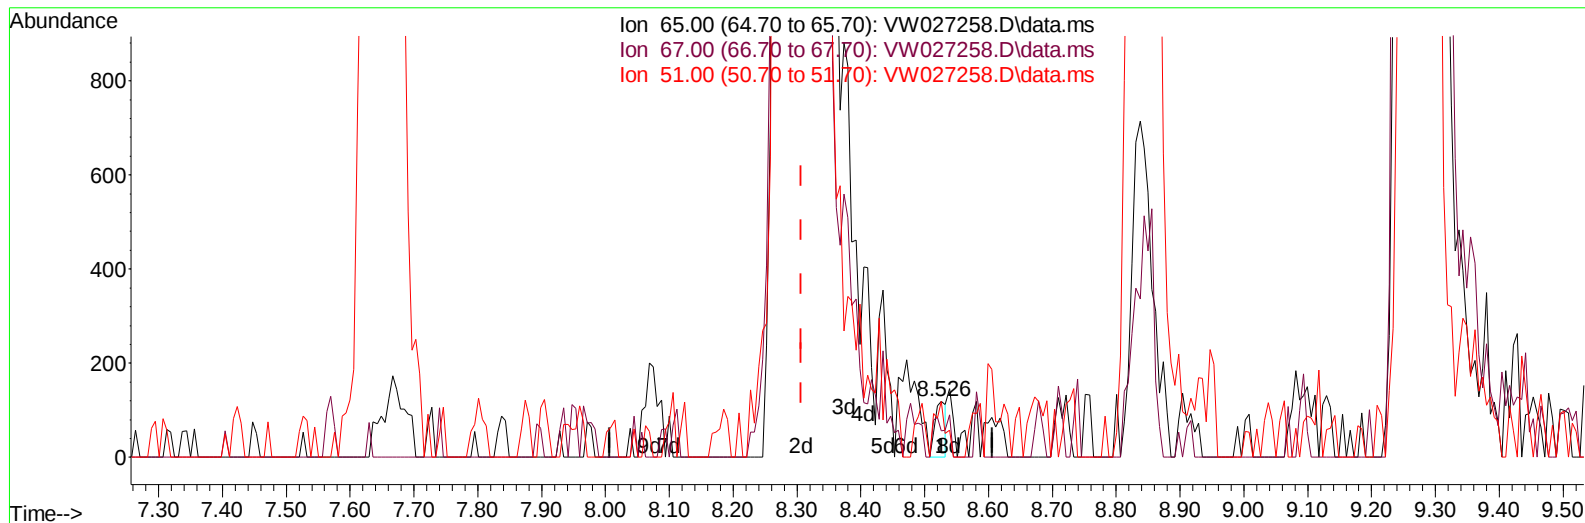

TIC: VW027258.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.526min (+ 0.220) 0.01 ug/L

response 144

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	56.25
51.00	119.20	102.78
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100623\
Data File : VW027258.D
Acq On : 06 Oct 2023 13:22
Operator : SY/MD
Sample : 04771-04
Misc : 4.23g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:24:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 07 00:22:13 2023
Response via : Initial Calibration

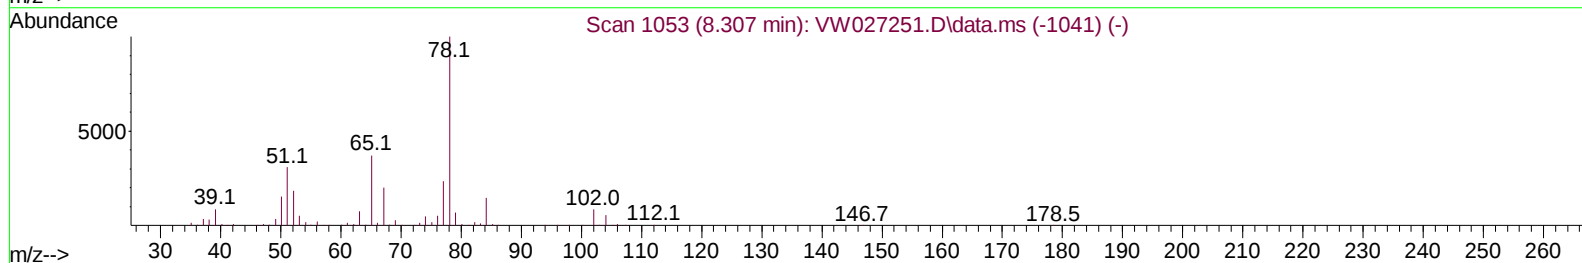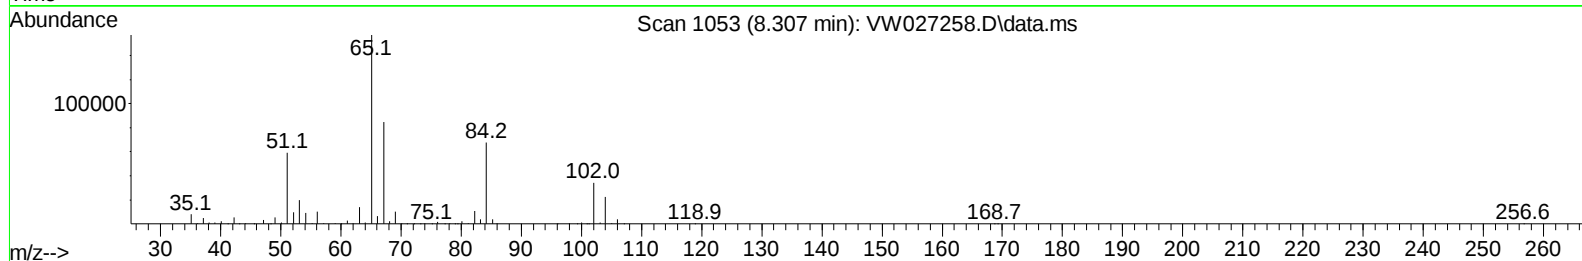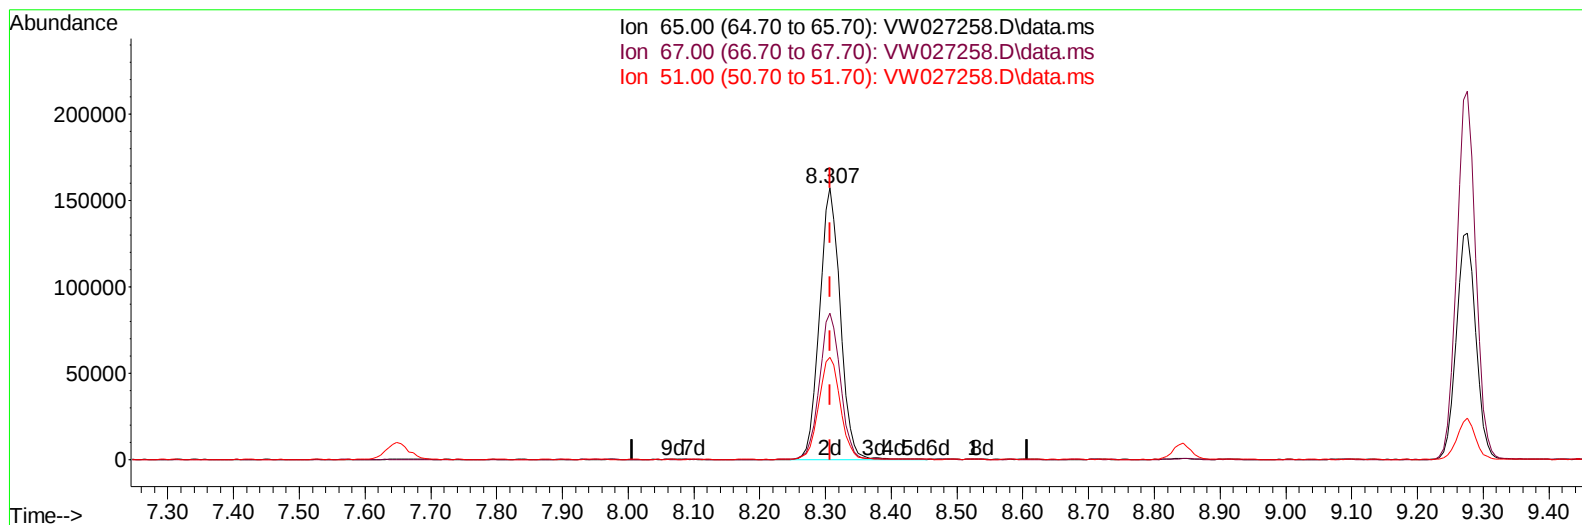

TIC: VW027258.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.307min (+ 0.000) 25.19 ug/L m****response 342753**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.02#
51.00	119.20	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100623\
 Data File : VW027258.D
 Acq On : 06 Oct 2023 13:22
 Operator : SY/MD
 Sample : 04771-04
 Misc : 4.23g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:24:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 07 00:22:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	970282	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	948176	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	388517	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	343702	22.546	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	90.200%	
7) Chloroethane-d5	2.899	69	296091	24.575	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	98.280%	
11) 1,1-Dichloroethene-d2	4.021	65	136687	21.581	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	86.320%	
21) 2-Butanone-d5	7.075	46	169338	53.732	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	107.460%	
24) Chloroform-d	7.648	84	679415	23.925	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.720%	
26) 1,2-Dichloroethane-d4	8.307	65	342753m	25.186	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	100.760%	
32) Benzene-d6	8.276	84	1348131	23.200	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.800%	
36) 1,2-Dichloropropane-d6	9.276	67	429487	24.687	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	98.760%	
41) Toluene-d8	10.325	98	1126833	21.975	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	87.880%	
43) trans-1,3-Dichloroprop...	10.575	79	153837	22.533	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.120%	
47) 2-Hexanone-d5	10.922	63	120127	45.139	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	90.280%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	344384	25.866	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	103.480%	
66) 1,2-Dichlorobenzene-d4	13.849	152	334109	25.648	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	102.600%	
Target Compounds						
					Qvalue	
16) Methylene chloride	4.917	84	34640	1.824	ug/L	98
31) Carbon tetrachloride	8.069	117	53994	2.425	ug/L	98
34) Trichloroethene	9.087	95	12042	0.688	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100623\
Data File : VW027258.D
Acq On : 06 Oct 2023 13:22
Operator : SY/MD
Sample : 04771-04
Misc : 4.23g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:24:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 07 00:22:13 2023
Response via : Initial Calibration

