
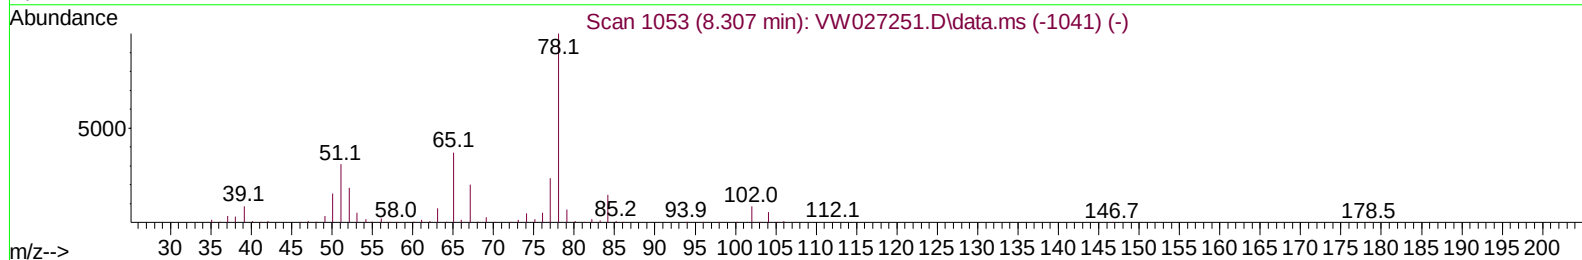
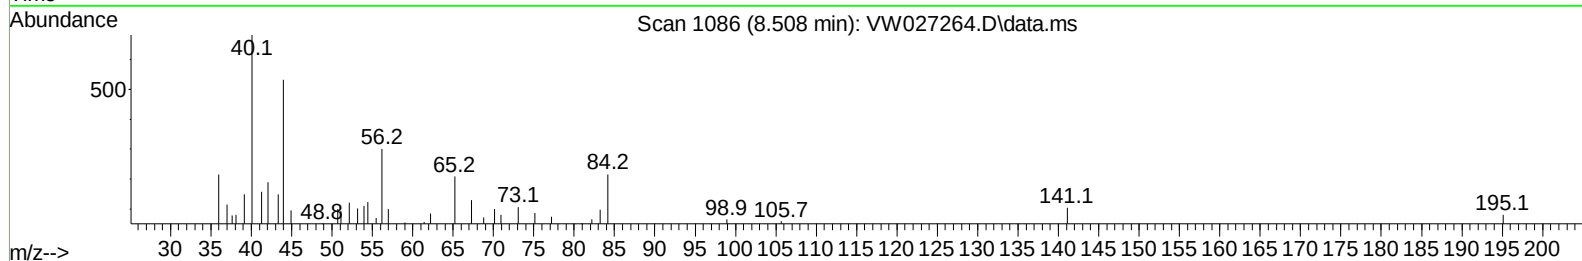


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100623\
Data File : VW027264.D
Acq On : 06 Oct 2023 15:46
Operator : SY/MD
Sample : 04771-10
Misc : 3.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:25:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 07 00:22:13 2023
Response via : Initial Calibration

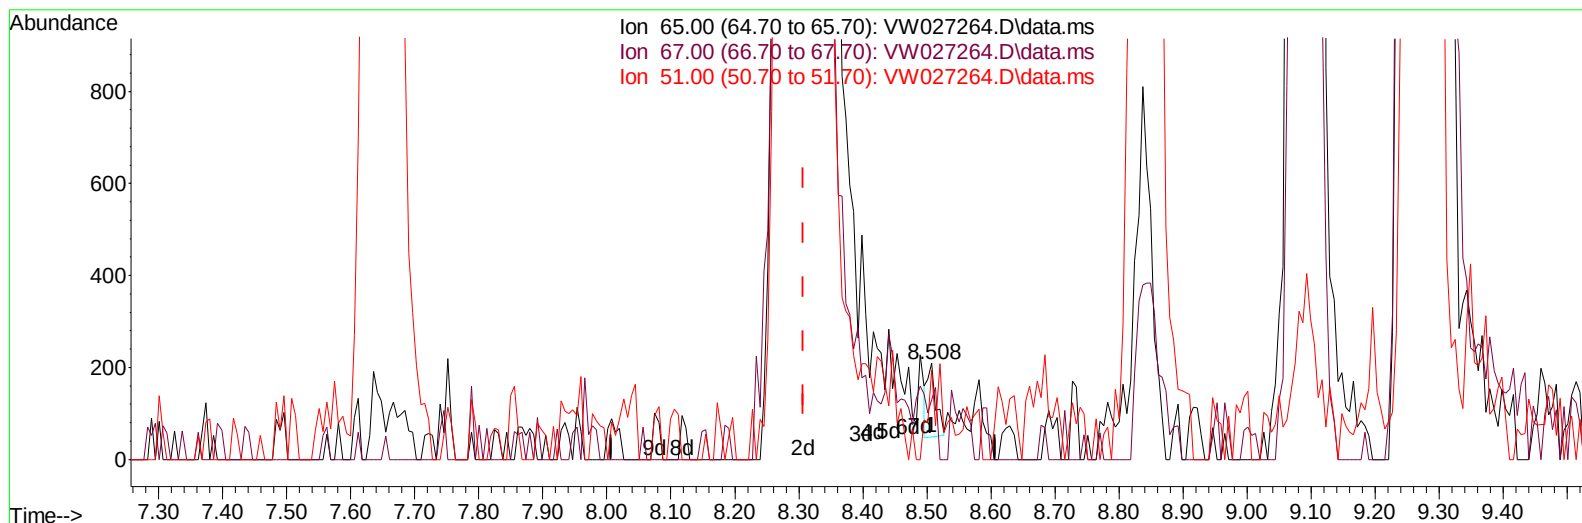

TIC: VW027264.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.508min (+ 0.201) 0.01 ug/L

response 150

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	70.00
51.00	119.20	106.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100623\
 Data File : VW027264.D
 Acq On : 06 Oct 2023 15:46
 Operator : SY/MD
 Sample : 04771-10
 Misc : 3.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:25:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 07 00:22:13 2023
 Response via : Initial Calibration

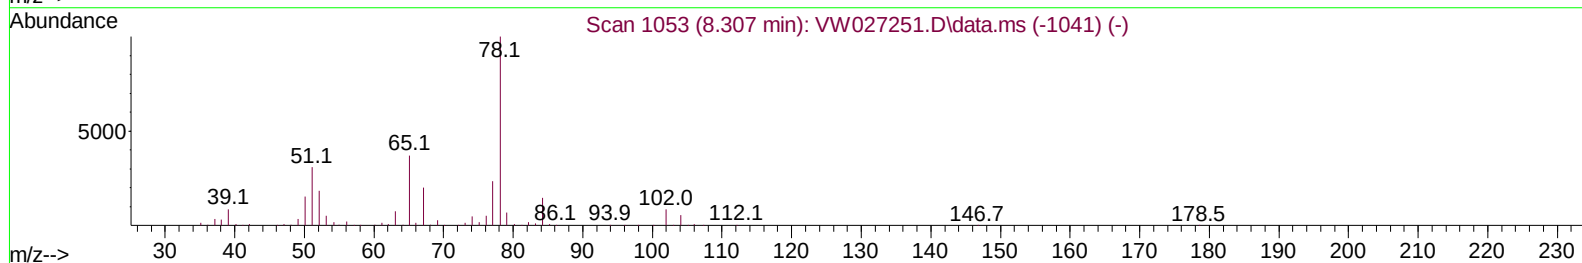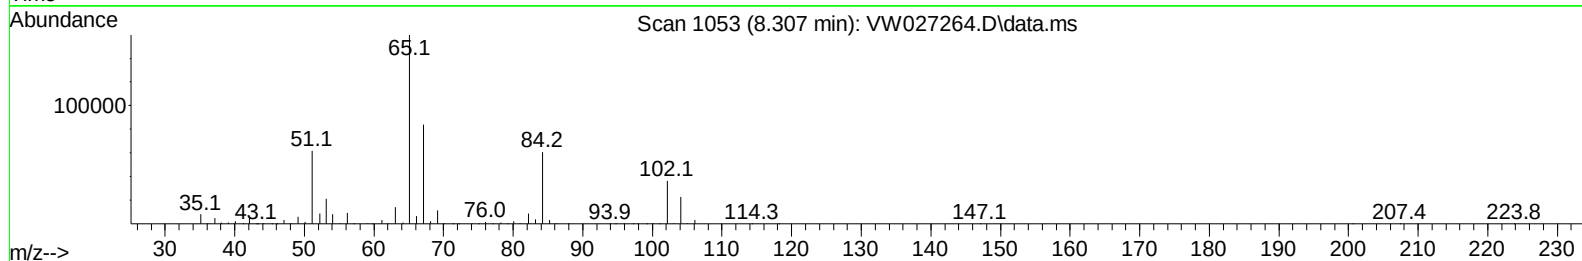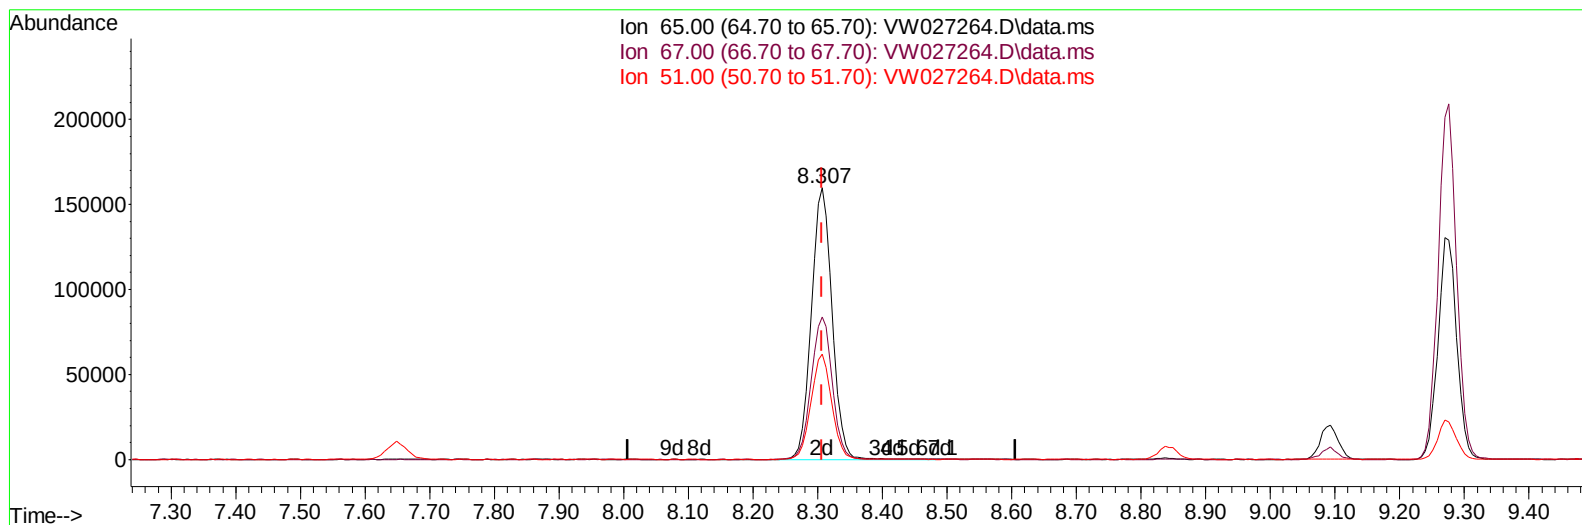

TIC: VW027264.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.307min (-0.000) 28.73 ug/L m****response 356210**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.03#
51.00	119.20	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100623\
 Data File : VW027264.D
 Acq On : 06 Oct 2023 15:46
 Operator : SY/MD
 Sample : 04771-10
 Misc : 3.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:25:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 07 00:22:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	884121	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	749634	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	218203	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	263105	18.941	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.760%	
7) Chloroethane-d5	2.899	69	258344	23.531	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.120%	
11) 1,1-Dichloroethene-d2	4.021	65	122766	21.272	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	85.080%	
21) 2-Butanone-d5	7.075	46	175559	61.135	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	122.280%	
24) Chloroform-d	7.648	84	653880	25.270	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	101.080%	
26) 1,2-Dichloroethane-d4	8.307	65	356210m	28.725	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	114.920%	
32) Benzene-d6	8.276	84	1283831	27.944	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	111.760%	
36) 1,2-Dichloropropane-d6	9.276	67	416438	30.277	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	121.120%#	
41) Toluene-d8	10.319	98	960679	23.696	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	94.800%	
43) trans-1,3-Dichloroprop...	10.581	79	138778	25.711	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	102.840%	
47) 2-Hexanone-d5	10.922	63	117446	55.819	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	111.640%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	299942	28.495	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	113.960%	
66) 1,2-Dichlorobenzene-d4	13.848	152	182916	25.002	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.000%	
Target Compounds						
20) cis-1,2-Dichloroethene	7.173	96	17161	1.094	ug/L	93
34) Trichloroethene	9.093	95	2151116	155.471	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100623\
Data File : VW027264.D
Acq On : 06 Oct 2023 15:46
Operator : SY/MD
Sample : 04771-10
Misc : 3.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:25:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 07 00:22:13 2023
Response via : Initial Calibration

