

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100625\
 Data File : VW032353.D
 Acq On : 06 Oct 2025 12:37
 Operator : SY/MD
 Sample : VW1006SBL01
 Misc : 5.00g/5mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW1006SBL01

Quant Time: Oct 07 03:42:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W100125S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 02 21:24:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.959	168	168139	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	378247	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.629	117	382025	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	188486	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	158534	64.644	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	129.280%
35) Dibromofluoromethane	7.898	113	137927	56.307	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	112.620%
50) Toluene-d8	10.325	98	472361	52.248	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	104.500%
62) 4-Bromofluorobenzene	12.617	95	169464	49.592	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	99.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100625\
Data File : VW032353.D
Acq On : 06 Oct 2025 12:37
Operator : SY/MD
Sample : VW1006SBL01
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW1006SBL01

Quant Time: Oct 07 03:42:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W100125S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 02 21:24:16 2025
Response via : Initial Calibration




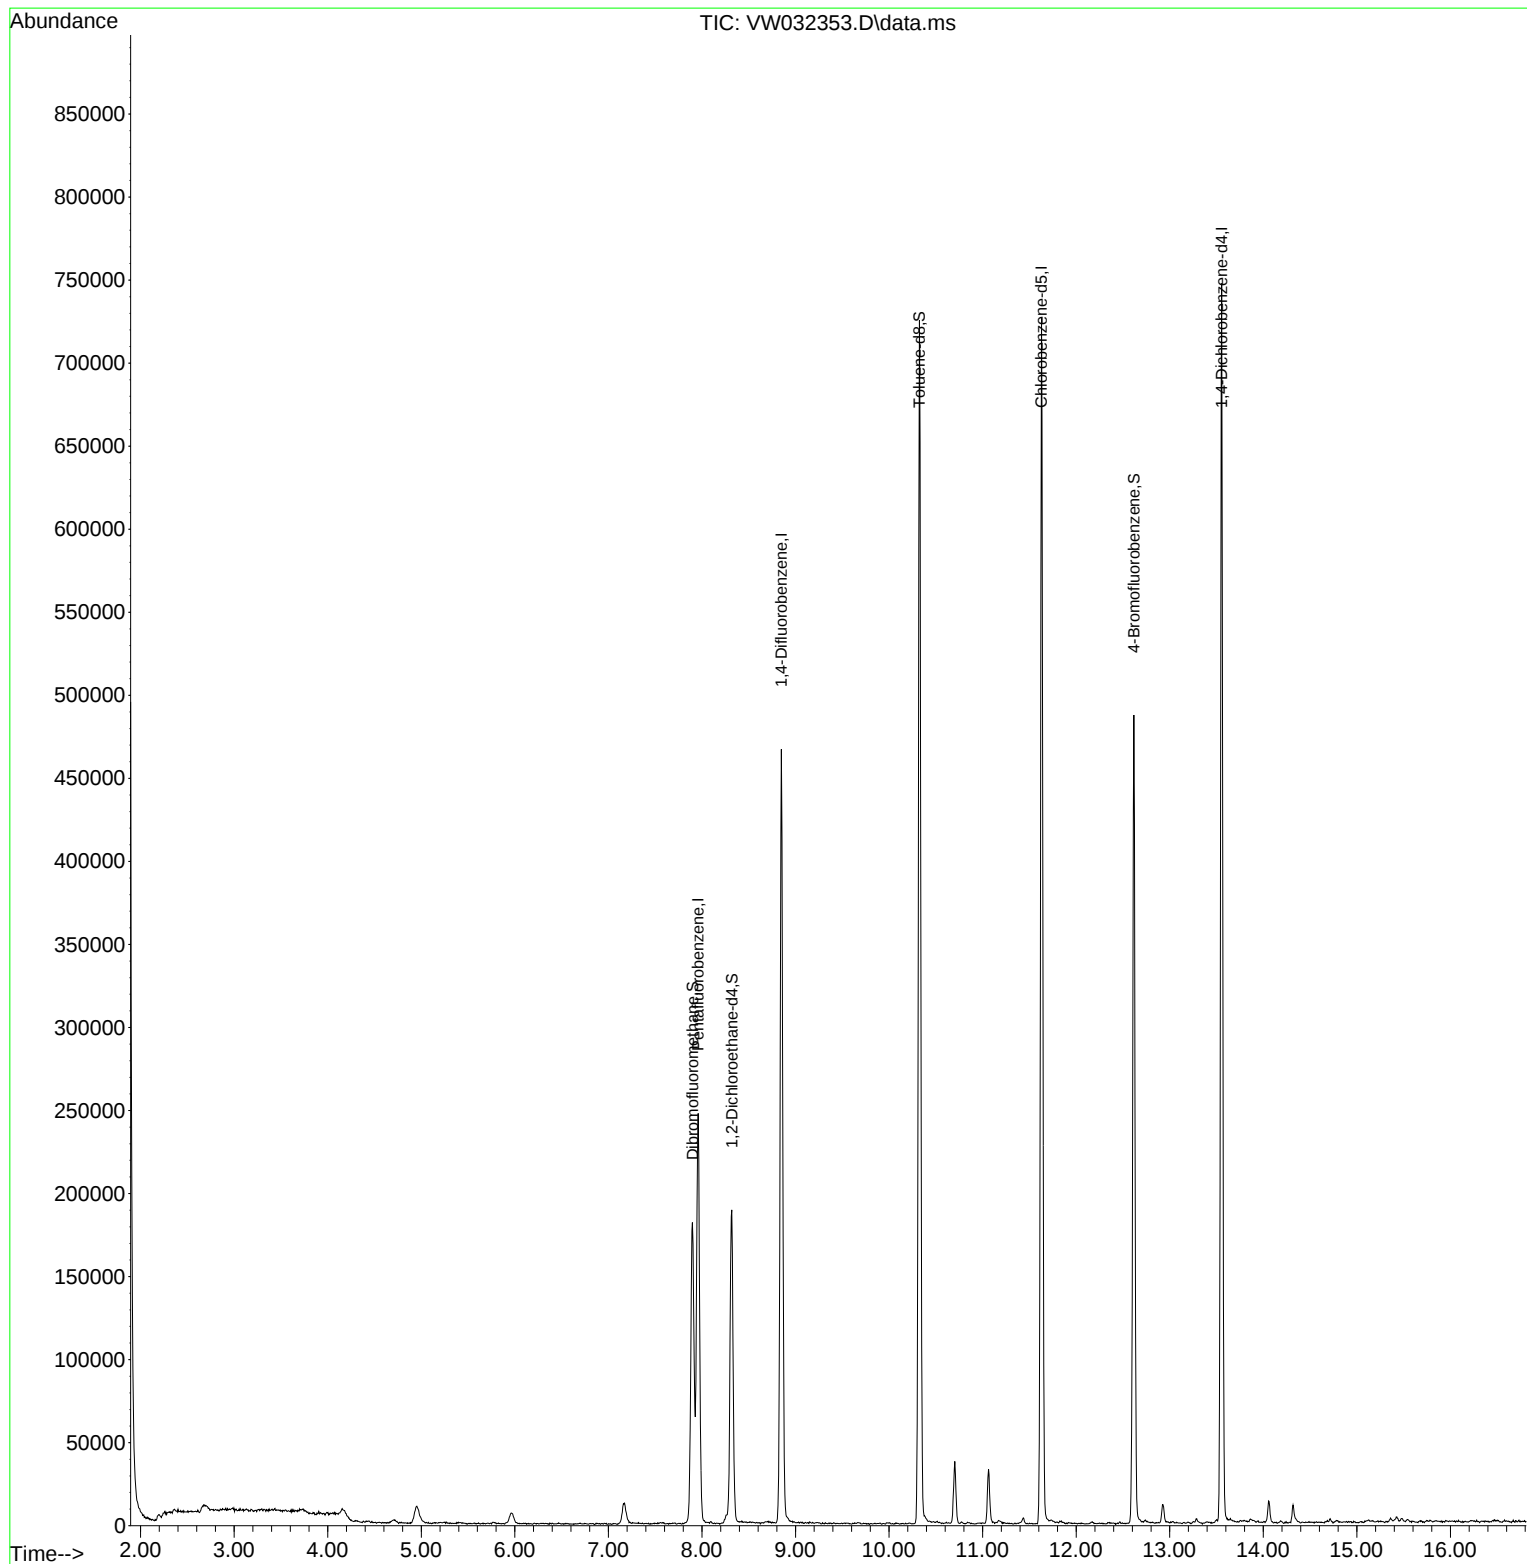


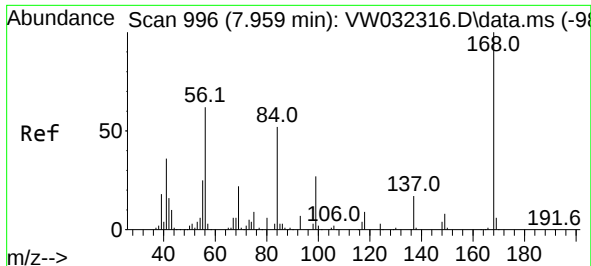

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.959 min Scan# 996
Delta R.T. -0.006 min
Lab File: VW032353.D
Acq: 06 Oct 2025 12:37




Instrument :
MSVOA_W
ClientSampleId :
VW1006SBL01


Tgt Ion:168 Resp: 168139
Ion Ratio Lower Upper
168 100
99 58.8 49.3 73.9

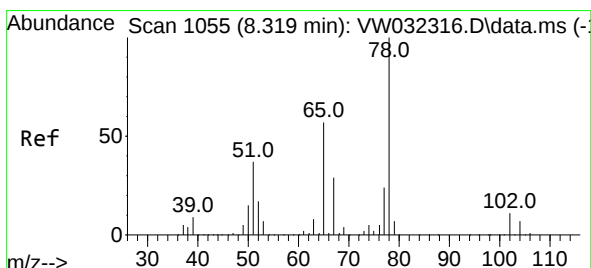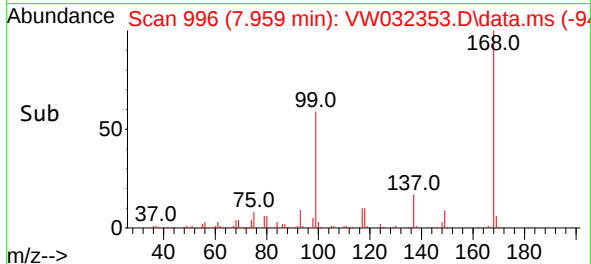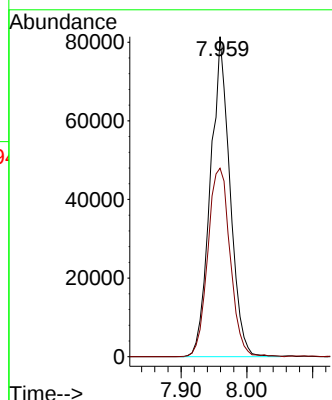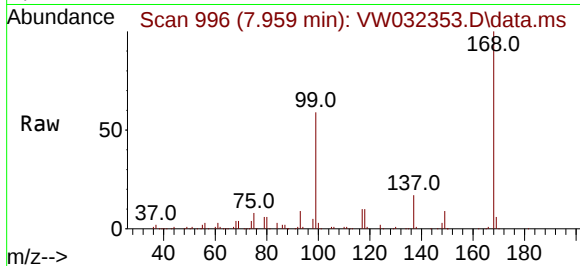

#33
1,2-Dichloroethane-d4
Concen: 64.644 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. -0.000 min
Lab File: VW032353.D
Acq: 06 Oct 2025 12:37

Tgt Ion: 65 Resp: 158534
Ion Ratio Lower Upper
65 100
67 51.8 0.0 99.6

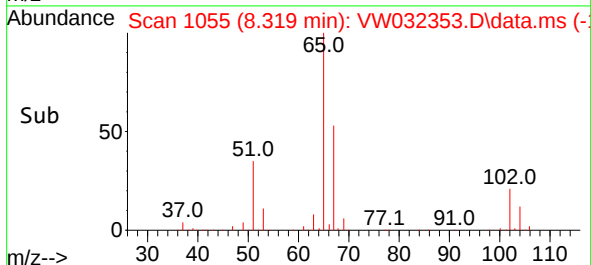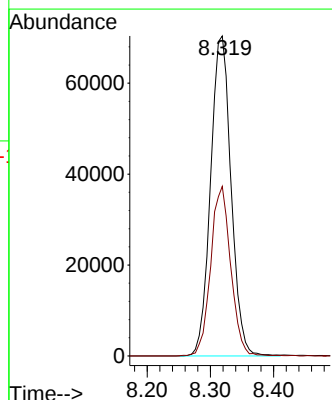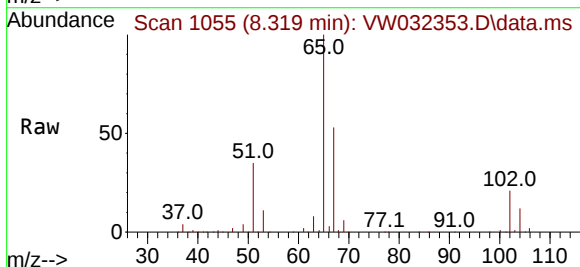

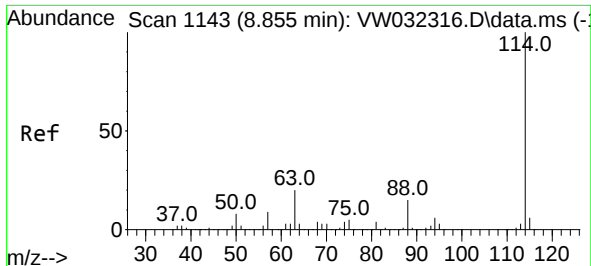

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.849 min Scan# 1143

Delta R.T. -0.006 min

Lab File: VW032353.D

Acq: 06 Oct 2025 12:37

Instrument :

MSVOA_W

ClientSampleId :

VW1006SBL01





Tgt Ion:114 Resp: 378247

Ion Ratio Lower Upper

114 100

63 21.7 0.0 40.4

88 15.6 0.0 32.0

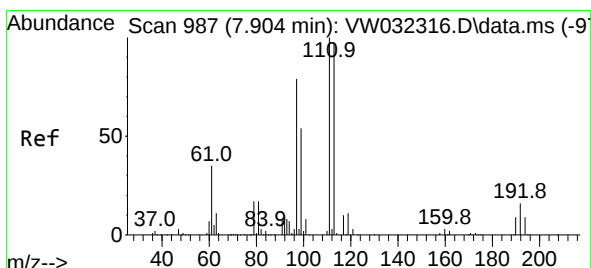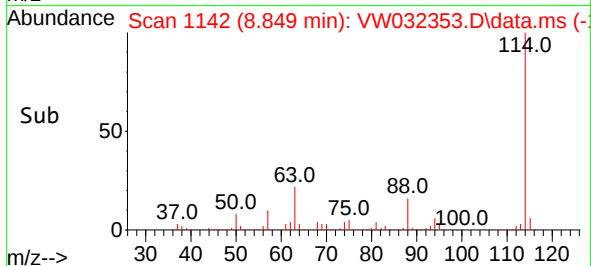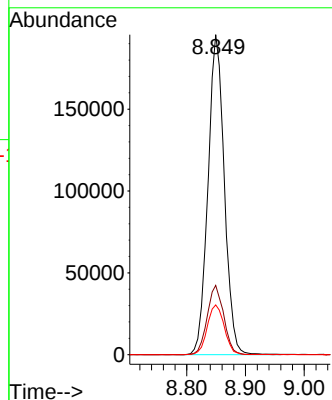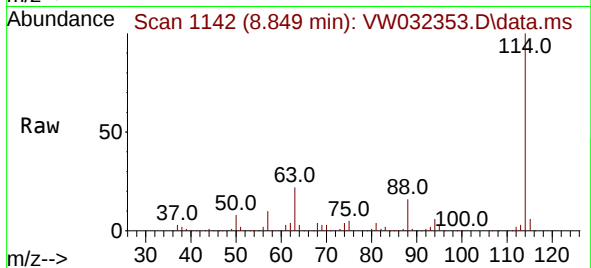

#35

Dibromofluoromethane

Concen: 56.307 ug/l

RT: 7.898 min Scan# 986

Delta R.T. -0.006 min

Lab File: VW032353.D

Acq: 06 Oct 2025 12:37




Tgt Ion:113 Resp: 137927


Ion Ratio Lower Upper

113 100

111 101.5 83.9 125.9

192 15.9 14.6 21.8


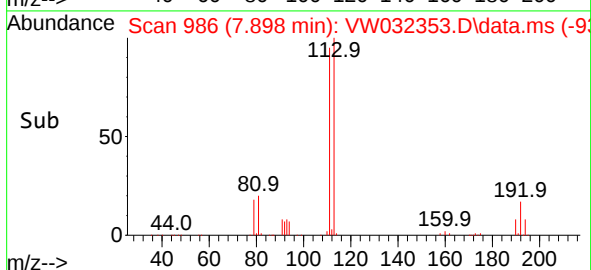
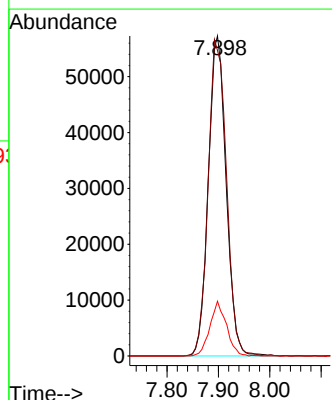
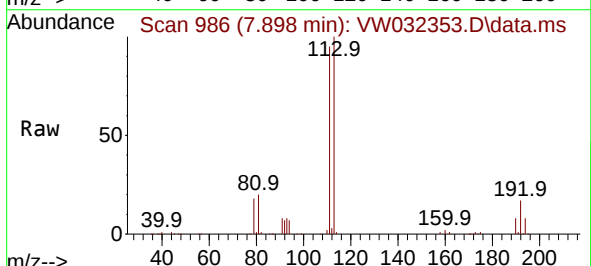


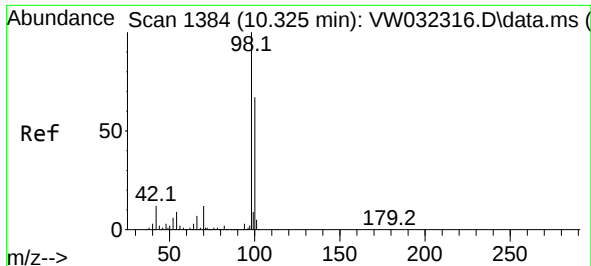

#50
Toluene-d8
Concen: 52.248 ug/l
RT: 10.325 min Scan# 1
Delta R.T. -0.000 min
Lab File: VW032353.D
Acq: 06 Oct 2025 12:37




Instrument :
MSVOA_W
ClientSampleId :
VW1006SBL01


Tgt Ion: 98 Resp: 472361
Ion Ratio Lower Upper
98 100
100 64.3 51.4 77.2

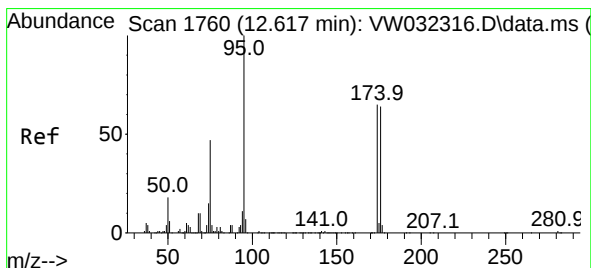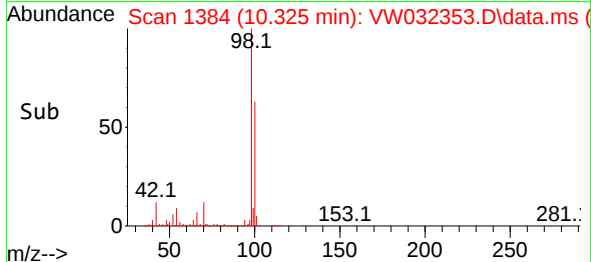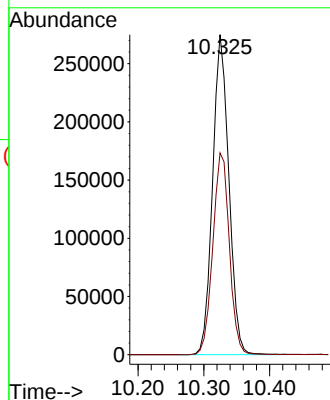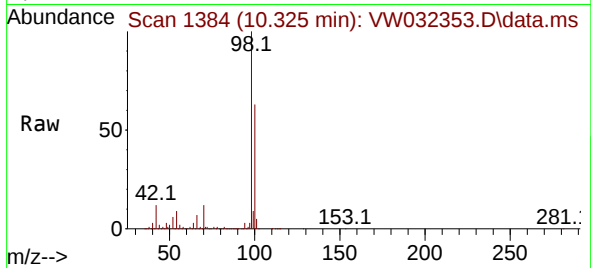

#62
4-Bromofluorobenzene
Concen: 49.592 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. -0.000 min
Lab File: VW032353.D
Acq: 06 Oct 2025 12:37

Tgt Ion: 95 Resp: 169464
Ion Ratio Lower Upper
95 100
174 65.6 0.0 145.6
176 65.6 0.0 140.8


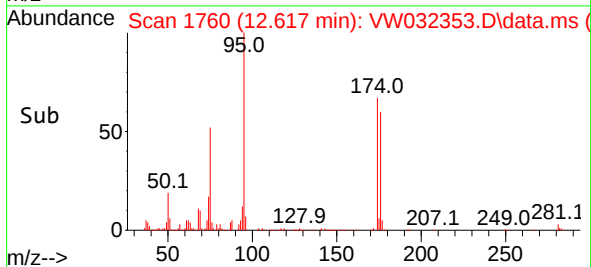
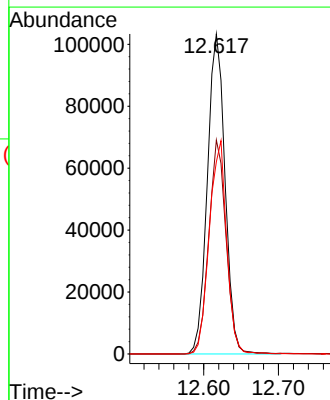
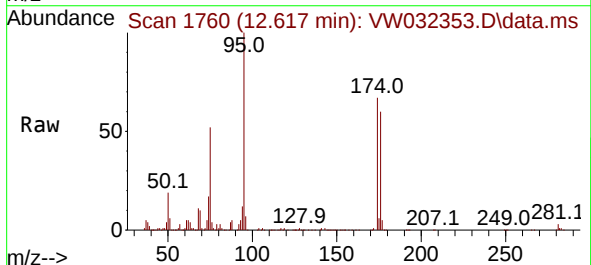


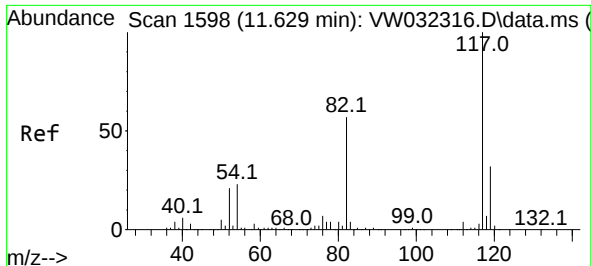

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.629 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW032353.D
Acq: 06 Oct 2025 12:37

Instrument :
MSVOA_W
ClientSampleId :
VW1006SBL01

Tgt Ion:117 Resp: 382025
Ion Ratio Lower Upper
117 100
82 63.7 42.7 64.1
119 33.2 25.2 37.8

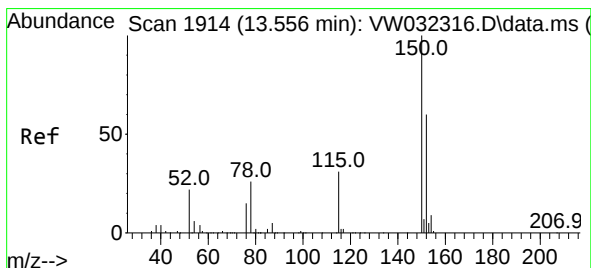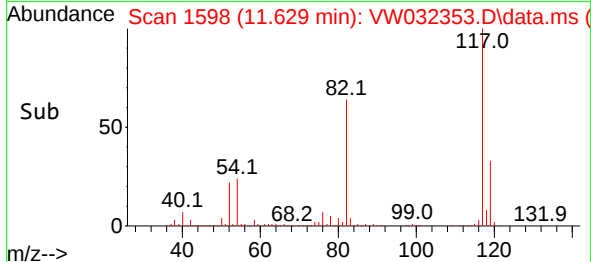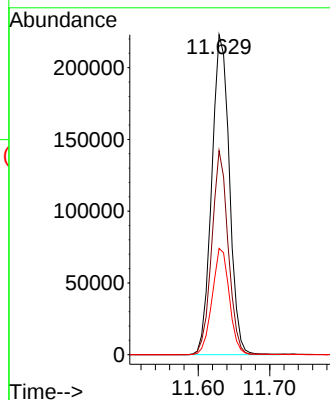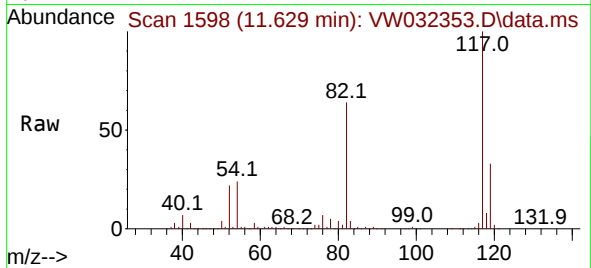

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. -0.000 min
Lab File: VW032353.D
Acq: 06 Oct 2025 12:37

Tgt Ion:152 Resp: 188486
Ion Ratio Lower Upper
152 100
115 62.5 31.8 95.4
150 154.4 0.0 343.0

