

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
 Data File : VW030414.D
 Acq On : 07 Oct 2024 13:36
 Operator : SY/MD
 Sample : VW1007SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 08 01:22:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 08 01:21:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	198510	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	191035	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	85378	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	43255	27.885	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.520%
7) Chloroethane-d5	2.899	69	35061	31.064	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	124.240%
11) 1,1-Dichloroethene-d2	4.021	65	25601	22.609	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.440%
21) 2-Butanone-d5	7.081	46	26562	42.580	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.160%
24) Chloroform-d	7.648	84	136186	25.537	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.160%
26) 1,2-Dichloroethane-d4	8.307	65	70117	25.189	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.760%
32) Benzene-d6	8.276	84	260590	24.338	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.360%
36) 1,2-Dichloropropane-d6	9.276	67	81581	25.333	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.320%
41) Toluene-d8	10.325	98	234583	23.893	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.560%
43) trans-1,3-Dichloroprop...	10.581	79	29627	22.119	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.480%
47) 2-Hexanone-d5	10.922	63	22033	41.434	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.860%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	57955	24.084	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.320%
66) 1,2-Dichlorobenzene-d4	13.849	152	78201	27.588	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.360%
Target Compounds						
39) cis-1,3-Dichloropropene	10.038	75	2196	0.467	ug/L	Qvalue # 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
Data File : VW030414.D
Acq On : 07 Oct 2024 13:36
Operator : SY/MD
Sample : VW1007SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 08 01:22:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 08 01:21:40 2024
Response via : Initial Calibration

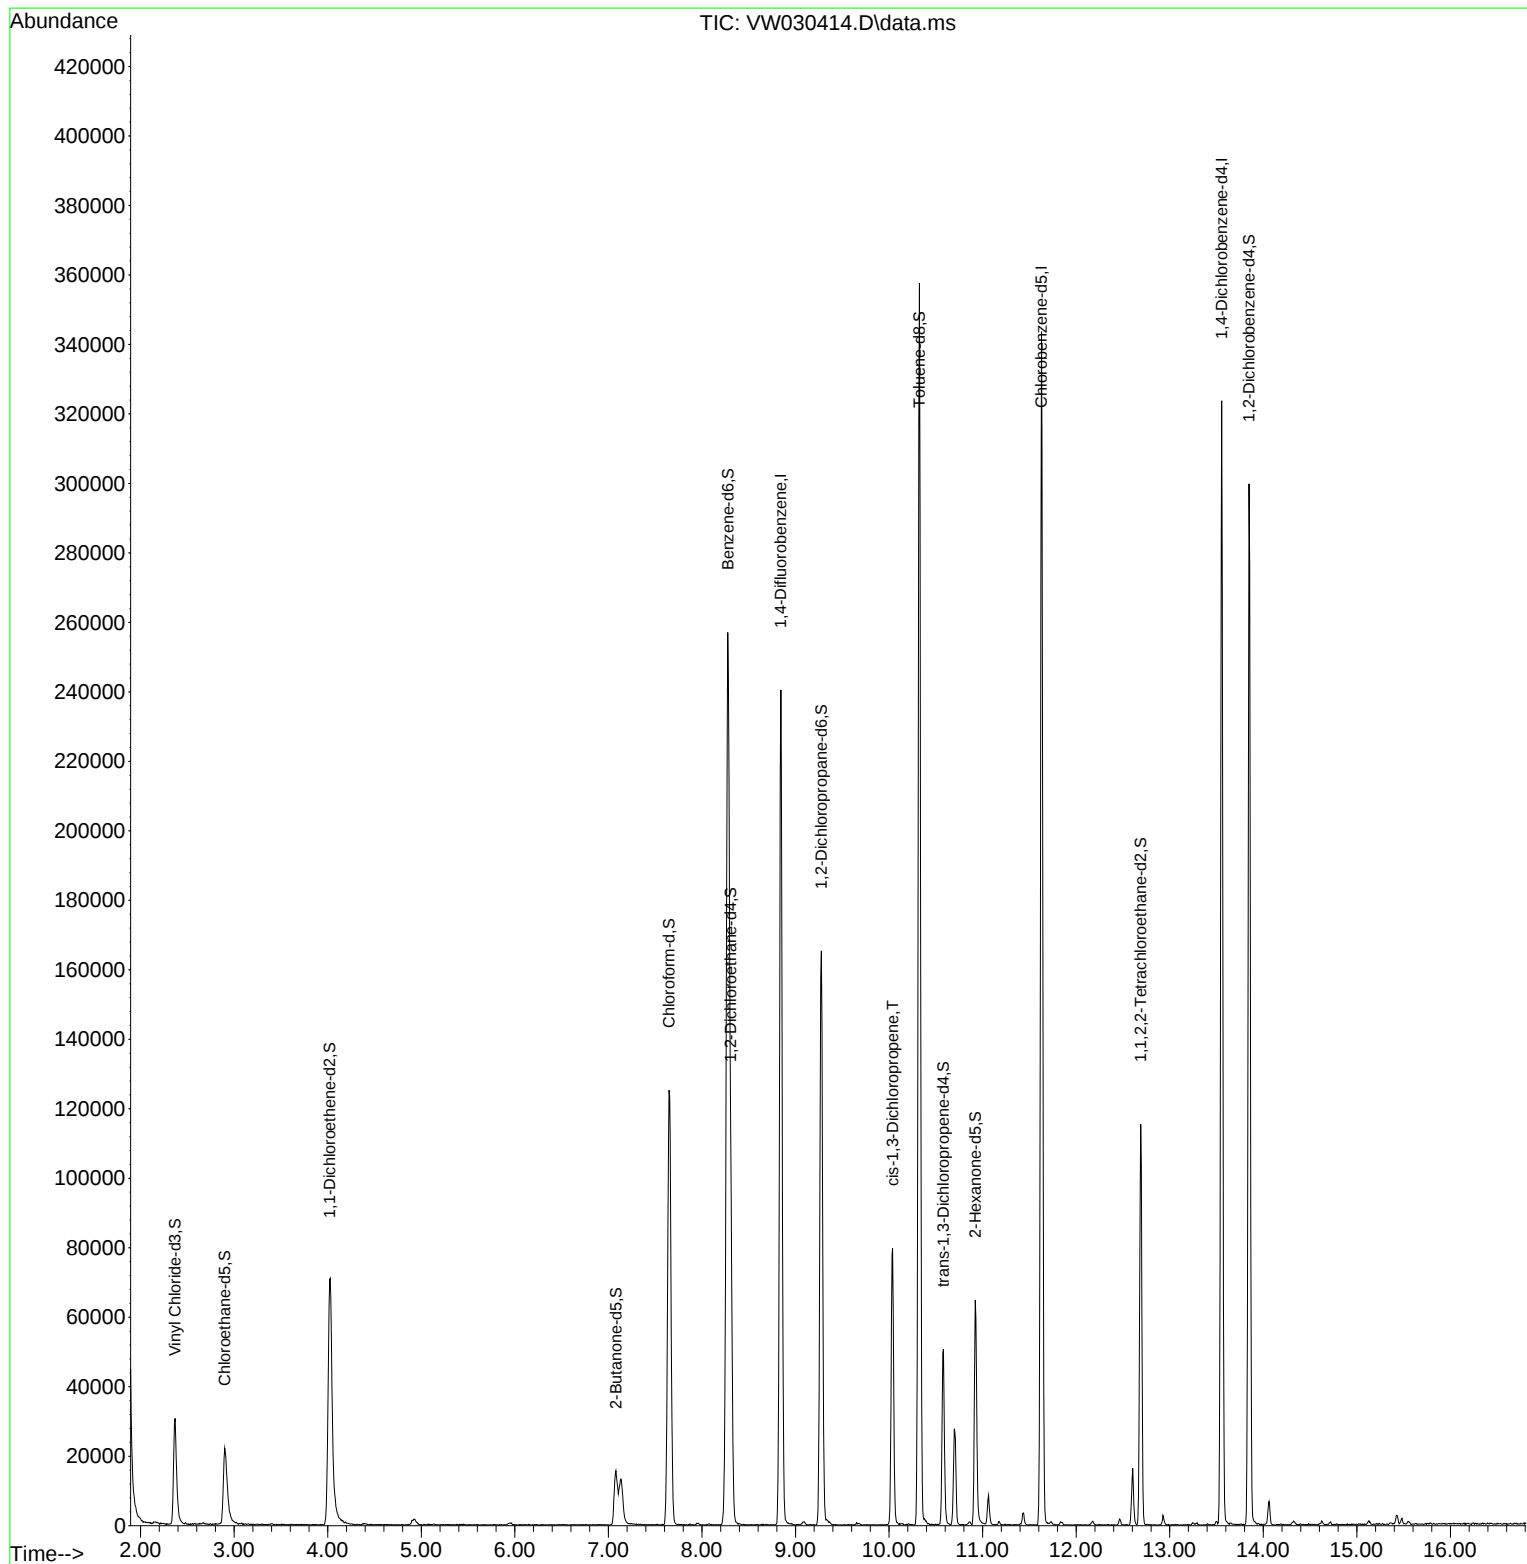

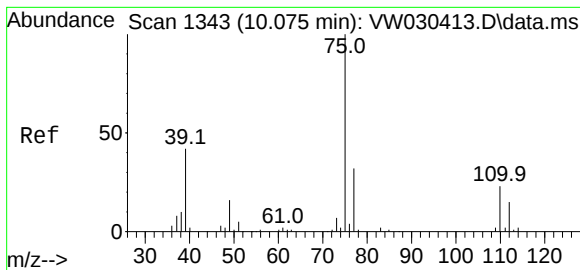

#39
 cis-1,3-Dichloropropene
 Concen: 0.467 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW030414.D
 Acq: 07 Oct 2024 13:36

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 2196
 Ion Ratio Lower Upper
 75 100
 77 52.2 22.0 40.8#

