

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
 Data File : VW030434.D
 Acq On : 07 Oct 2024 21:50
 Operator : SY/MD
 Sample : P4329-04
 Misc : 5.34g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 08 01:31:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 08 01:21:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	56279	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	65923	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	23528	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	0.000	65	0	0.000	ug/L	
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.000%#
7) Chloroethane-d5	0.000	69	0	0.000	ug/L	
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.000%#
11) 1,1-Dichloroethene-d2	0.000	65	0	0.000	ug/L	
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.000%#
21) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
24) Chloroform-d	0.000	84	0	0.000	ug/L	
Spiked Amount	25.000	Range	40 - 150	Recovery	=	0.000%#
26) 1,2-Dichloroethane-d4	8.319	65	63	0.080	ug/L	0.01
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.320%#
32) Benzene-d6	8.288	84	164	0.044	ug/L	0.01
Spiked Amount	25.000	Range	20 - 135	Recovery	=	0.160%#
36) 1,2-Dichloropropane-d6	0.000	67	0	0.000	ug/L	
Spiked Amount	25.000	Range	70 - 120	Recovery	=	0.000%#
41) Toluene-d8	10.337	98	280	0.083	ug/L	0.01
Spiked Amount	25.000	Range	30 - 130	Recovery	=	0.320%#
43) trans-1,3-Dichloroprop...	10.575	79	51	0.110	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	0.440%#
47) 2-Hexanone-d5	0.000	63	0	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
56) 1,1,2,2-Tetrachloroeth...	12.696	84	125	0.151	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	0.600%#
66) 1,2-Dichlorobenzene-d4	13.860	152	461	0.590	ug/L	0.01
Spiked Amount	25.000	Range	75 - 120	Recovery	=	2.360%#
Target Compounds						Qvalue
13) Acetone	4.131	43	797	4.248	ug/L	62
34) Trichloroethene	8.843	95	1786	1.672	ug/L #	4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
Data File : VW030434.D
Acq On : 07 Oct 2024 21:50
Operator : SY/MD
Sample : P4329-04
Misc : 5.34g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 08 01:31:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 08 01:21:40 2024
Response via : Initial Calibration




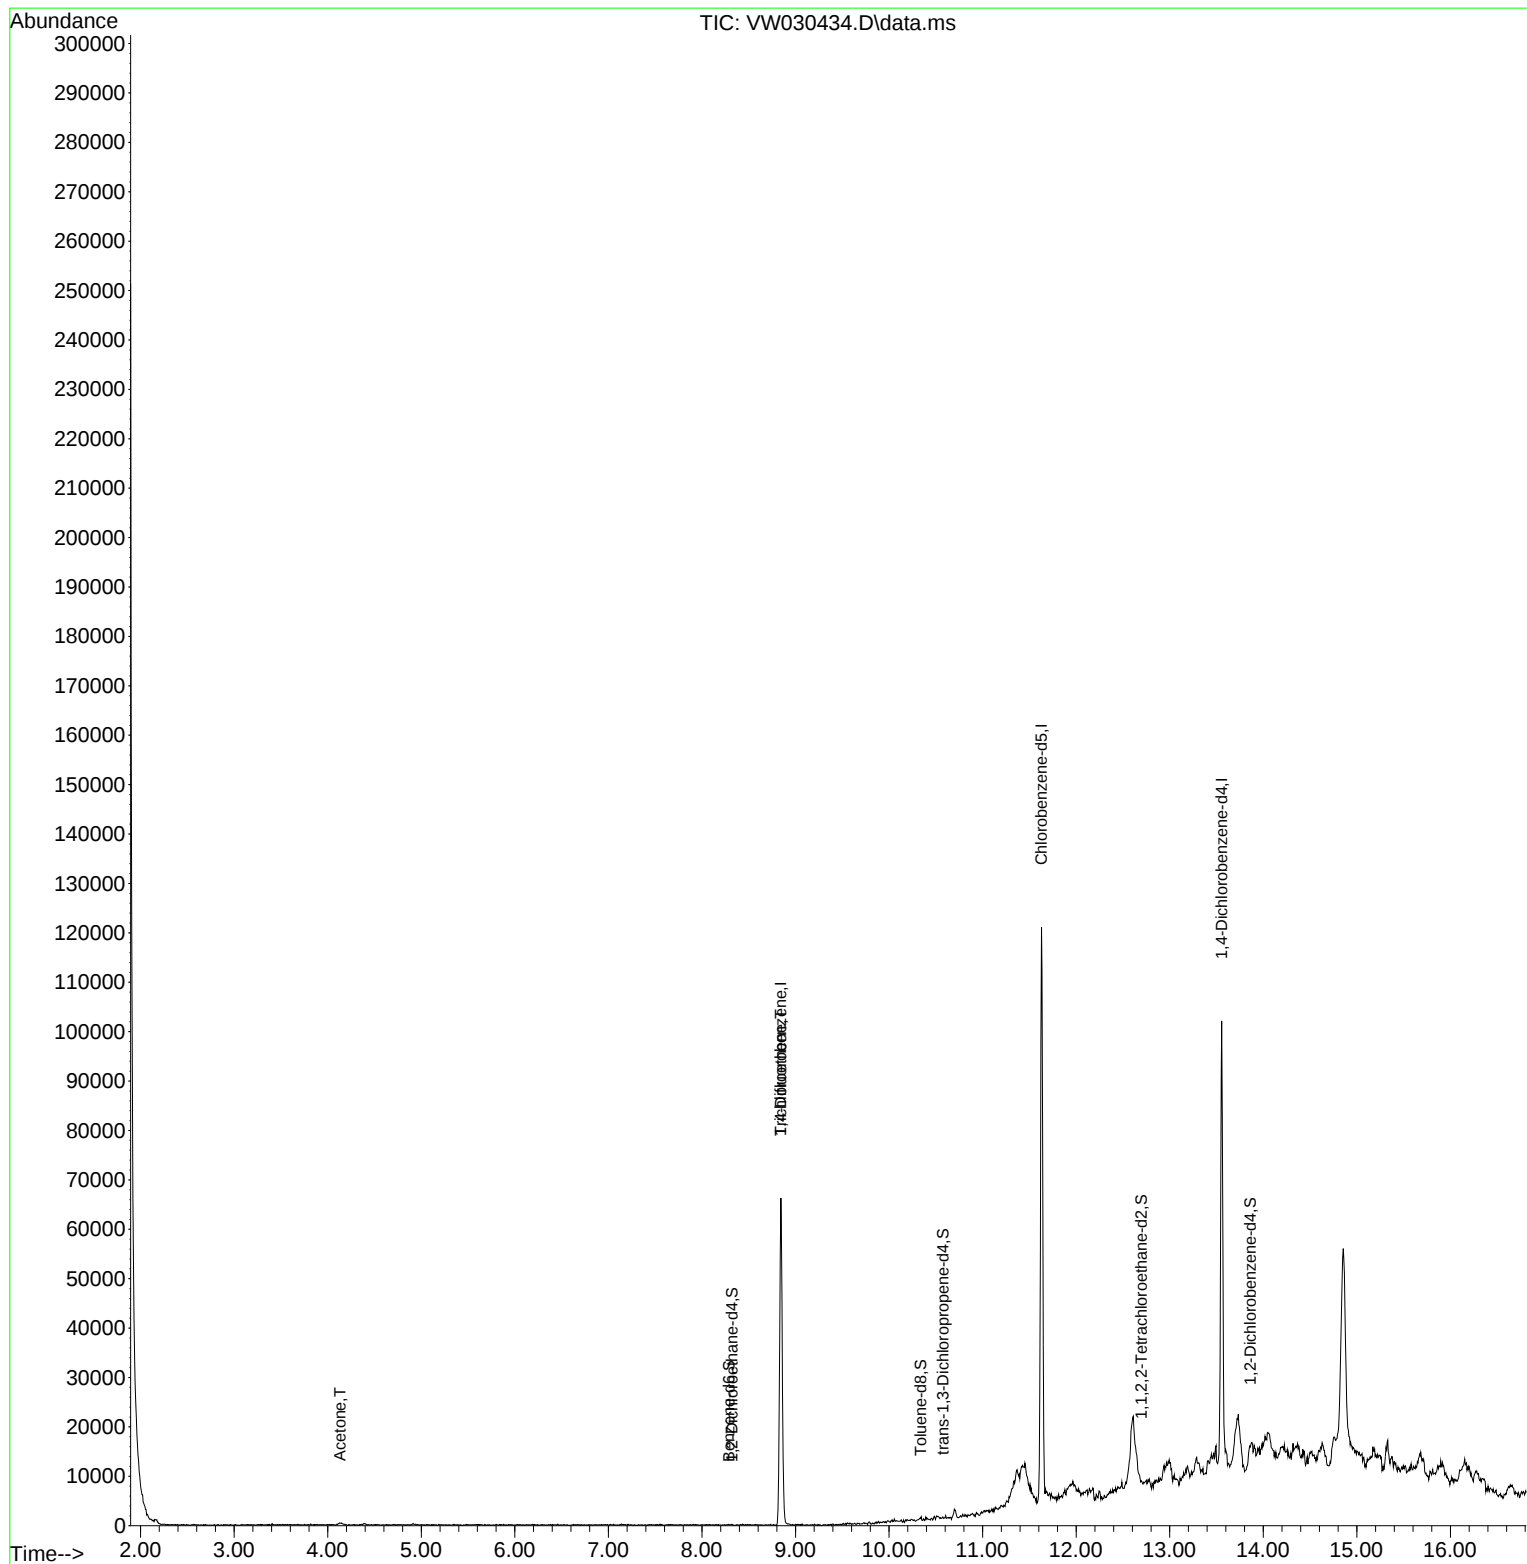


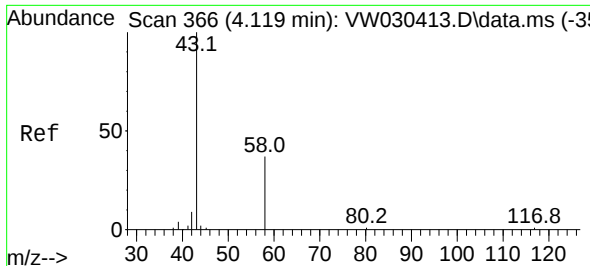

#13
Acetone
Concen: 4.248 ug/L
RT: 4.131 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW030434.D
Acq: 07 Oct 2024 21:50

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 43 Resp: 797
Ion Ratio Lower Upper
43 100
58 10.5 0.0 64.0

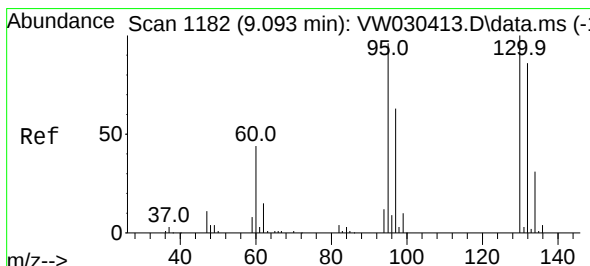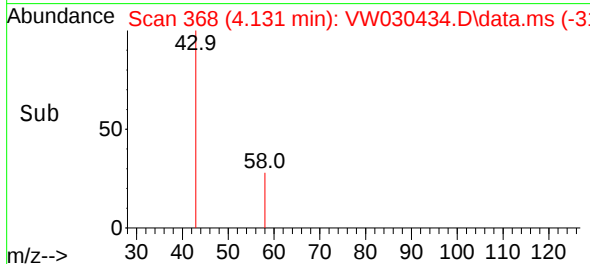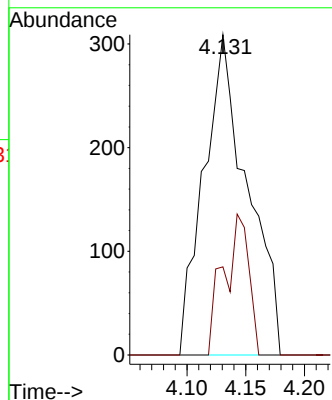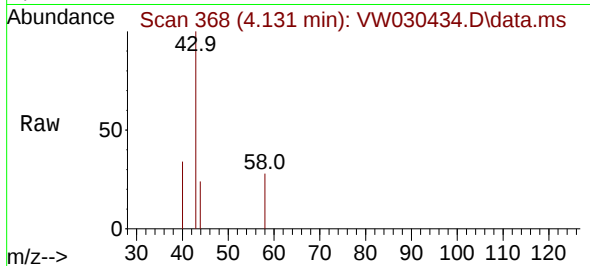

#34
Trichloroethene
Concen: 1.672 ug/L
RT: 8.843 min Scan# 1141
Delta R.T. -0.250 min
Lab File: VW030434.D
Acq: 07 Oct 2024 21:50

Tgt Ion: 95 Resp: 1786
Ion Ratio Lower Upper
95 100
97 0.0 47.5 88.1#
132 0.0 66.7 123.9#
130 0.0 72.4 134.5#

