

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
 Data File : VW030424.D
 Acq On : 07 Oct 2024 17:51
 Operator : SY/MD
 Sample : P4284-14
 Misc : 4.79g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EW4

Quant Time: Oct 08 01:28:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 08 01:21:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	341236	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	279593	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	127656	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	45867	17.201	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.800%
7) Chloroethane-d5	2.899	69	33267	17.147	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.600%
11) 1,1-Dichloroethene-d2	4.027	65	35057	18.011	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.040%
21) 2-Butanone-d5	7.075	46	30303	28.259	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.520%
24) Chloroform-d	7.648	84	187399	20.442	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.760%
26) 1,2-Dichloroethane-d4	8.307	65	92859	19.406	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	77.640%
32) Benzene-d6	8.276	84	382288	24.396	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.600%
36) 1,2-Dichloropropane-d6	9.276	67	110967	23.544	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.160%
41) Toluene-d8	10.325	98	352971	24.564	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.240%
43) trans-1,3-Dichloroprop...	10.581	79	42605	21.733	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.920%
47) 2-Hexanone-d5	10.922	63	26349	33.856	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.720%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	79923	22.694	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	100982	23.826	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.320%
Target Compounds						
13) Acetone	4.119	43	7092	6.235	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
Data File : VW030424.D
Acq On : 07 Oct 2024 17:51
Operator : SY/MD
Sample : P4284-14
Misc : 4.79g/10mL/MSVOA_W/SOIL/B
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EW4

Quant Time: Oct 08 01:28:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 08 01:21:40 2024
Response via : Initial Calibration

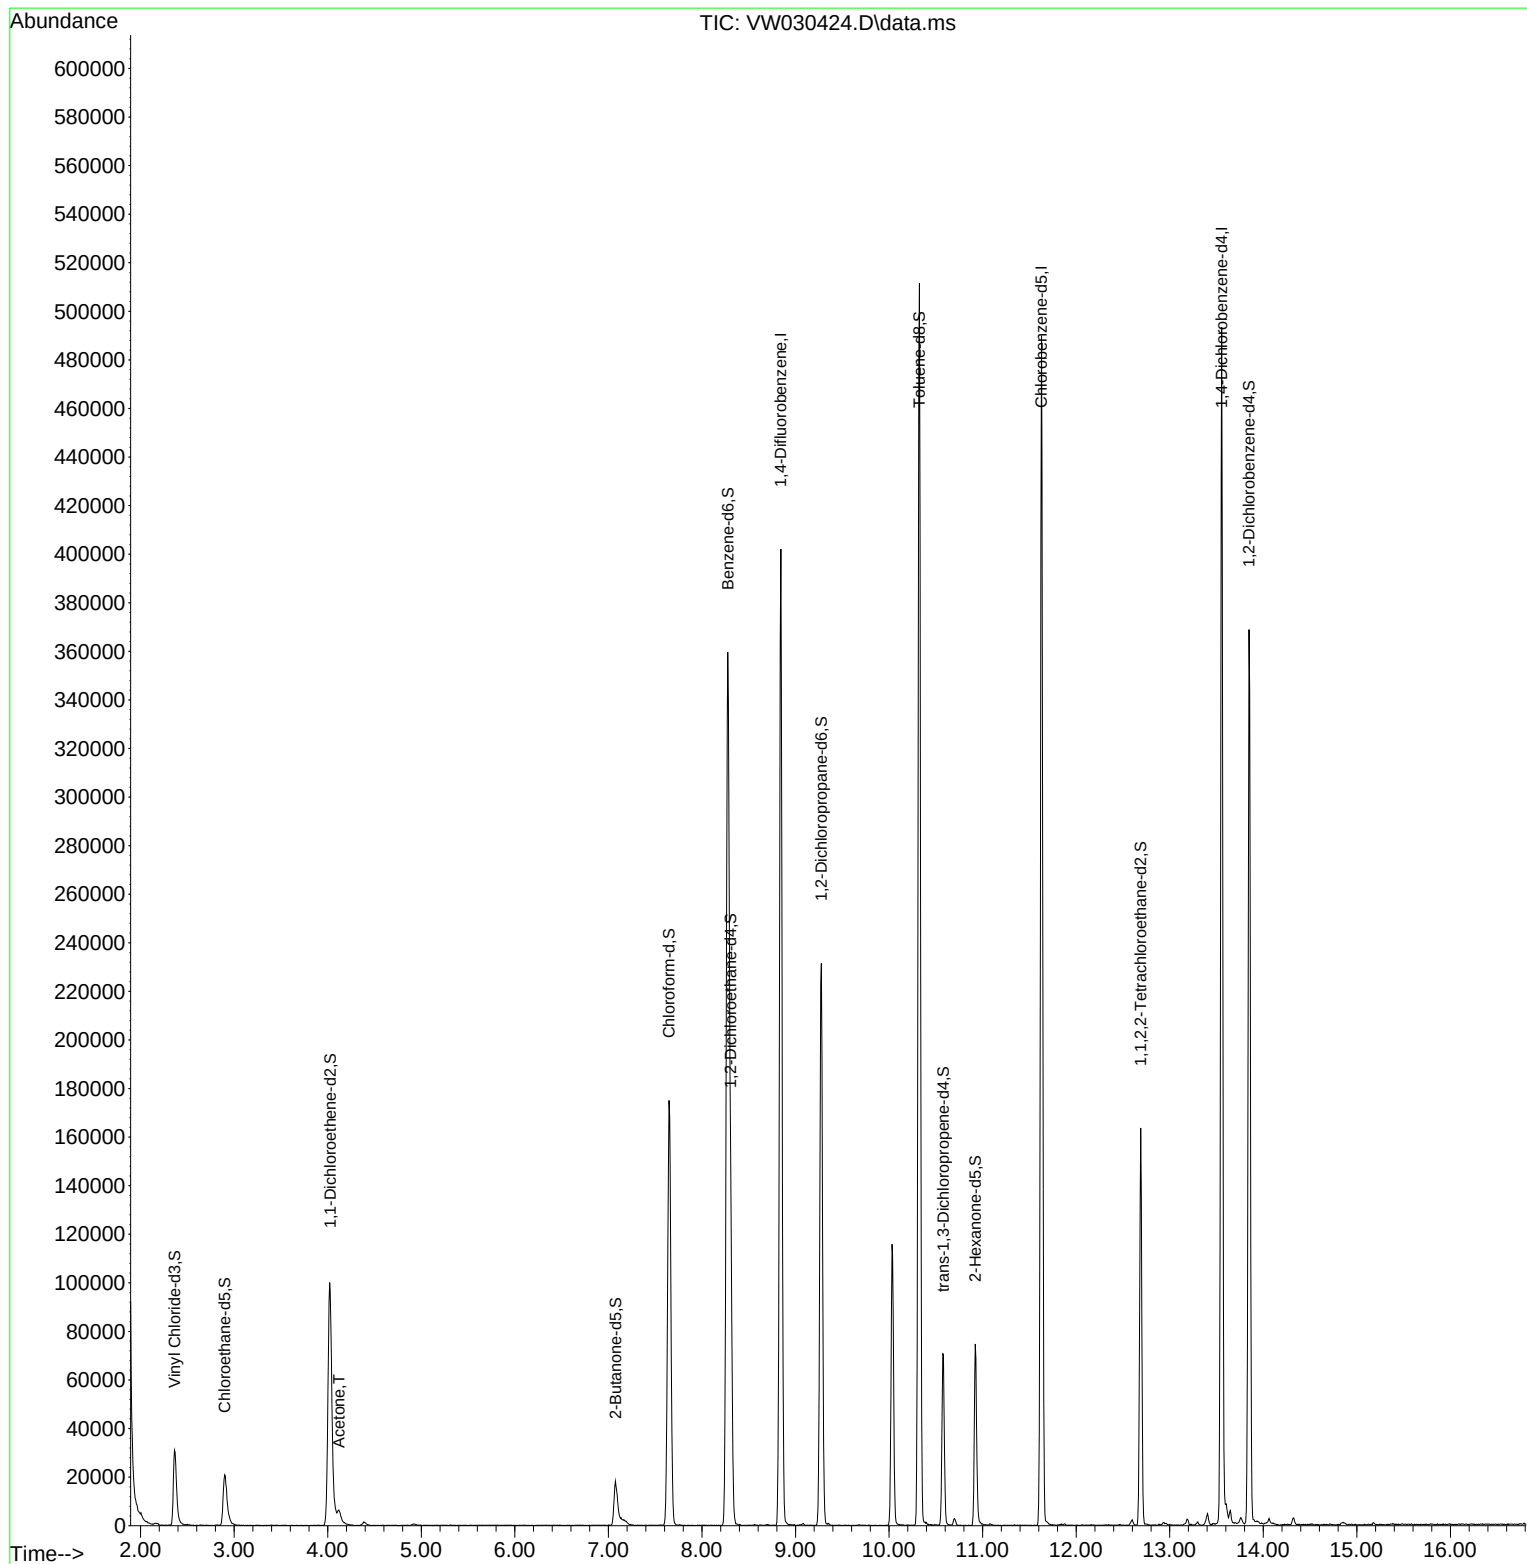

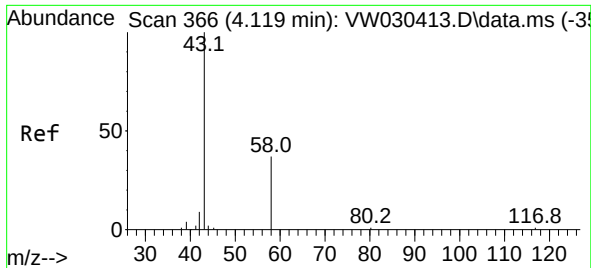

#13
 Acetone
 Concen: 6.235 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW030424.D
 Acq: 07 Oct 2024 17:51

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EW4

Tgt Ion: 43 Resp: 7092
 Ion Ratio Lower Upper
 43 100
 58 32.9 0.0 64.0

