

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
 Data File : VW030428.D
 Acq On : 07 Oct 2024 19:27
 Operator : SY/MD
 Sample : P4284-18RE
 Misc : 5.63g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EZ3RE

Quant Time: Oct 08 01:29:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 08 01:21:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	211033	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	130540	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	35570	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	36370	22.055	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.200%		
7) Chloroethane-d5	2.899	69	25806	21.508	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.040%		
11) 1,1-Dichloroethene-d2	4.021	65	22364	18.579	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	74.320%		
21) 2-Butanone-d5	7.081	46	7219	10.886	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	21.780%		
24) Chloroform-d	7.648	84	129412	22.826	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	91.320%		
26) 1,2-Dichloroethane-d4	8.307	65	67870	22.935	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.760%		
32) Benzene-d6	8.270	84	234198	32.010	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	128.040%		
36) 1,2-Dichloropropane-d6	9.276	67	68128	30.960	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	123.840%#		
41) Toluene-d8	10.325	98	177363	26.437	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	105.760%		
43) trans-1,3-Dichloroprop...	10.581	79	5426	5.928	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	23.720%#		
47) 2-Hexanone-d5	10.928	63	3003	8.264	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	16.520%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	42595	25.904	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.600%		
66) 1,2-Dichlorobenzene-d4	13.848	152	27837	23.571	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.280%		
Target Compounds					Qvalue	
13) Acetone	4.124	43	4859	6.907	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
Data File : VW030428.D
Acq On : 07 Oct 2024 19:27
Operator : SY/MD
Sample : P4284-18RE
Misc : 5.63g/10mL/MSVOA_W/SOIL/B
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EZ3RE

Quant Time: Oct 08 01:29:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 08 01:21:40 2024
Response via : Initial Calibration

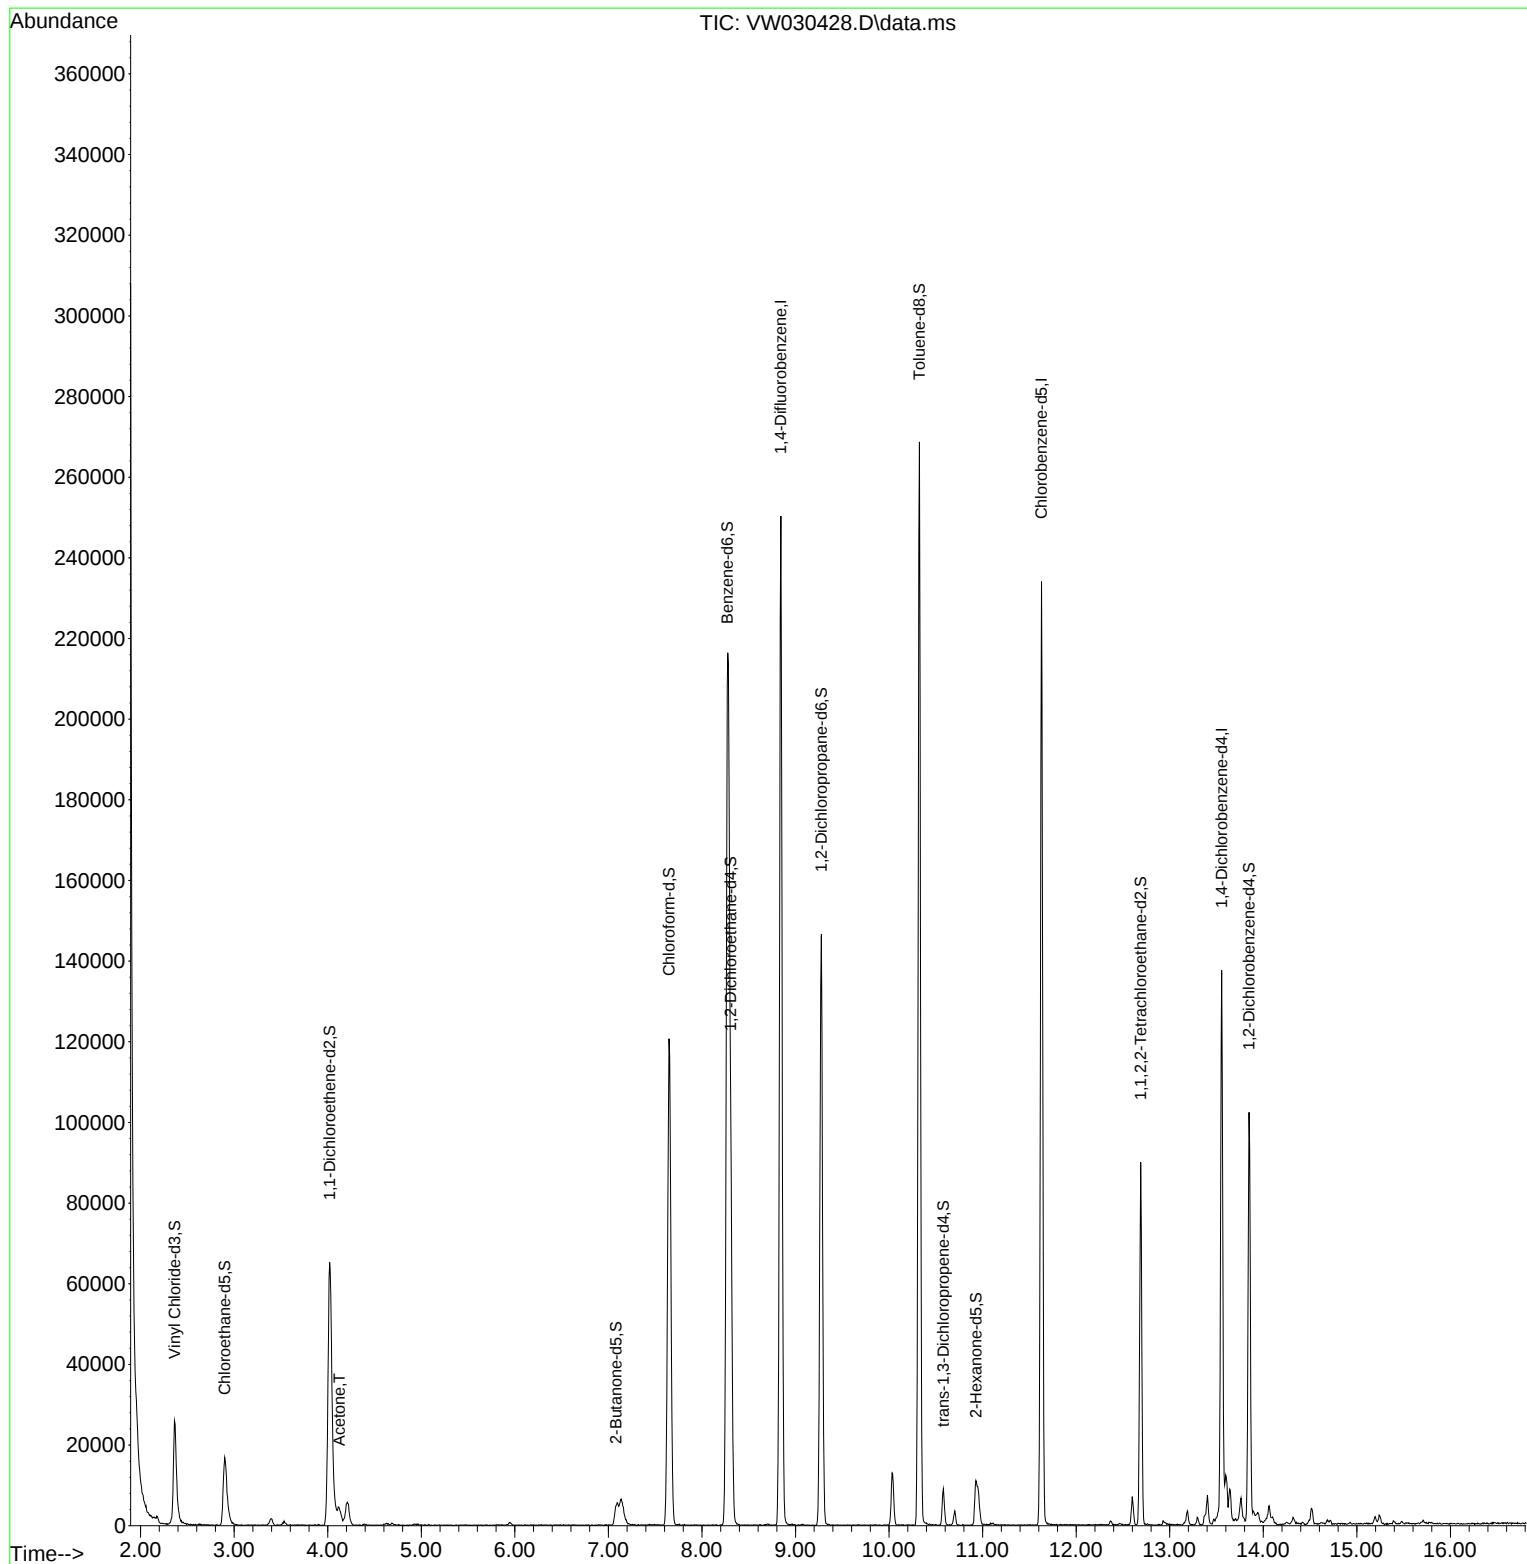

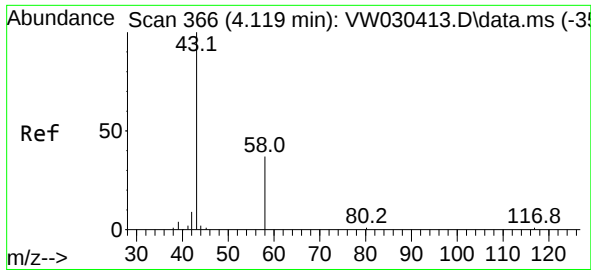

#13
 Acetone
 Concen: 6.907 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW030428.D
 Acq: 07 Oct 2024 19:27

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EZ3RE

Tgt Ion: 43 Resp: 4859
 Ion Ratio Lower Upper
 43 100
 58 31.9 0.0 64.0

