

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
 Data File : VW030434.D
 Acq On : 07 Oct 2024 21:50
 Operator : SY/MD
 Sample : P4329-04
 Misc : 5.34g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EG5

Quant Time: Oct 08 01:31:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 08 01:21:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	56279	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	65923	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	23528	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	0.000	65	0	0.000	ug/L	
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.000%#
7) Chloroethane-d5	0.000	69	0	0.000	ug/L	
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.000%#
11) 1,1-Dichloroethene-d2	0.000	65	0	0.000	ug/L	
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.000%#
21) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
24) Chloroform-d	0.000	84	0	0.000	ug/L	
Spiked Amount	25.000	Range	40 - 150	Recovery	=	0.000%#
26) 1,2-Dichloroethane-d4	0.000	65	0d	0.000	ug/L	
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.000%#
32) Benzene-d6	0.000	84	0d	0.000	ug/L	
Spiked Amount	25.000	Range	20 - 135	Recovery	=	0.000%#
36) 1,2-Dichloropropane-d6	0.000	67	0	0.000	ug/L	
Spiked Amount	25.000	Range	70 - 120	Recovery	=	0.000%#
41) Toluene-d8	0.000	98	0d	0.000	ug/L	
Spiked Amount	25.000	Range	30 - 130	Recovery	=	0.000%#
43) trans-1,3-Dichloroprop...	0.000	79	0d	0.000	ug/L	
Spiked Amount	25.000	Range	30 - 135	Recovery	=	0.000%#
47) 2-Hexanone-d5	0.000	63	0	0.000	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.000%#
56) 1,1,2,2-Tetrachloroeth...	0.000	84	0d	0.000	ug/L	
Spiked Amount	25.000	Range	45 - 120	Recovery	=	0.000%#
66) 1,2-Dichlorobenzene-d4	0.000	152	0d	0.000	ug/L	
Spiked Amount	25.000	Range	75 - 120	Recovery	=	0.000%#
Target Compounds						Qvalue
13) Acetone	4.131	43	797	4.248	ug/L	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
Data File : VW030434.D
Acq On : 07 Oct 2024 21:50
Operator : SY/MD
Sample : P4329-04
Misc : 5.34g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EG5

Quant Time: Oct 08 01:31:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 08 01:21:40 2024
Response via : Initial Calibration

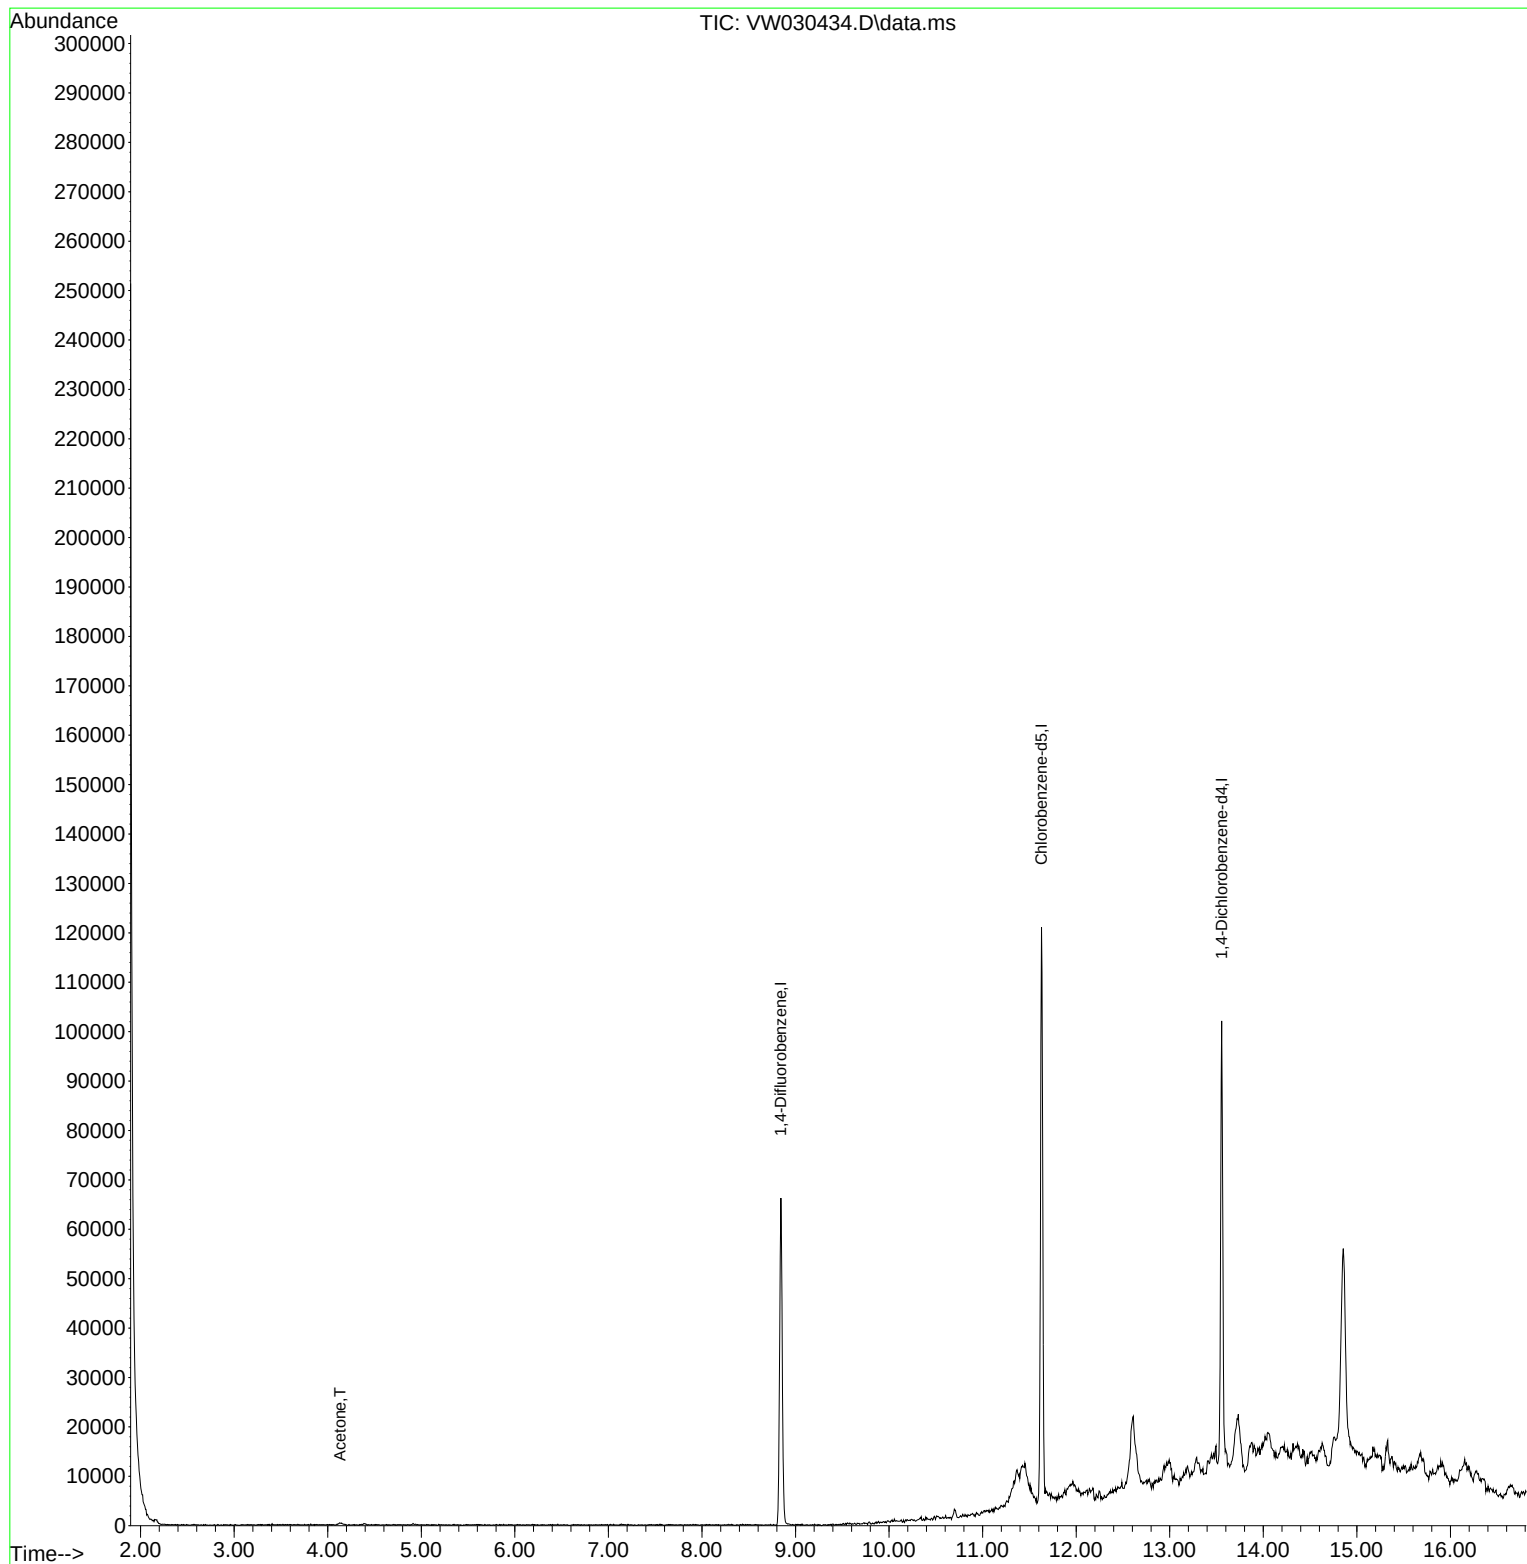

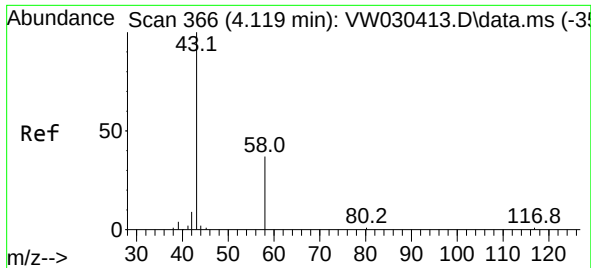

#13
 Acetone
 Concen: 4.248 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW030434.D
 Acq: 07 Oct 2024 21:50

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EG5

Tgt Ion: 43 Resp: 797
 Ion Ratio Lower Upper
 43 100
 58 10.5 0.0 64.0

