
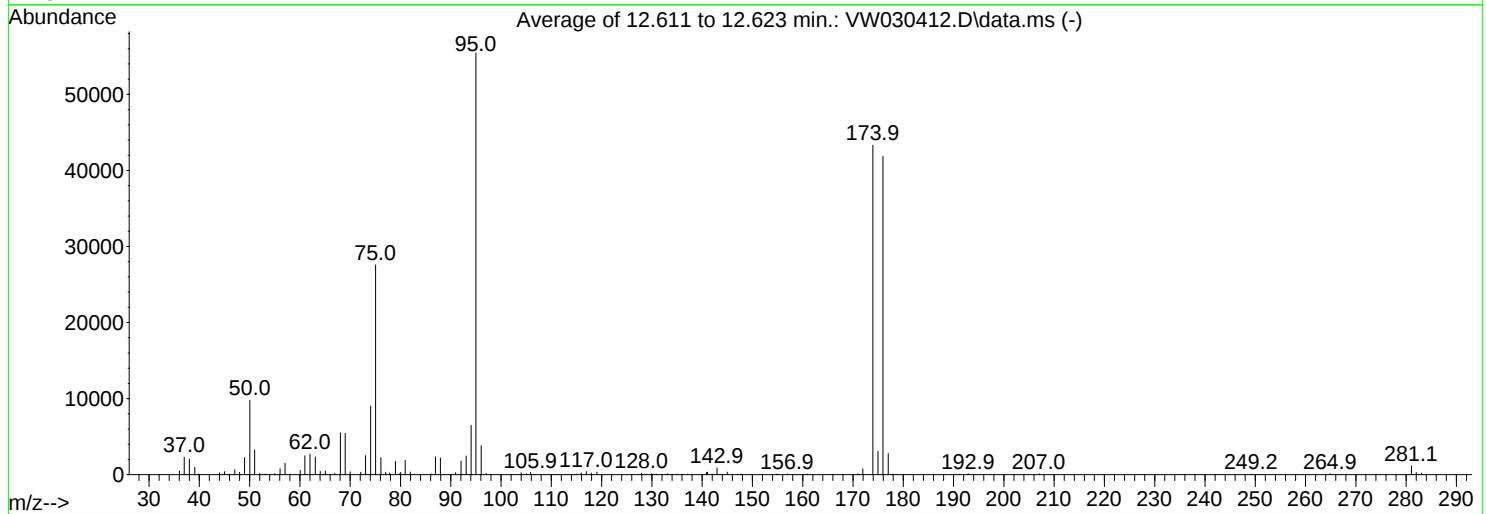


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100724\
Data File : VW030412.D
Acq On : 07 Oct 2024 11:02
Operator : SY/MD
Sample : BFB570
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB570

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Title : SFAM01.0
Last Update : Tue Oct 08 01:21:40 2024

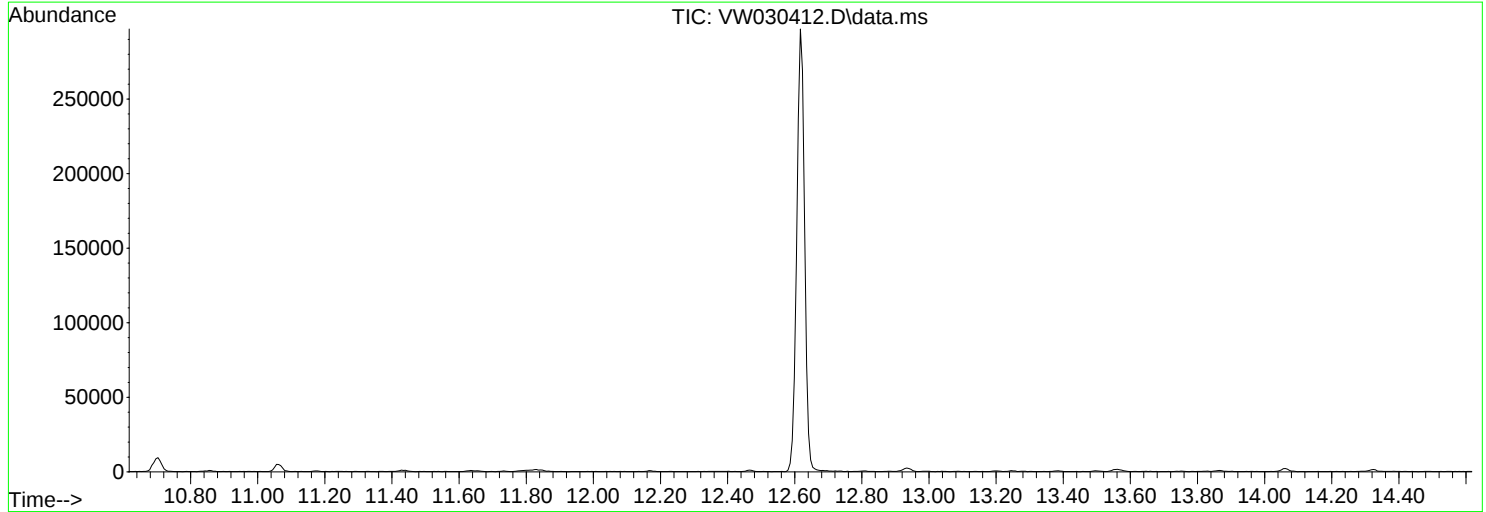

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	9784	PASS
75	95	30	80	49.7	27576	PASS
95	95	100	100	100.0	55464	PASS
96	95	5	9	6.9	3811	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.1	43312	PASS
175	174	5	9	7.1	3065	PASS
176	174	95	101	96.6	41851	PASS
177	176	5	9	6.7	2784	PASS

Scan 1752 (12.568 min): VW030412.D\data.ms
BFB570

m/z	Abundance
39.90	107.0
43.90	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB570

m/z	Abundance
36.00	469.0
37.00	2227.0
38.00	1991.0
39.10	939.0
39.90	225.0
44.00	359.0
45.00	395.0
45.90	101.0
47.10	523.0
48.10	200.0
49.00	2190.0
50.10	9392.0
51.00	3089.0
52.00	165.0
53.10	54.0
55.00	180.0
56.10	686.0
57.10	1276.0
58.00	83.0
60.10	467.0
61.00	2413.0
62.00	2623.0
63.00	2071.0
64.10	517.0
65.10	611.0
66.90	103.0
68.00	5179.0
69.00	5232.0
70.00	364.0
72.20	266.0
73.00	2314.0
74.00	8429.0
75.00	24576.0
76.10	2271.0
77.10	290.0
77.90	217.0
79.00	1775.0
79.90	476.0
81.00	1942.0
82.00	398.0
86.10	91.0
86.90	2220.0
88.00	1836.0
90.90	309.0
92.10	1706.0
93.00	2321.0
94.10	5862.0
95.00	51872.0
96.00	3689.0
97.00	100.0
103.90	247.0
105.00	68.0
105.90	292.0
111.00	71.0
112.90	54.0
114.70	65.0
115.90	192.0
116.90	434.0
118.00	197.0
119.10	283.0
125.00	71.0
128.00	165.0
129.00	69.0
129.90	193.0
130.90	54.0
133.20	243.0
135.10	129.0
140.90	375.0
143.00	697.0
145.00	255.0
147.70	117.0
150.10	56.0
154.00	52.0
155.20	59.0
156.90	51.0
161.00	79.0
171.00	199.0
171.90	593.0
173.90	34888.0
175.00	2822.0
176.00	31368.0
177.00	2094.0
178.90	67.0
191.10	93.0
192.90	169.0
207.10	192.0
249.20	87.0
250.90	51.0
264.90	221.0
266.00	116.0
266.90	78.0
281.10	1560.0

Instrument :
MSVOA_W
ClientSampleId :
BFB570

282.00463.0

283.10291.0

Instrument :
MSVOA_W
ClientSampleId :
BFB570

m/z	Abundance
36.10	441.0
37.00	2557.0
38.00	2182.0
39.10	1093.0
40.00	171.0
44.00	302.0
45.00	535.0
46.00	52.0
46.90	664.0
48.00	384.0
49.00	2518.0
50.10	11194.0
51.00	4060.0
52.00	158.0
53.00	118.0
55.00	185.0
56.00	963.0
57.00	1804.0
58.00	91.0
60.00	662.0
61.00	2744.0
62.00	3002.0
63.10	2717.0
64.00	430.0
65.00	589.0
66.00	69.0
66.90	171.0
68.10	6003.0
69.00	5922.0
70.00	388.0
72.00	367.0
73.10	2765.0
74.10	10041.0
75.10	31328.0
76.10	2404.0
77.00	336.0
77.80	173.0
79.00	1875.0
80.10	499.0
80.90	2011.0
81.90	353.0
86.10	153.0
87.00	2455.0
87.90	2693.0
90.90	183.0
92.00	1958.0
93.10	2608.0
94.10	7424.0
95.00	59080.0
96.10	4233.0
97.00	165.0
104.00	276.0
105.10	156.0
105.90	369.0
110.00	75.0
111.00	65.0
112.90	71.0
114.90	81.0
116.00	275.0
116.90	352.0
117.90	252.0
118.90	405.0
127.90	188.0
128.90	95.0
129.90	210.0
130.80	107.0
133.00	129.0
134.80	88.0
135.20	63.0
137.10	124.0
140.80	468.0
141.10	471.0
142.00	90.0
142.90	1080.0
143.80	83.0
145.00	466.0
146.00	91.0
147.90	166.0
154.00	54.0
155.00	165.0
157.00	127.0
161.00	71.0
171.20	183.0
172.00	1074.0
173.90	45672.0
174.90	3480.0
175.90	48688.0
177.00	3216.0
178.00	121.0
178.90	52.0
191.10	106.0
192.90	193.0

Instrument :
MSVOA_W
ClientSampleId :
BFB570

206.90	112.0
249.20	62.0
264.90	145.0
281.10	1314.0
282.00	308.0
283.00	233.0

Instrument :
MSVOA_W
ClientSampleId :
BFB570

m/z	Abundance
36.00	466.0
37.00	2070.0
38.00	1978.0
39.10	841.0
39.90	167.0
44.10	268.0
45.00	246.0
45.90	69.0
47.10	801.0
47.90	294.0
49.00	1969.0
50.00	8765.0
51.00	2591.0
52.00	162.0
53.10	82.0
54.20	80.0
55.20	106.0
56.00	670.0
57.00	1375.0
60.00	596.0
61.00	2279.0
62.00	2497.0
63.10	2199.0
64.00	403.0
65.00	350.0
66.00	76.0
67.00	159.0
68.00	5300.0
69.00	5217.0
70.00	416.0
72.10	322.0
73.00	2422.0
74.10	8580.0
75.10	26824.0
76.10	1996.0
77.10	318.0
77.80	331.0
79.00	1560.0
80.00	382.0
81.00	1646.0
82.00	316.0
86.10	74.0
87.00	2367.0
88.00	2013.0
91.00	246.0
92.00	1720.0
93.10	2457.0
94.00	6237.0
95.00	55440.0
96.10	3510.0
97.10	155.0
104.10	253.0
105.00	110.0
105.90	200.0
106.80	72.0
110.00	71.0
115.00	76.0
115.90	247.0
117.00	387.0
118.00	213.0
119.10	344.0
127.90	206.0
129.00	58.0
130.10	131.0
130.80	76.0
132.90	74.0
134.80	54.0
136.90	53.0
141.00	524.0
142.00	80.0
143.00	850.0
145.00	262.0
146.10	89.0
147.00	64.0
147.70	71.0
149.90	58.0
154.80	172.0
157.00	172.0
158.80	53.0
160.90	105.0
170.90	142.0
171.90	611.0
174.00	49376.0
175.00	2893.0
176.00	45496.0
177.00	3042.0
177.90	56.0
206.90	78.0
280.90	620.0
282.00	131.0
283.00	101.0

Instrument :
MSVOA_W
ClientSampleId :
BFB570