

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
 Data File : VW030443.D
 Acq On : 08 Oct 2024 13:24
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 09 01:18:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 09 01:13:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	127400	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	121211	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	60618	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	19576	19.664	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.640%
7) Chloroethane-d5	2.905	69	15180	20.957	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.840%
11) 1,1-Dichloroethene-d2	4.021	65	15460	21.274	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	85.080%
21) 2-Butanone-d5	7.081	46	15176	37.907	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.820%
24) Chloroform-d	7.654	84	76231	22.273	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.080%
26) 1,2-Dichloroethane-d4	8.307	65	41811	23.404	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.600%
32) Benzene-d6	8.276	84	148804	21.904	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.600%
36) 1,2-Dichloropropane-d6	9.276	67	42139	20.623	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.480%
41) Toluene-d8	10.325	98	141261	22.676	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.720%
43) trans-1,3-Dichloroprop...	10.581	79	18815	22.138	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.560%
47) 2-Hexanone-d5	10.922	63	14718	43.622	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.240%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	36428	23.859	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.440%
66) 1,2-Dichlorobenzene-d4	13.849	152	55859	27.755	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.000%
Target Compounds			Qvalue			
37) 1,2-Dichloropropane	9.276	63	5102	2.619	ug/L #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
Data File : VW030443.D
Acq On : 08 Oct 2024 13:24
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 09 01:18:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 09 01:13:46 2024
Response via : Initial Calibration

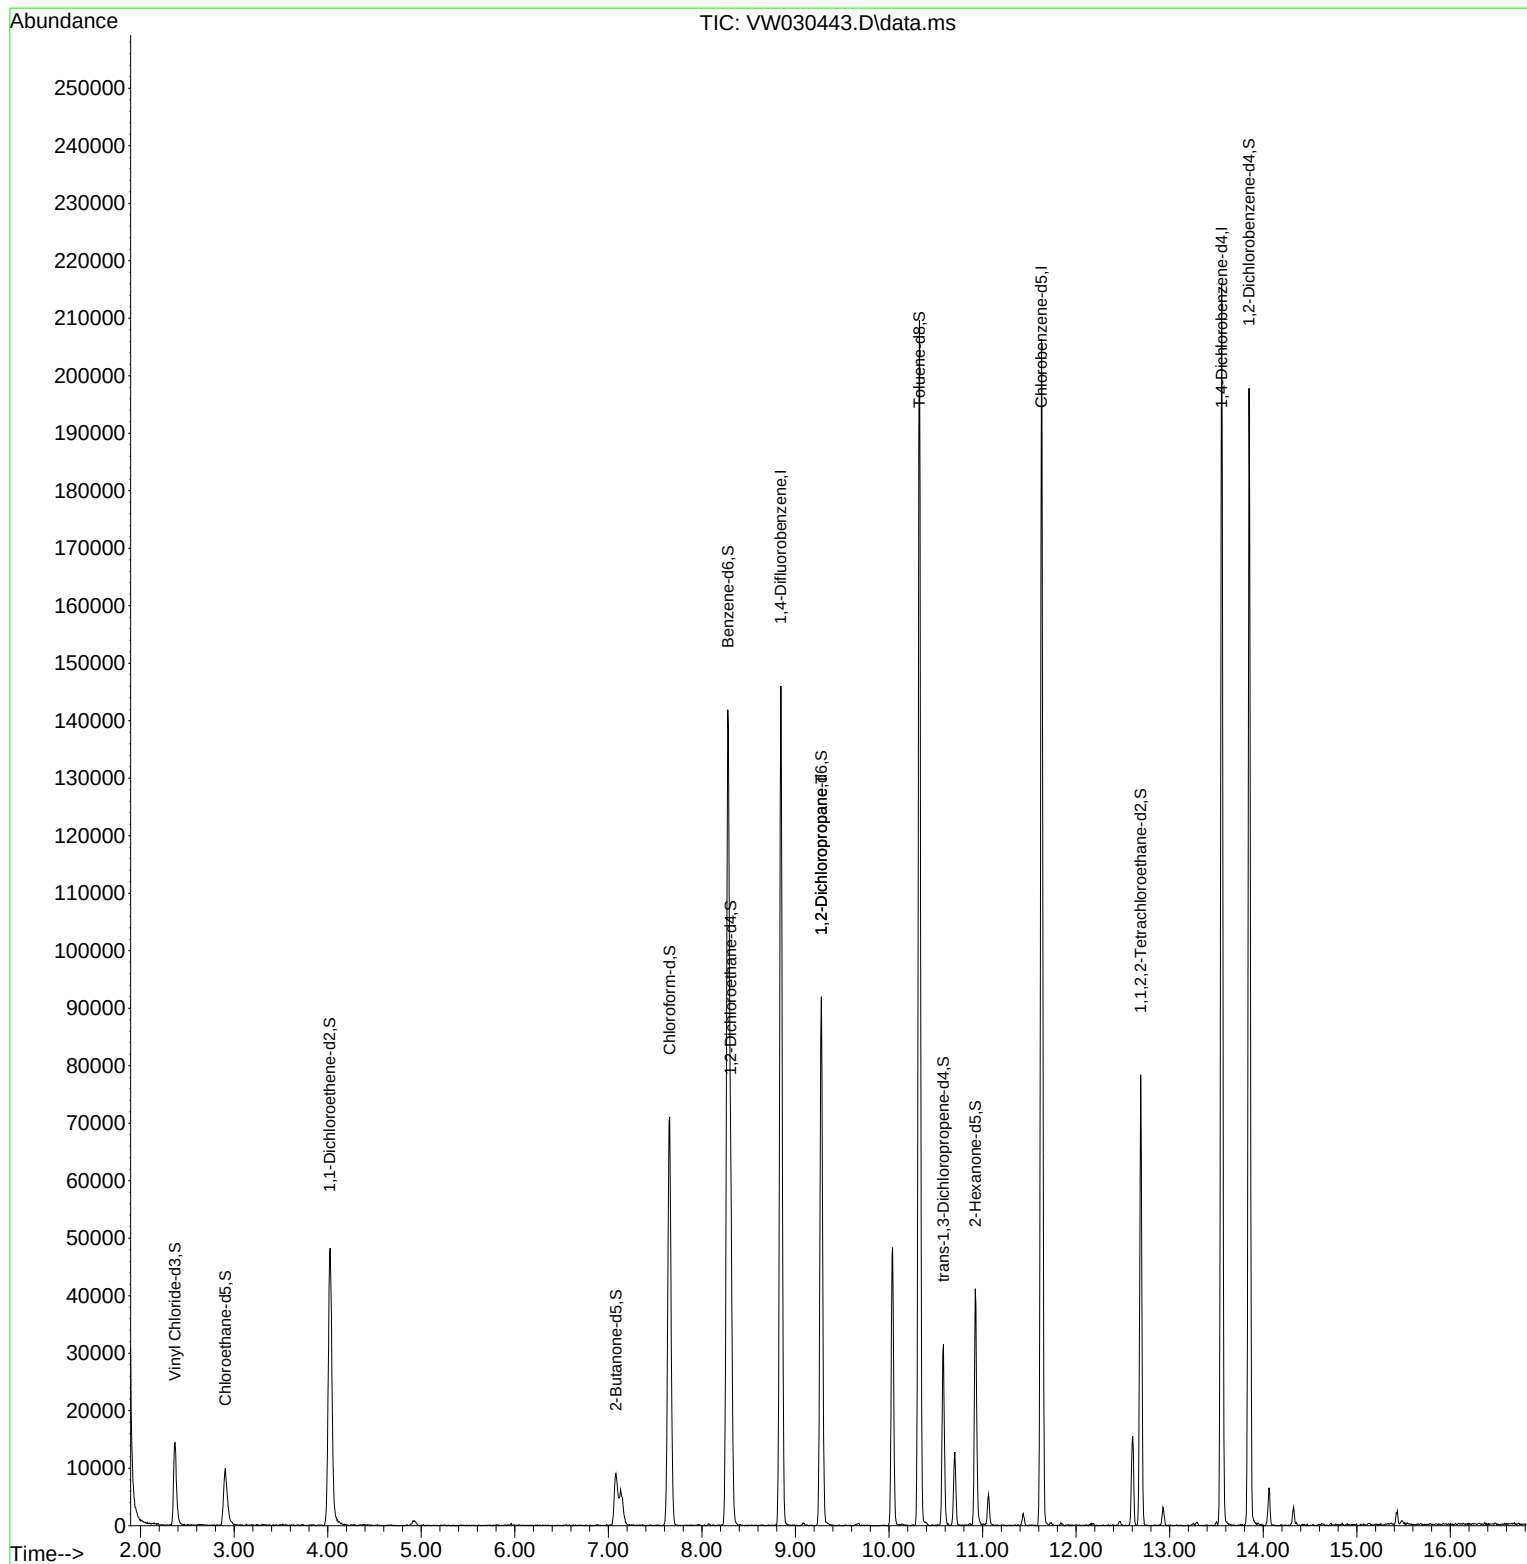

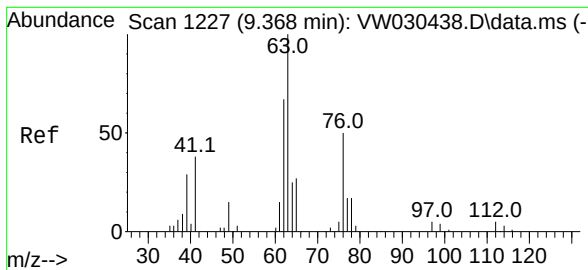

#37

1,2-Dichloropropane

Concen: 2.619 ug/L

RT: 9.276 min Scan# 11

Delta R.T. -0.091 min


Lab File: VW030443.D

Acq: 08 Oct 2024 13:24

Instrument :

MSVOA_W

ClientSampleId :

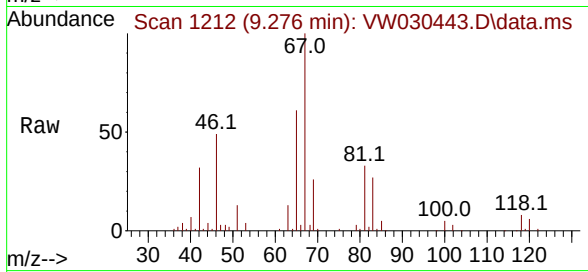

Tgt Ion: 63 Resp: 5102

Ion Ratio Lower Upper

63 100

112 0.0 3.4 5.2#

