

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
 Data File : VW030451.D
 Acq On : 08 Oct 2024 16:59
 Operator : SY/MD
 Sample : P4329-04
 Misc : 5.54g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EG5

Quant Time: Oct 09 01:20:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 09 01:13:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	226594	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	203250	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	96992	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	30104	17.002	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.000%
7) Chloroethane-d5	2.899	69	22283	17.296	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.200%
11) 1,1-Dichloroethene-d2	4.021	65	24435	18.905	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.640%
21) 2-Butanone-d5	7.081	46	15710	22.063	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	44.120%
24) Chloroform-d	7.648	84	109356	17.964	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.840%
26) 1,2-Dichloroethane-d4	8.307	65	56054	17.641	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	70.560%
32) Benzene-d6	8.276	84	222810	19.559	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.240%
36) 1,2-Dichloropropane-d6	9.276	67	57804	16.871	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	67.480%#
41) Toluene-d8	10.325	98	212438	20.337	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.360%
43) trans-1,3-Dichloroprop...	10.581	79	25495	17.890	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.560%
47) 2-Hexanone-d5	10.922	63	15478	27.358	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.720%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	40324	15.750	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	63.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	68132	21.157	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.640%
Target Compounds						
13) Acetone	4.118	43	4244	5.619	ug/L	Qvalue 74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
Data File : VW030451.D
Acq On : 08 Oct 2024 16:59
Operator : SY/MD
Sample : P4329-04
Misc : 5.54g/10mL/MSVOA_W/SOIL/B
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EG5

Quant Time: Oct 09 01:20:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 09 01:13:46 2024
Response via : Initial Calibration

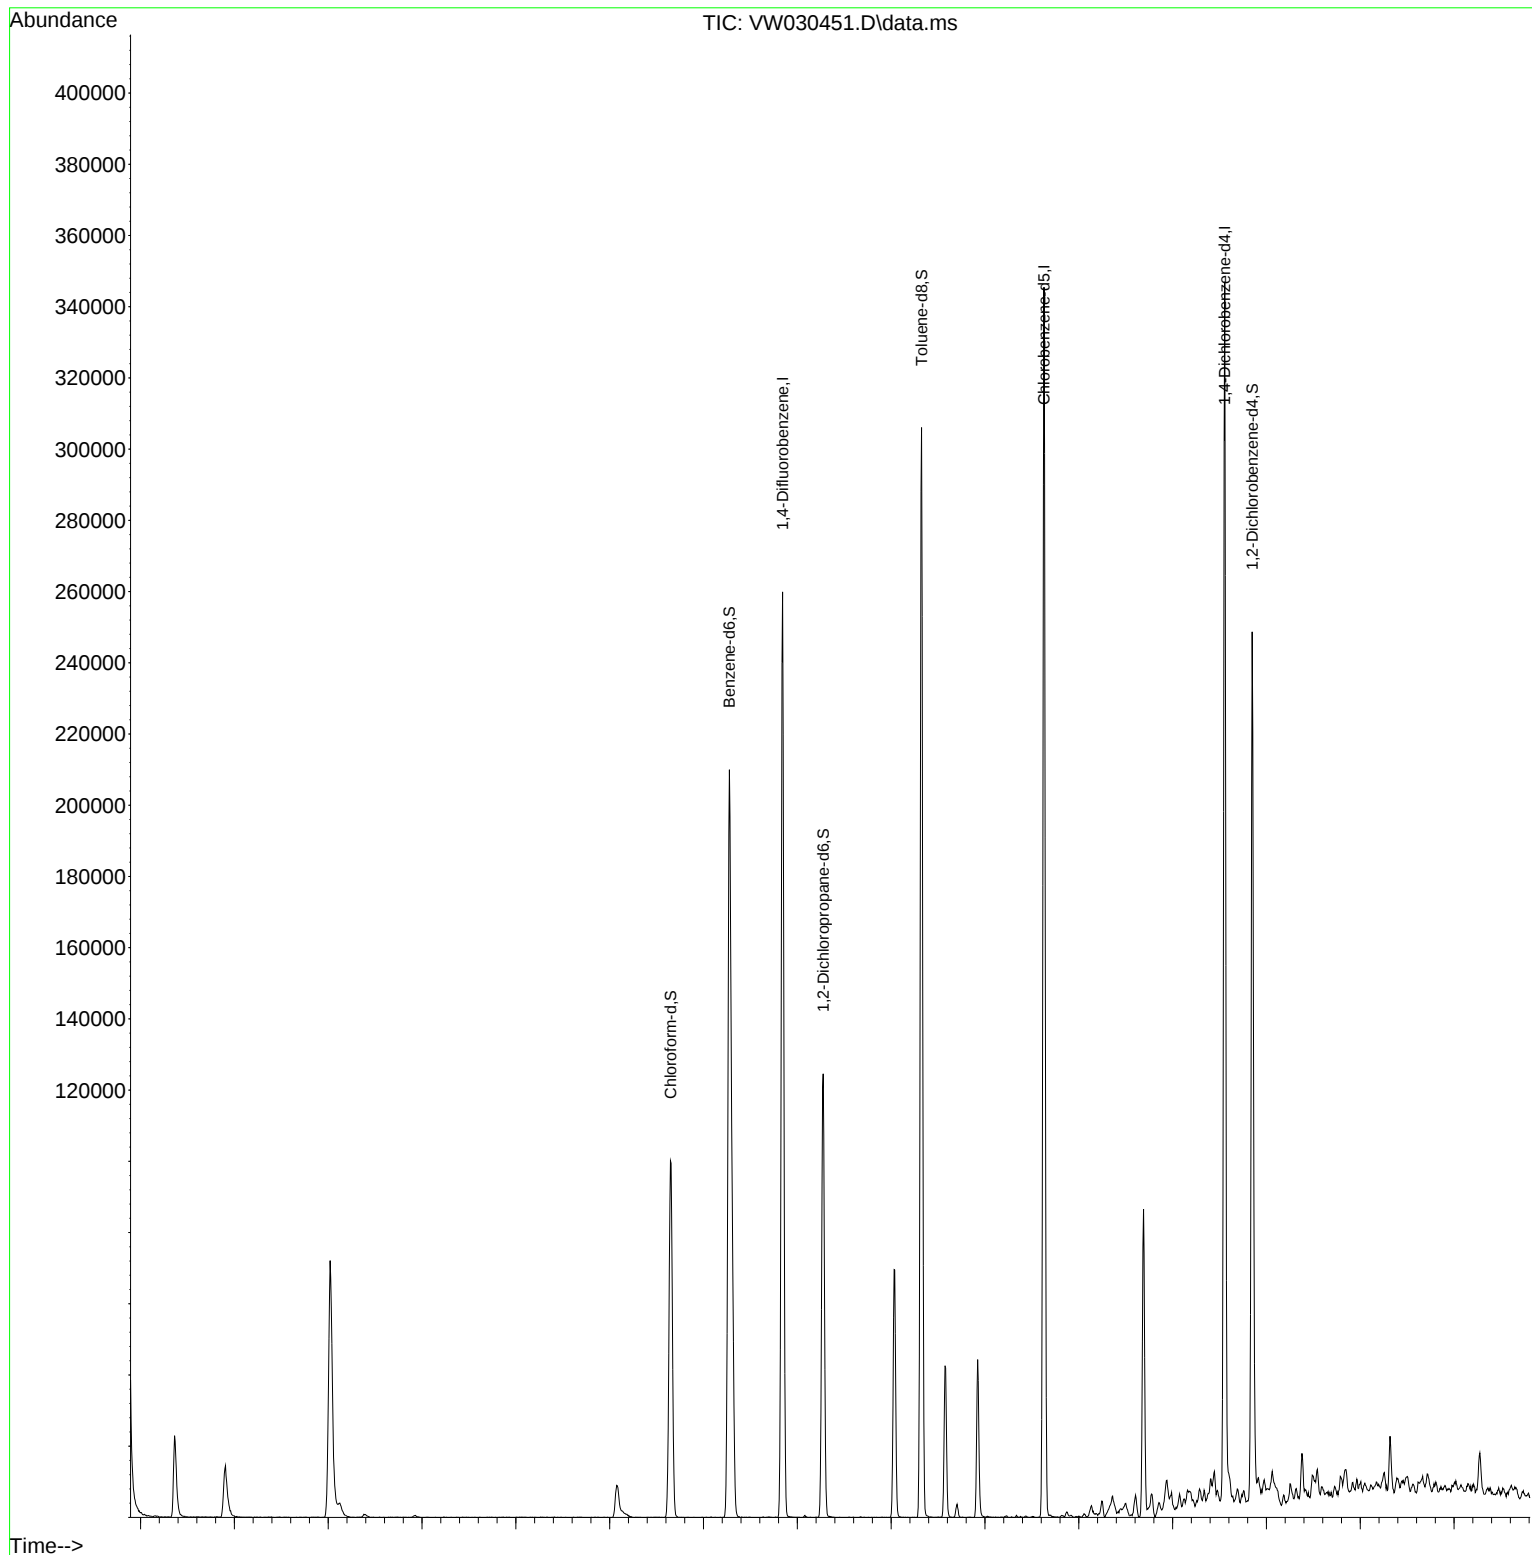

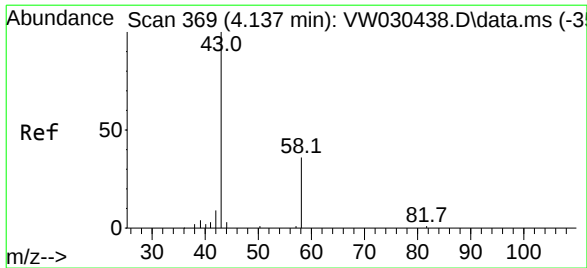

#13
 Acetone
 Concen: 5.619 ug/L
 RT: 4.118 min Scan# 36
 Delta R.T. -0.018 min
 Lab File: VW030451.D
 Acq: 08 Oct 2024 16:59

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EG5

Tgt Ion: 43	Resp: 4244
Ion Ratio	Lower Upper
43	100
58	17.5 0.0 64.0

