

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
 Data File : VW030466.D
 Acq On : 09 Oct 2024 00:11
 Operator : SY/MD
 Sample : P4346-02
 Misc : 3.10g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW4

Quant Time: Oct 09 04:23:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 09 01:13:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	174301	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	117028	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	31940	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	27148	19.932	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	79.720%	
7) Chloroethane-d5	2.899	69	21033	21.224	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	84.880%	
11) 1,1-Dichloroethene-d2	4.021	65	21371	21.495	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	86.000%	
21) 2-Butanone-d5	7.081	46	17948	32.768	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	65.540%	
24) Chloroform-d	7.648	84	103279	22.056	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	88.240%	
26) 1,2-Dichloroethane-d4	8.307	65	55902	22.872	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	91.480%	
32) Benzene-d6	8.276	84	199664	30.441	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	121.760%	
36) 1,2-Dichloropropane-d6	9.270	67	53811	27.277	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	109.120%	
41) Toluene-d8	10.325	98	167891	27.915	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	111.640%	
43) trans-1,3-Dichloroprop...	10.575	79	20813	25.365	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	101.440%	
47) 2-Hexanone-d5	10.922	63	18025	55.332	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	110.660%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	35759	24.258	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	97.040%	
66) 1,2-Dichlorobenzene-d4	13.848	152	28283	26.671	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	106.680%	
Target Compounds					Qvalue	
13) Acetone	4.137	43	3541	6.094	ug/L	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
Data File : VW030466.D
Acq On : 09 Oct 2024 00:11
Operator : SY/MD
Sample : P4346-02
Misc : 3.10g/10mL/MSVOA_W/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW4

Quant Time: Oct 09 04:23:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 09 01:13:46 2024
Response via : Initial Calibration

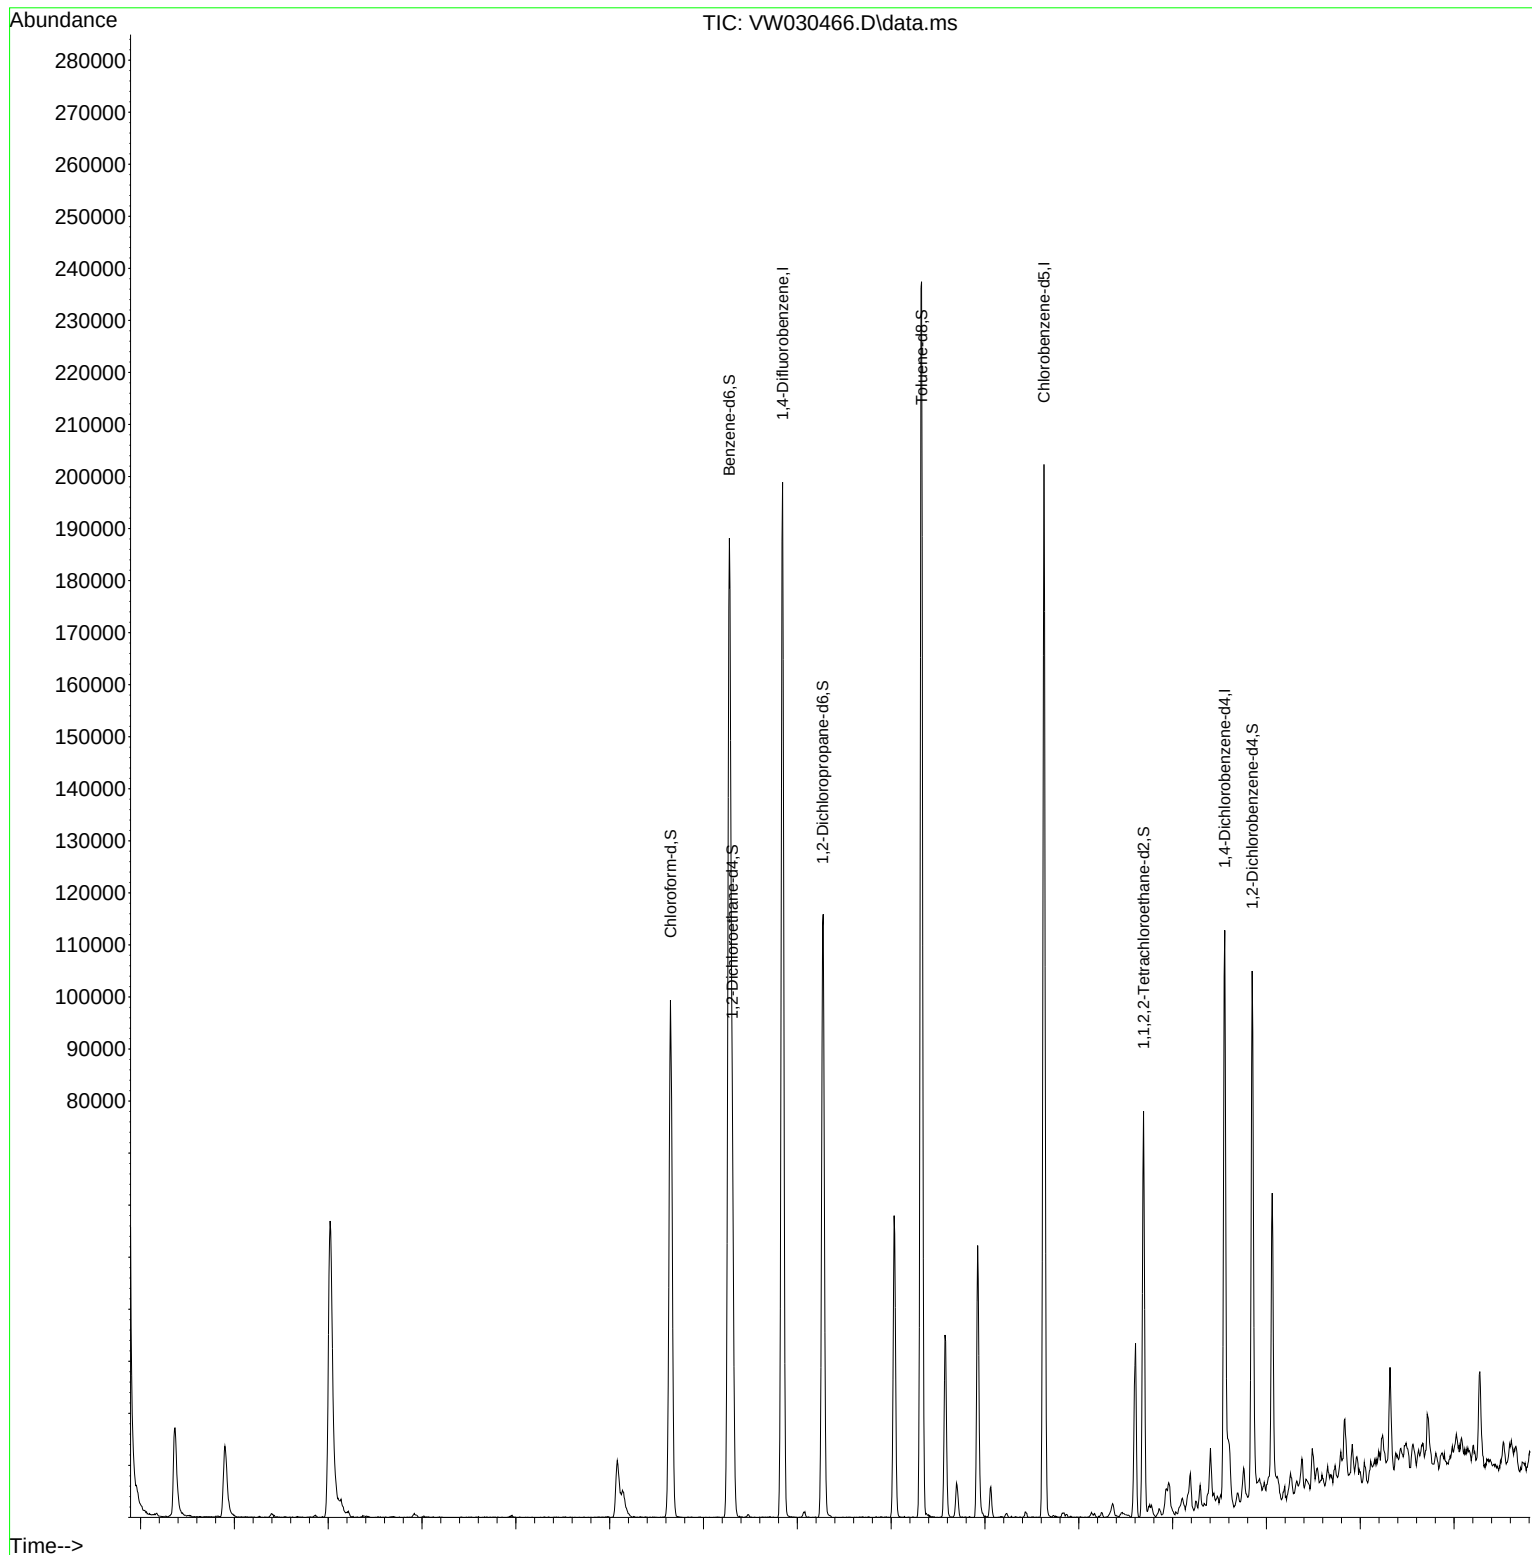

Abundance Scan 367 (4.125 min): VW030464.D\data.ms (-3

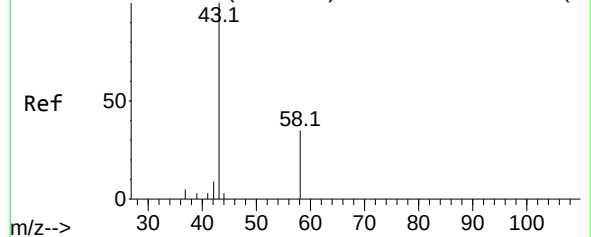

#13

Acetone

Concen: 6.094 ug/L

RT: 4.137 min Scan# 36

Delta R.T. -0.000 min

Lab File: VW030466.D

Acq: 09 Oct 2024 00:11


Instrument :

MSVOA_W

ClientSampleId :

EOAW4

Abundance Scan 369 (4.137 min): VW030466.D\data.ms

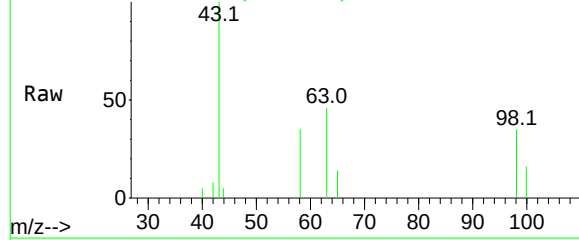


Tgt Ion: 43 Resp: 3541

Ion Ratio Lower Upper

43 100

58 21.3 0.0 64.0

Abundance Scan 369 (4.137 min): VW030466.D\data.ms (-3

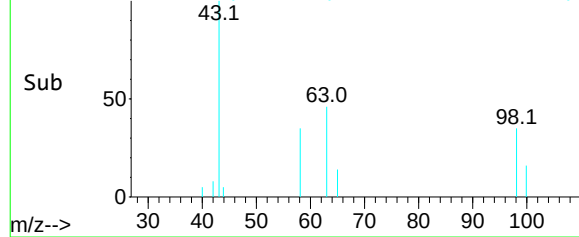

Abundance

