

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
 Data File : VW030467.D
 Acq On : 09 Oct 2024 00:35
 Operator : SY/MD
 Sample : P4346-03
 Misc : 3.75g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW5

Quant Time: Oct 09 04:28:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 09 01:13:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	107332	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	76778	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	25554	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	15955	19.023	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.080%
7) Chloroethane-d5	2.899	69	12420	20.352	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.400%
11) 1,1-Dichloroethene-d2	4.015	65	12163	19.867	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.480%
21) 2-Butanone-d5	7.075	46	13776	40.843	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.680%
24) Chloroform-d	7.654	84	60353	20.931	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.720%
26) 1,2-Dichloroethane-d4	8.307	65	36799	24.450	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.800%
32) Benzene-d6	8.276	84	119738	27.825	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.320%
36) 1,2-Dichloropropane-d6	9.270	67	32887	25.410	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.640%
41) Toluene-d8	10.325	98	97936	24.820	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.280%
43) trans-1,3-Dichloroprop...	10.575	79	14240	26.452	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	105.800%
47) 2-Hexanone-d5	10.922	63	13323	62.339	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.680%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	25188	26.044	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.160%
66) 1,2-Dichlorobenzene-d4	13.849	152	21269	25.069	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.280%
Target Compounds					Qvalue	
13) Acetone	4.131	43	2015	5.632	ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
Data File : VW030467.D
Acq On : 09 Oct 2024 00:35
Operator : SY/MD
Sample : P4346-03
Misc : 3.75g/10mL/MSVOA_W/SOIL/A
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW5

Quant Time: Oct 09 04:28:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 09 01:13:46 2024
Response via : Initial Calibration

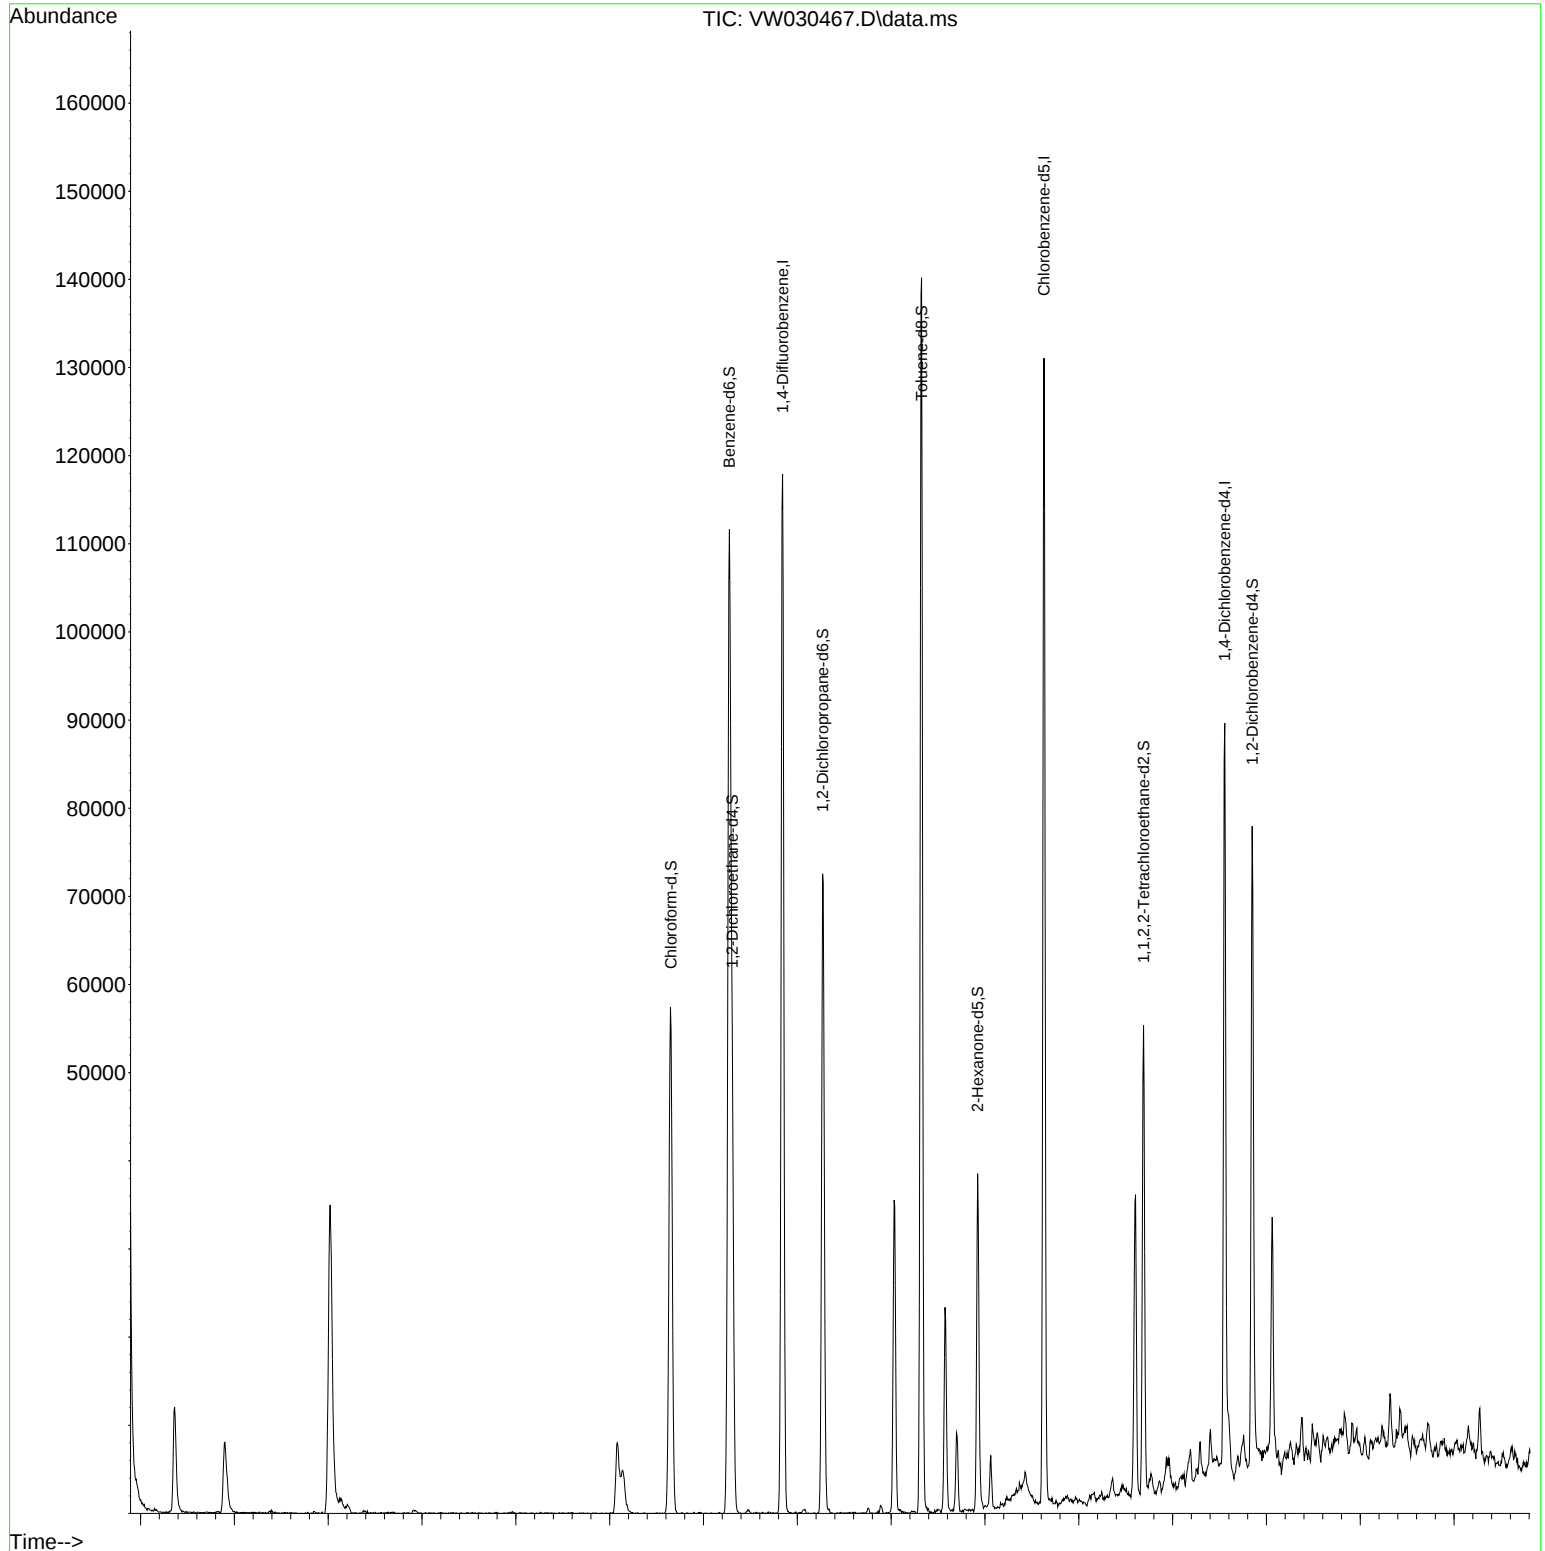

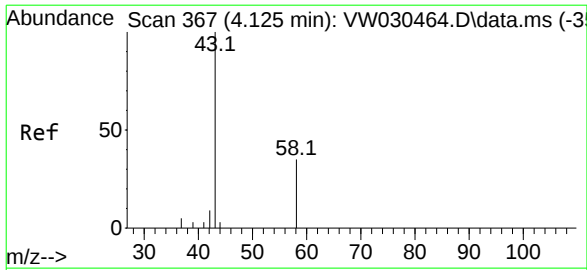

#13
 Acetone
 Concen: 5.632 ug/L
 RT: 4.131 min Scan# 368
 Delta R.T. -0.006 min
 Lab File: VW030467.D
 Acq: 09 Oct 2024 00:35

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW5

Tgt Ion: 43 Resp: 2015
 Ion Ratio Lower Upper
 43 100
 58 20.1 0.0 64.0

