

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
 Data File : VW030468.D
 Acq On : 09 Oct 2024 00:59
 Operator : SY/MD
 Sample : P4346-04
 Misc : 2.87g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW6

Quant Time: Oct 09 04:31:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 09 01:13:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	158417	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	113904	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	41380	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	22687	18.327	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.320%
7) Chloroethane-d5	2.899	69	17559	19.495	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.960%
11) 1,1-Dichloroethene-d2	4.021	65	17488	19.353	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.400%
21) 2-Butanone-d5	7.081	46	17404	34.960	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.920%
24) Chloroform-d	7.648	84	86691	20.370	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.480%
26) 1,2-Dichloroethane-d4	8.307	65	51387	23.133	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.520%
32) Benzene-d6	8.276	84	169222	26.507	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	106.040%
36) 1,2-Dichloropropane-d6	9.270	67	46457	24.195	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.800%
41) Toluene-d8	10.318	98	143999	24.599	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.400%
43) trans-1,3-Dichloroprop...	10.574	79	20003	25.046	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.200%
47) 2-Hexanone-d5	10.922	63	17446	55.024	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.040%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	37530	26.158	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.640%
66) 1,2-Dichlorobenzene-d4	13.848	152	35766	26.033	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.120%
Target Compounds						
13) Acetone	4.130	43	2398	4.541	ug/L	Qvalue 57

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
Data File : VW030468.D
Acq On : 09 Oct 2024 00:59
Operator : SY/MD
Sample : P4346-04
Misc : 2.87g/10mL/MSVOA_W/SOIL/A
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW6

Quant Time: Oct 09 04:31:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 09 01:13:46 2024
Response via : Initial Calibration

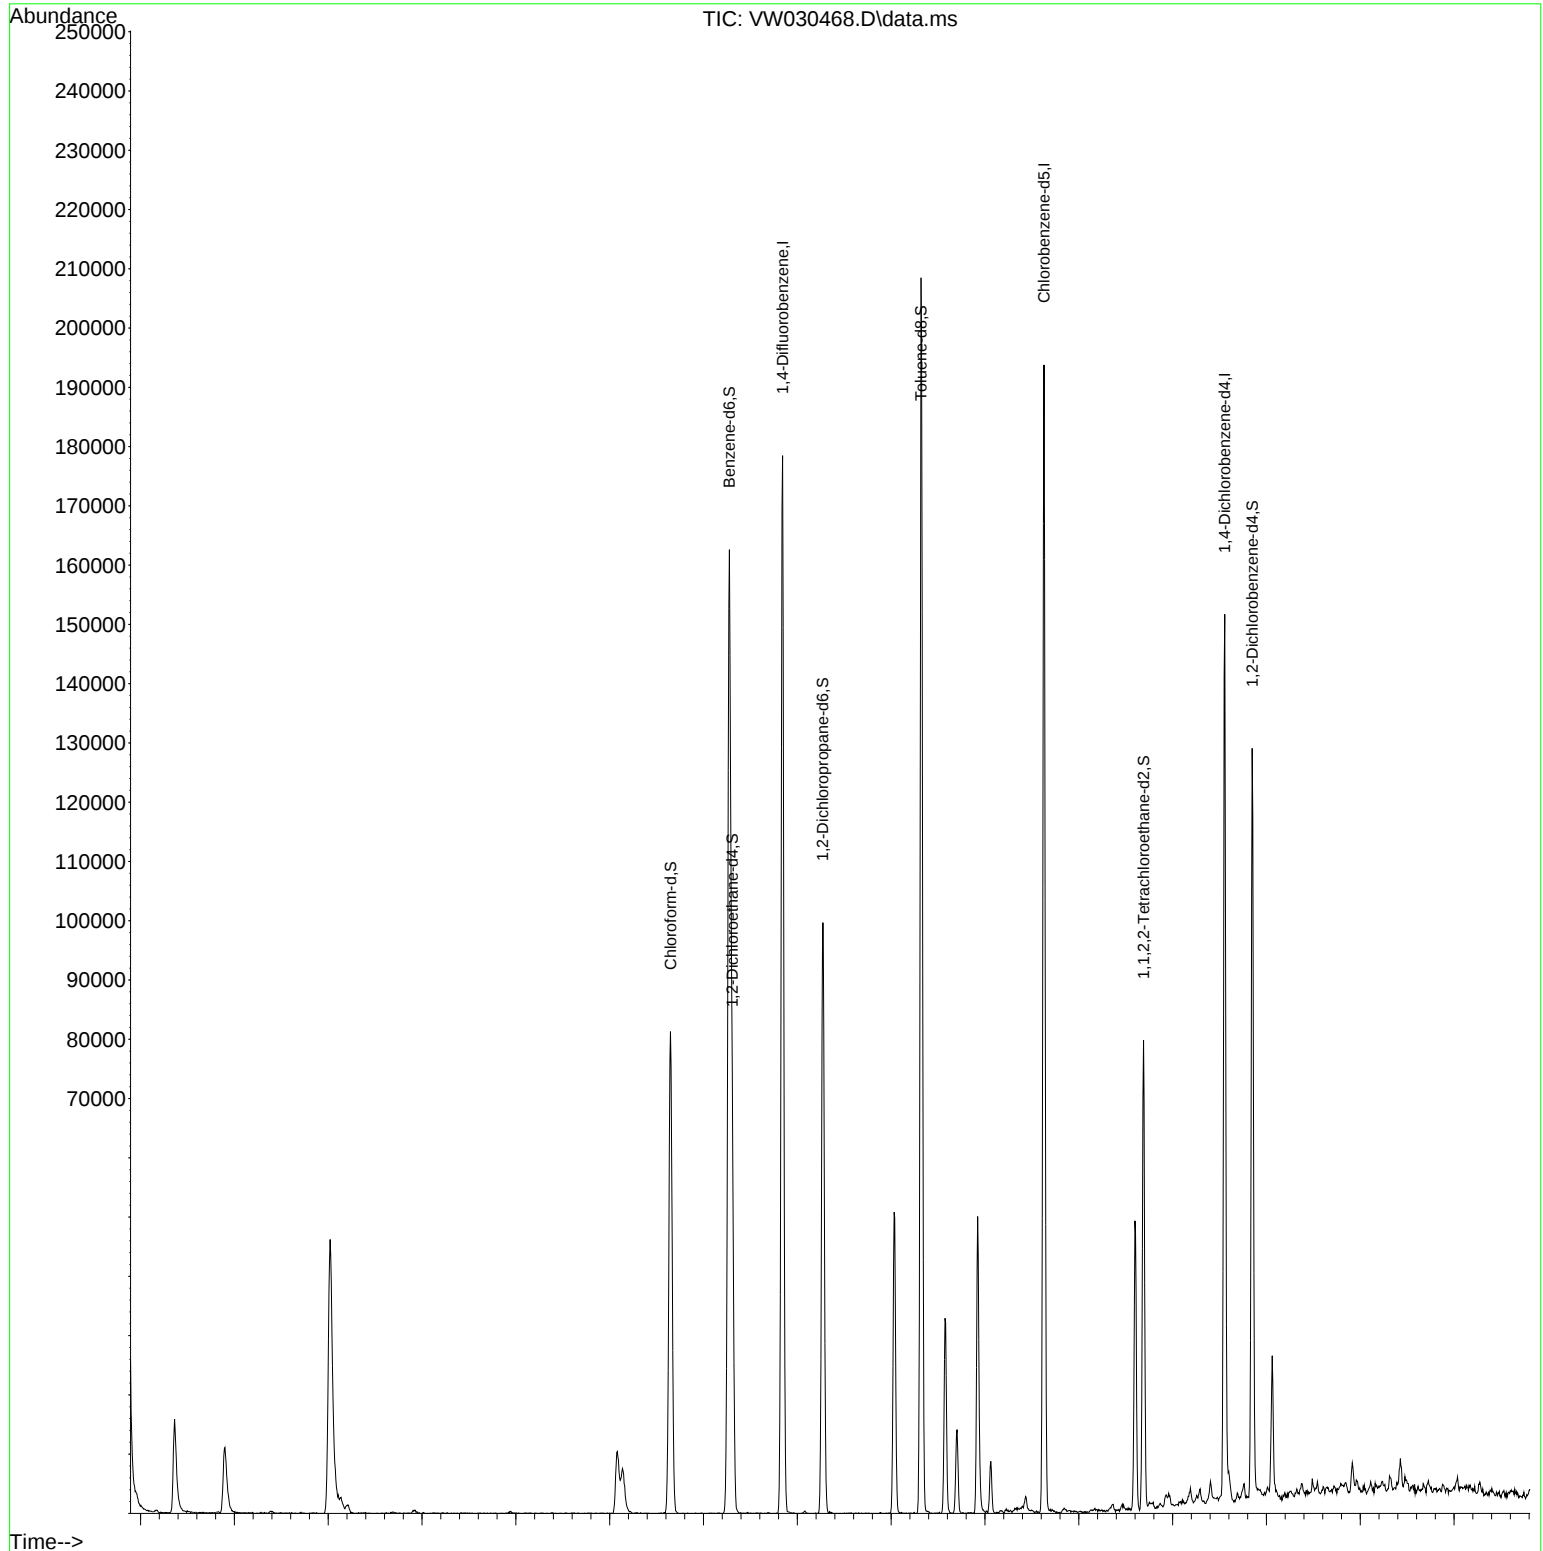

Abundance Scan 367 (4.125 min): VW030464.D\data.ms (-3

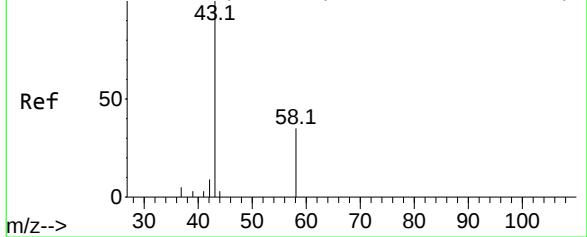

#13

Acetone

Concen: 4.541 ug/L

RT: 4.130 min Scan# 36

Delta R.T. -0.006 min

Lab File: VW030468.D

Acq: 09 Oct 2024 00:59


Instrument :

MSVOA_W

ClientSampleId :

EOAW6

Abundance Scan 368 (4.130 min): VW030468.D\data.ms

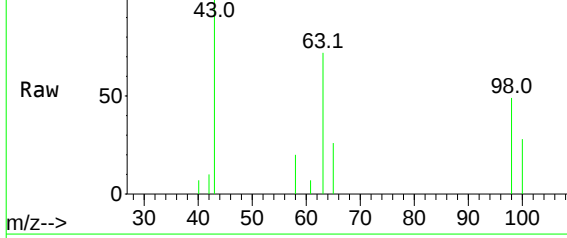

Tgt Ion: 43 Resp: 2398

Ion Ratio Lower Upper

43 100

58 8.1 0.0 64.0

Abundance Scan 368 (4.130 min): VW030468.D\data.ms (-3

