
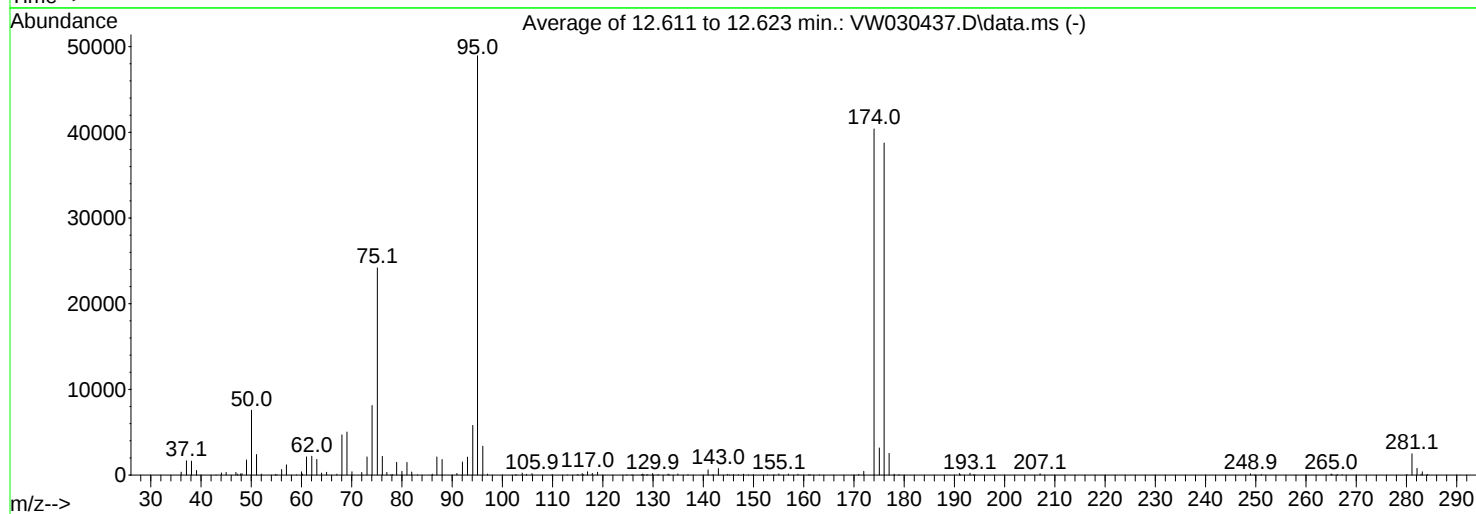


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100824\
Data File : VW030437.D
Acq On : 08 Oct 2024 09:38
Operator : SY/MD
Sample : BFB571
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB571

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Title : SFAM01.0
Last Update : Wed Oct 09 01:13:46 2024

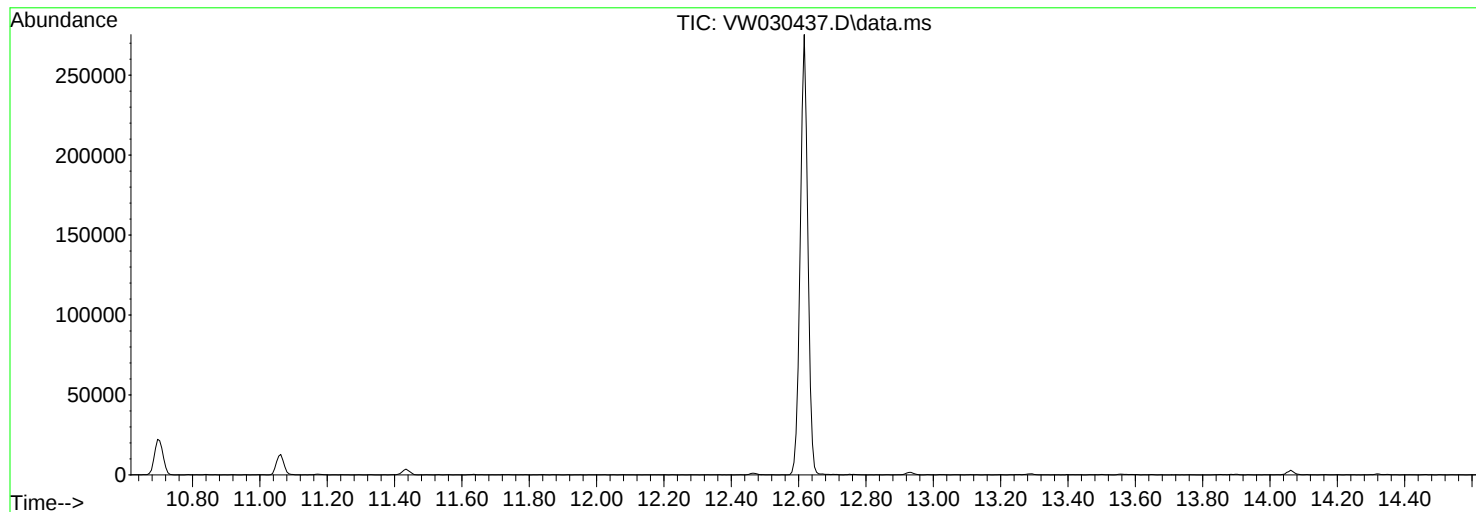

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	7573	PASS
75	95	30	80	49.4	24184	PASS
95	95	100	100	100.0	48939	PASS
96	95	5	9	6.9	3367	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.5	40395	PASS
175	174	5	9	7.8	3169	PASS
176	174	95	101	95.9	38747	PASS
177	176	5	9	6.5	2531	PASS

m/z	Abundance
40.20	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB571

m/z	Abundance
36.10	318.0
37.10	1674.0
38.10	1650.0
39.10	621.0
44.10	211.0
45.00	332.0
46.90	452.0
47.90	256.0
49.10	1907.0
50.10	7886.0
51.00	2544.0
52.00	125.0
54.80	104.0
56.10	710.0
57.00	1234.0
59.00	73.0
60.00	536.0
61.00	2129.0
62.00	2333.0
63.10	2044.0
64.10	256.0
65.00	385.0
67.00	118.0
68.10	4717.0
69.10	5211.0
70.10	312.0
72.00	254.0
73.00	2113.0
74.10	8133.0
75.10	23992.0
76.10	2111.0
77.00	351.0
77.80	107.0
79.00	1440.0
80.00	403.0
81.00	1471.0
82.00	343.0
83.20	55.0
86.00	121.0
86.90	1946.0
88.00	1813.0
91.00	179.0
92.00	1683.0
93.10	2018.0
94.10	5574.0
95.00	45656.0
96.10	3498.0
97.00	85.0
102.60	55.0
103.90	255.0
104.80	100.0
105.90	179.0
109.90	80.0
112.90	65.0
114.90	114.0
115.90	276.0
116.90	355.0
117.90	215.0
119.00	368.0
124.80	95.0
125.80	89.0
127.70	136.0
128.20	76.0
128.70	54.0
129.90	175.0
131.10	84.0
133.00	380.0
135.00	180.0
140.90	576.0
143.00	764.0
144.80	102.0
146.00	51.0
147.00	93.0
148.00	135.0
149.00	71.0
150.00	60.0
155.10	158.0
156.90	54.0
158.80	84.0
161.30	85.0
163.10	75.0
171.00	114.0
172.00	351.0
174.00	35144.0
175.10	2763.0
176.00	32104.0
177.00	2175.0
177.90	102.0
179.00	107.0
191.00	393.0
193.10	305.0
193.80	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB571

194.10	58.0
207.10	257.0
249.00	279.0
249.70	56.0
251.20	128.0
265.00	293.0
266.30	113.0
267.20	115.0
280.10	114.0
281.10	3798.0
282.10	1186.0
283.20	846.0
284.20	142.0

Instrument :
MSVOA_W
ClientSampleId :
BFB571

m/z	Abundance
36.10	392.0
37.10	1868.0
38.10	1753.0
39.00	553.0
40.00	64.0
44.10	262.0
45.00	326.0
47.30	321.0
48.10	340.0
49.00	1772.0
50.00	8783.0
51.00	2719.0
52.00	115.0
54.90	157.0
56.10	695.0
57.00	1345.0
60.00	624.0
61.00	2432.0
62.10	2514.0
63.10	1898.0
64.00	275.0
65.00	371.0
67.10	107.0
68.10	5027.0
69.10	5430.0
70.10	458.0
72.00	424.0
73.10	2252.0
74.10	8866.0
75.10	28232.0
76.10	2436.0
77.00	330.0
79.00	1595.0
80.00	618.0
81.00	1528.0
82.00	430.0
86.10	105.0
87.00	2669.0
88.00	1847.0
90.80	236.0
92.10	1677.0
93.00	2256.0
94.10	6424.0
95.10	55560.0
96.10	3663.0
97.00	119.0
102.80	63.0
103.90	239.0
104.80	85.0
106.00	176.0
109.90	59.0
115.10	57.0
115.90	253.0
116.90	434.0
118.00	216.0
119.00	339.0
127.90	199.0
128.90	62.0
129.90	161.0
131.00	86.0
133.20	174.0
134.90	93.0
136.90	79.0
140.90	725.0
142.00	65.0
143.00	845.0
144.70	76.0
145.20	62.0
146.00	83.0
148.00	93.0
149.90	56.0
155.00	145.0
157.00	121.0
158.90	100.0
161.20	97.0
171.00	53.0
172.00	513.0
174.00	47840.0
175.00	3988.0
176.00	47528.0
177.00	3044.0
178.00	162.0
178.90	74.0
191.00	160.0
193.10	248.0
207.00	119.0
248.90	154.0
251.00	78.0
265.20	180.0
266.10	56.0
281.10	2833.0
282.10	846.0

Instrument :
MSVOA_W
ClientSampleId :
BFB571

283.10317.0

284.2055.0

Instrument :
MSVOA_W
ClientSampleId :
BFB571

m/z	Abundance
35.90	339.0
37.10	1478.0
38.10	1509.0
39.20	434.0
40.10	65.0
43.00	54.0
44.00	276.0
45.00	285.0
47.00	492.0
47.80	161.0
48.20	166.0
49.10	1608.0
50.10	6049.0
51.10	1931.0
52.10	100.0
55.10	126.0
56.00	534.0
57.00	1016.0
60.20	340.0
61.00	1809.0
62.00	1762.0
63.00	1552.0
63.90	172.0
65.10	224.0
67.10	114.0
68.00	4357.0
69.00	4430.0
70.00	399.0
72.00	233.0
73.00	1997.0
74.00	7373.0
75.10	20328.0
76.10	2007.0
77.00	283.0
78.10	161.0
78.90	1445.0
80.10	321.0
81.00	1441.0
81.90	305.0
83.00	54.0
86.10	100.0
87.00	1745.0
88.00	1794.0
91.00	172.0
92.10	1226.0
93.10	2025.0
94.10	5396.0
95.00	45600.0
96.10	2939.0
97.10	135.0
104.00	216.0
104.80	83.0
105.80	160.0
116.10	165.0
117.00	375.0
117.80	173.0
118.90	294.0
128.00	190.0
129.00	82.0
129.90	203.0
130.90	51.0
135.00	139.0
137.00	109.0
141.00	533.0
141.90	69.0
143.00	665.0
144.90	64.0
146.00	90.0
147.90	71.0
152.80	55.0
154.10	59.0
155.00	97.0
156.80	103.0
157.10	101.0
158.90	140.0
161.00	116.0
170.80	91.0
171.90	450.0
174.00	38200.0
175.00	2756.0
176.00	36608.0
177.00	2373.0
178.10	81.0
191.20	124.0
193.20	124.0
207.00	104.0
265.00	110.0
280.90	840.0
282.10	339.0
282.90	275.0

Instrument :
MSVOA_W
ClientSampleId :
BFB571