




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030479.D
 Acq On : 09 Oct 2024 17:35
 Operator : SY/MD
 Sample : P4346-05
 Misc : 2.56g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW7

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:30:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

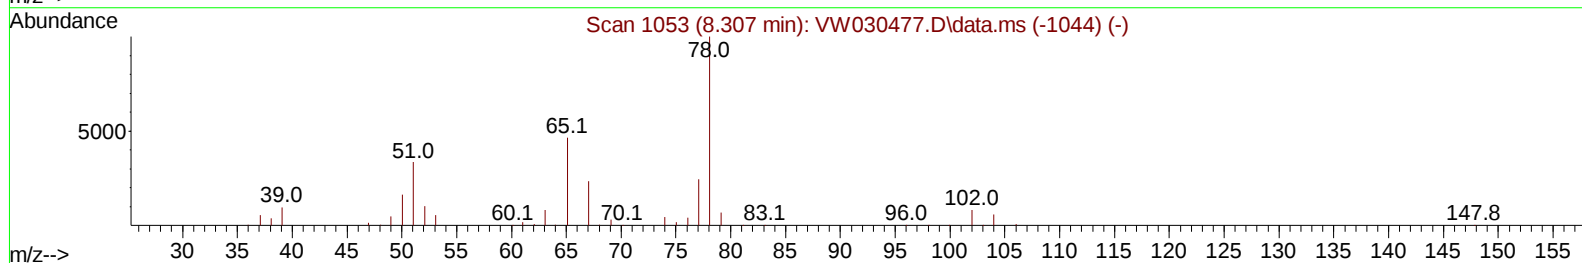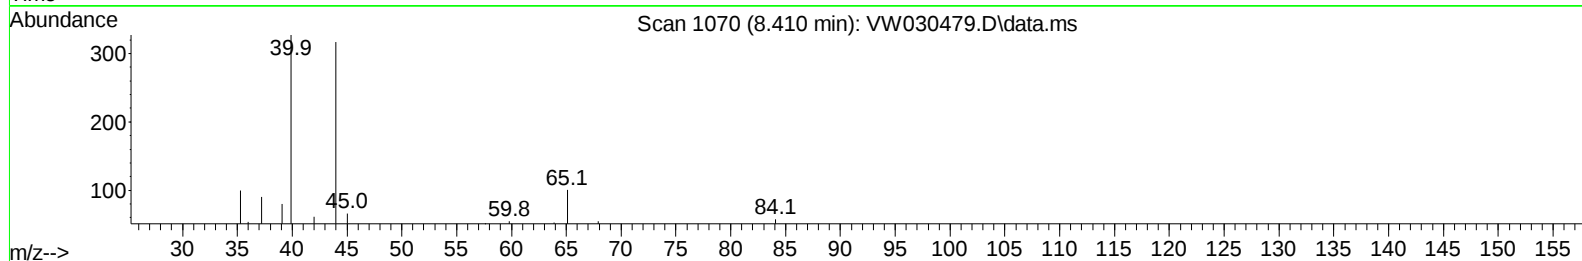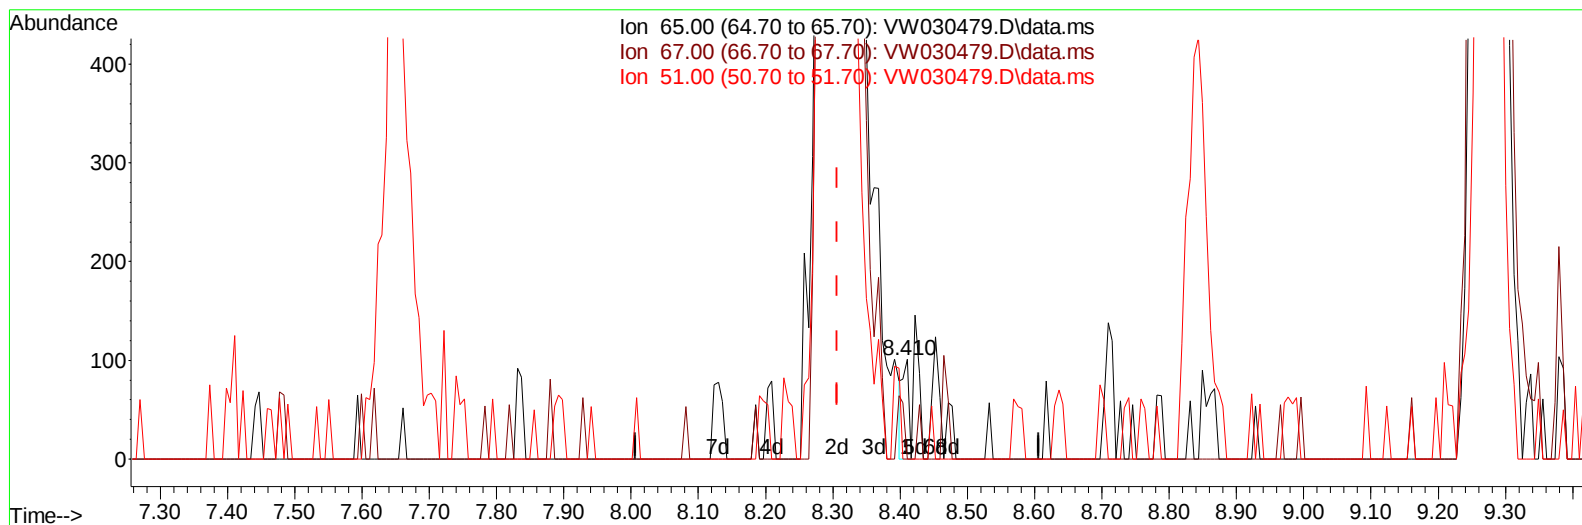

TIC: VW030479.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.410min (+ 0.104) 0.16 ug/L

response 67

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	65.67
51.00	109.40	101.49
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030479.D
 Acq On : 09 Oct 2024 17:35
 Operator : SY/MD
 Sample : P4346-05
 Misc : 2.56g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW7

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:30:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

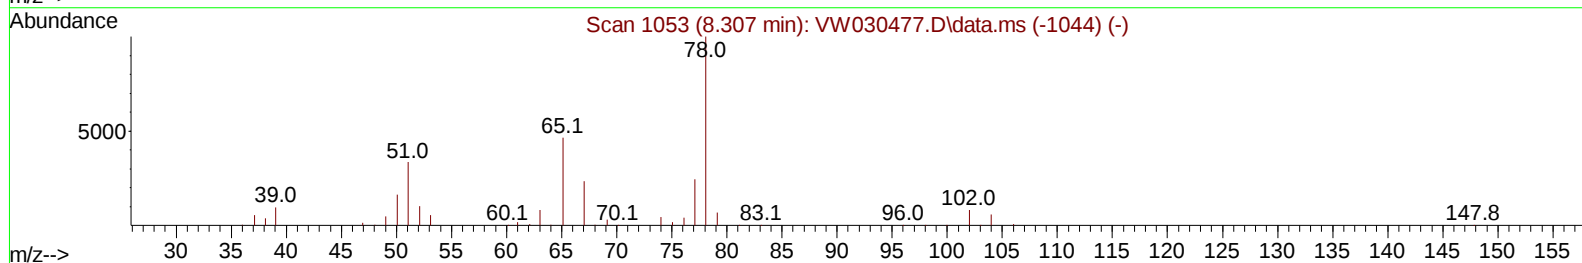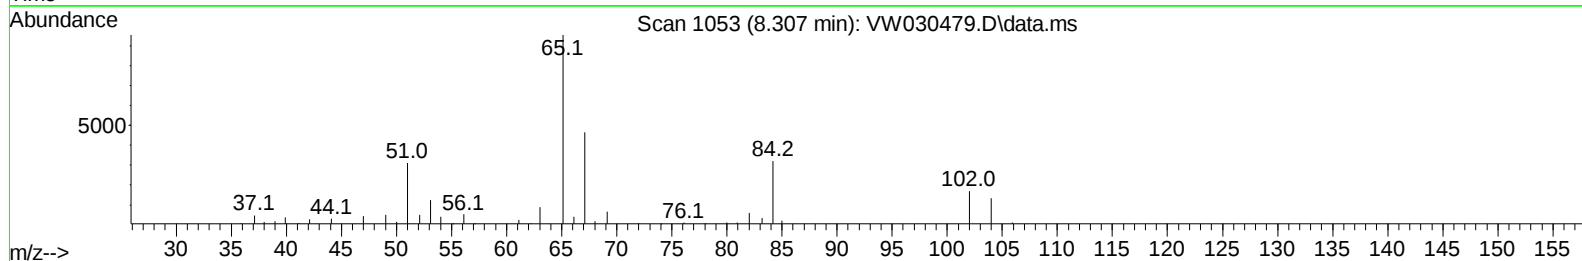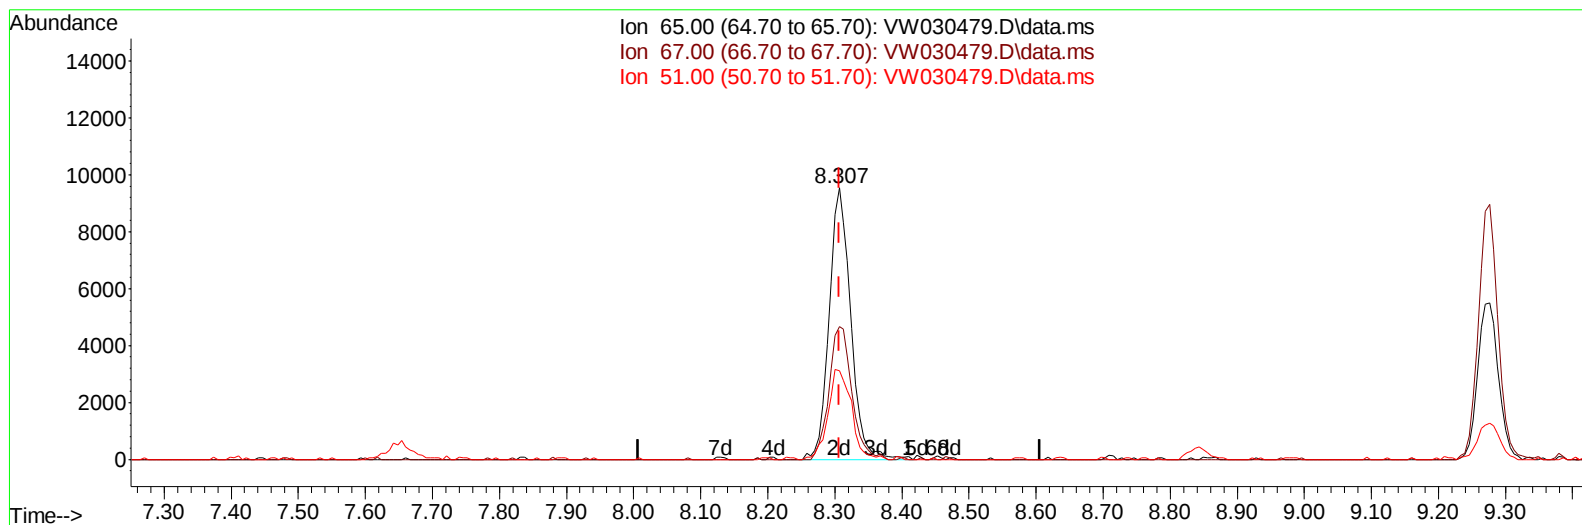

TIC: VW030479.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 49.58 ug/L m

response 21398

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.21#
51.00	109.40	0.32#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100924\
 Data File : VW030479.D
 Acq On : 09 Oct 2024 17:35
 Operator : SY/MD
 Sample : P4346-05
 Misc : 2.56g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW7

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:30:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		29020	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		24327	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		7532	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		11725	25.704	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	102.800%	
7) Chloroethane-d5	2.893	69		11452	33.167	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	132.680%	
11) 1,1-Dichloroethene-d2	4.027	65		4975	26.222	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	104.880%	
21) 2-Butanone-d5	7.087	46		8201	99.903	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135		Recovery	=	199.800%#	
24) Chloroform-d	7.654	84		29787	35.892	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	143.560%	
26) 1,2-Dichloroethane-d4	8.307	65		21398m	49.583	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	198.320%#	
32) Benzene-d6	8.276	84		48157	34.107	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	136.440%#	
36) 1,2-Dichloropropane-d6	9.276	67		18154	43.806	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	175.240%#	
41) Toluene-d8	10.325	98		31668	24.569	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	98.280%	
43) trans-1,3-Dichloroprop...	10.581	79		5082	29.286	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	117.160%	
47) 2-Hexanone-d5	10.928	63		4645	87.023	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	174.040%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		15309	50.301	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	201.200%#	
66) 1,2-Dichlorobenzene-d4	13.854	152		8881	34.848	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	139.400%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030479.D
Acq On : 09 Oct 2024 17:35
Operator : SY/MD
Sample : P4346-05
Misc : 2.56g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW7

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:30:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

