




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030480.D
 Acq On : 09 Oct 2024 17:59
 Operator : SY/MD
 Sample : P4346-06
 Misc : 3.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:30:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

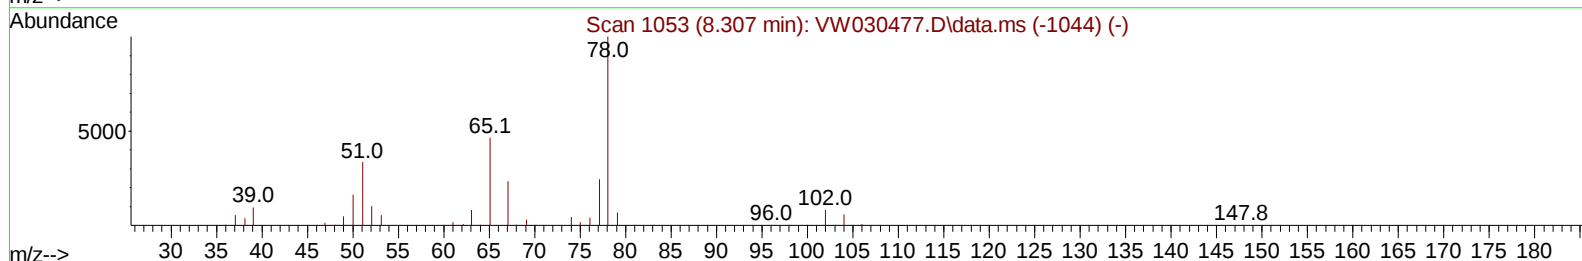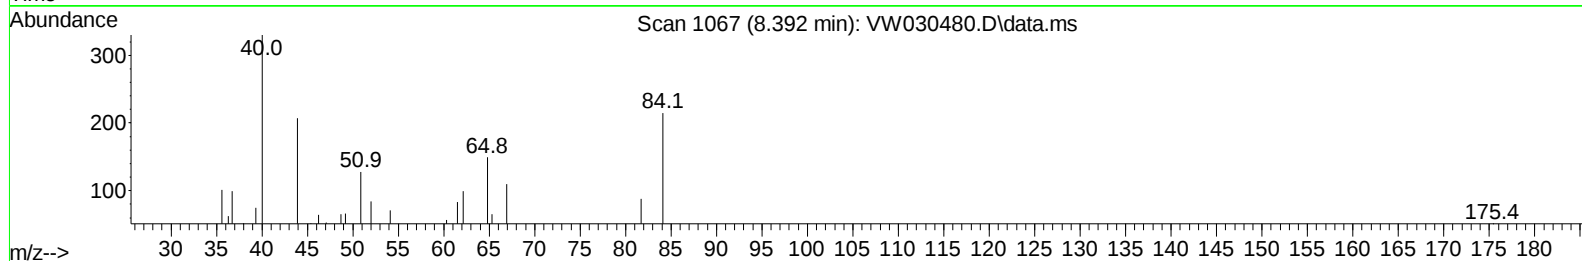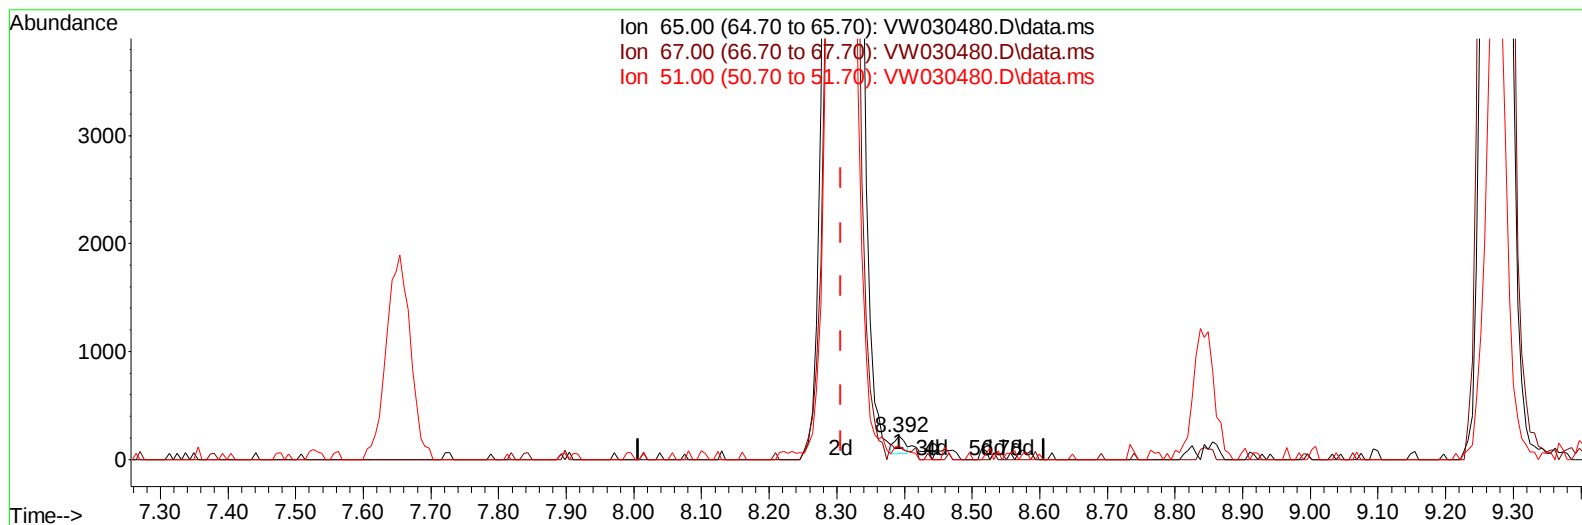

TIC: VW030480.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.392min (+ 0.085) 0.10 ug/L

response 167

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	53.89
51.00	109.40	113.77
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030480.D
 Acq On : 09 Oct 2024 17:59
 Operator : SY/MD
 Sample : P4346-06
 Misc : 3.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW8

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:30:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

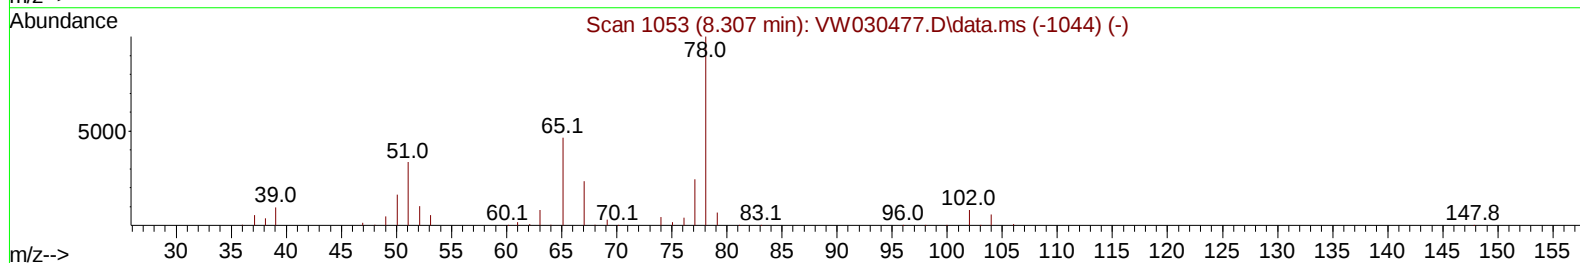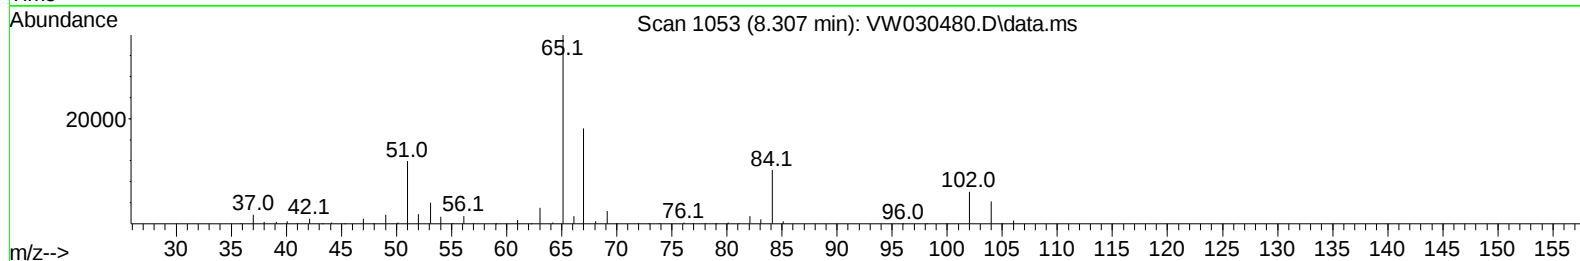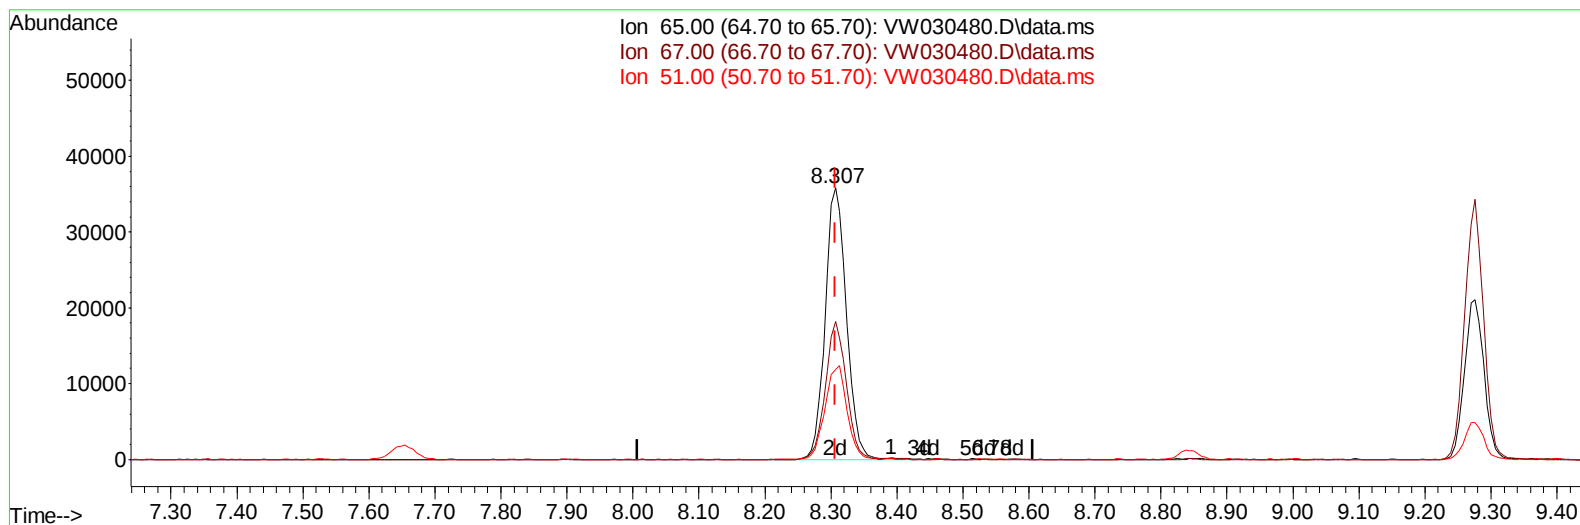

TIC: VW030480.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 48.65 ug/L m

response 80256

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.11#
51.00	109.40	0.24#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100924\
 Data File : VW030480.D
 Acq On : 09 Oct 2024 17:59
 Operator : SY/MD
 Sample : P4346-06
 Misc : 3.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:30:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		110921	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		96764	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		30067	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		33663	19.308	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	77.240%		
7) Chloroethane-d5	2.899	69		38816	29.411	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	117.640%		
11) 1,1-Dichloroethene-d2	4.021	65		15973	22.027	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	88.120%		
21) 2-Butanone-d5	7.081	46		32246	102.771	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	205.540%#		
24) Chloroform-d	7.648	84		107104	33.764	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	135.040%		
26) 1,2-Dichloroethane-d4	8.307	65		80256m	48.655	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	194.600%#		
32) Benzene-d6	8.276	84		174196	31.017	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	124.080%		
36) 1,2-Dichloropropane-d6	9.276	67		68216	41.383	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	165.520%#		
41) Toluene-d8	10.325	98		118661	23.145	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	92.560%		
43) trans-1,3-Dichloroprop...	10.575	79		22228	32.203	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	128.800%		
47) 2-Hexanone-d5	10.922	63		24794	116.781	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	233.560%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		61504	50.805	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	203.240%#		
66) 1,2-Dichlorobenzene-d4	13.848	152		35322	34.720	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	138.880%#		
Target Compounds							
13) Acetone	4.131	43		5570	12.126	ug/L	Qvalue 53

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030480.D
Acq On : 09 Oct 2024 17:59
Operator : SY/MD
Sample : P4346-06
Misc : 3.27g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:30:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

