




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030481.D
 Acq On : 09 Oct 2024 18:23
 Operator : SY/MD
 Sample : P4346-07
 Misc : 3.42g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW9

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:30:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

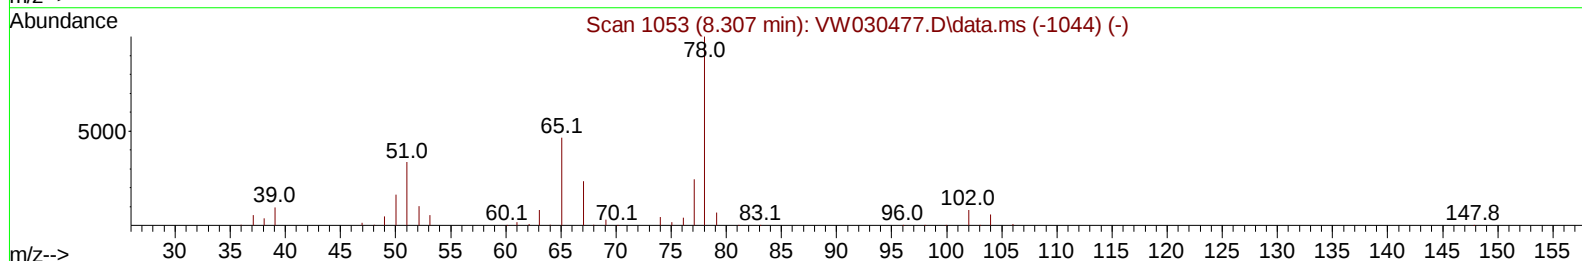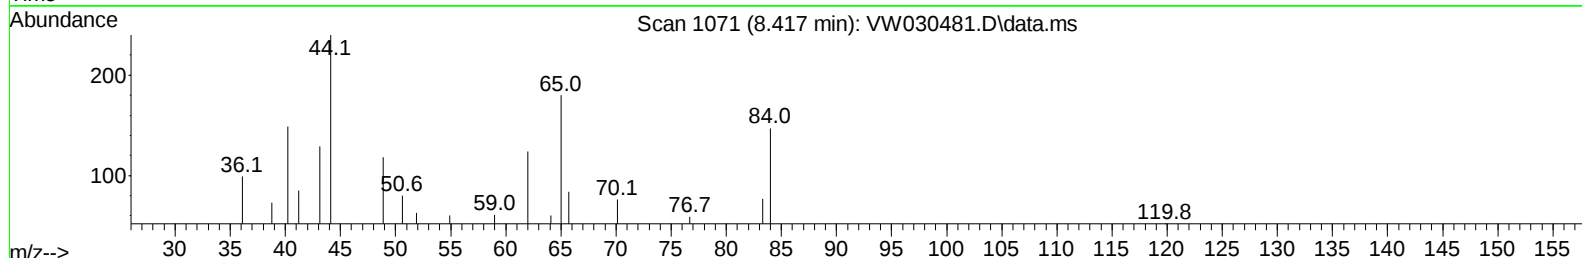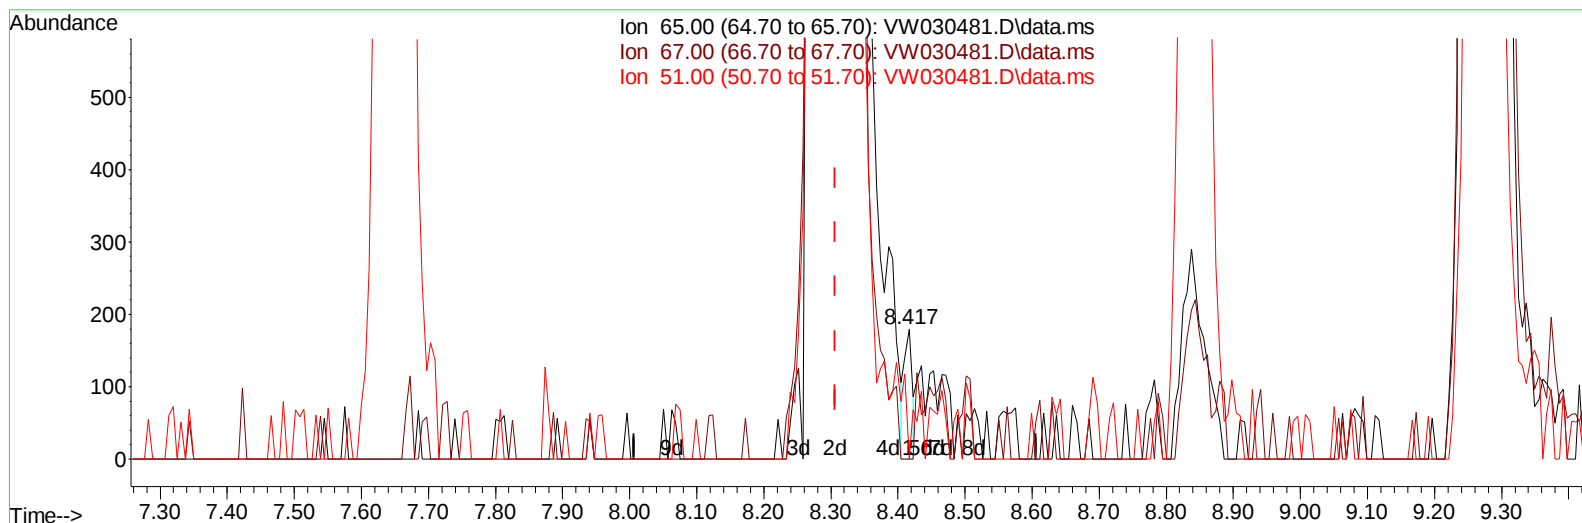

TIC: VW030481.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.417min (+ 0.110) 0.03 ug/L

response 149

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	48.32
51.00	109.40	104.03
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030481.D
 Acq On : 09 Oct 2024 18:23
 Operator : SY/MD
 Sample : P4346-07
 Misc : 3.42g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW9

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:30:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

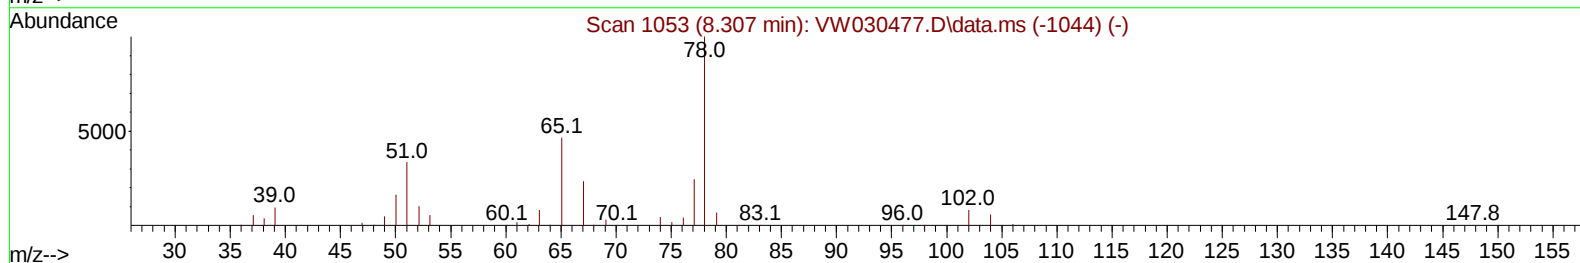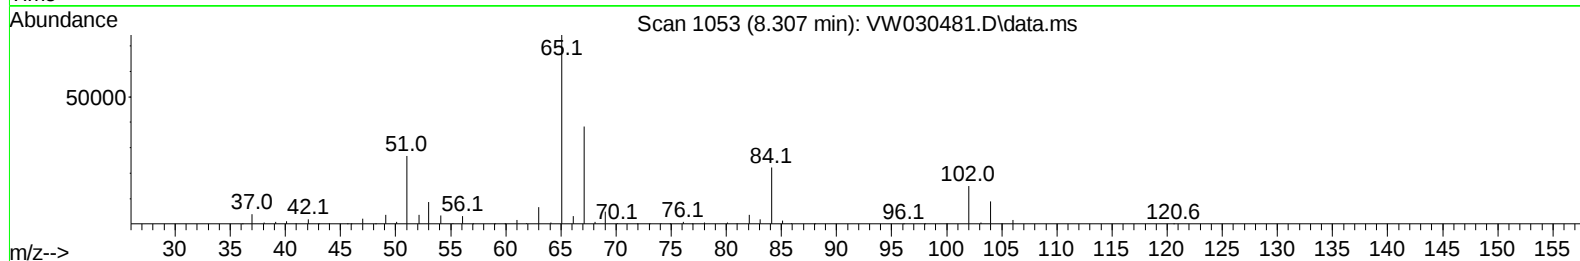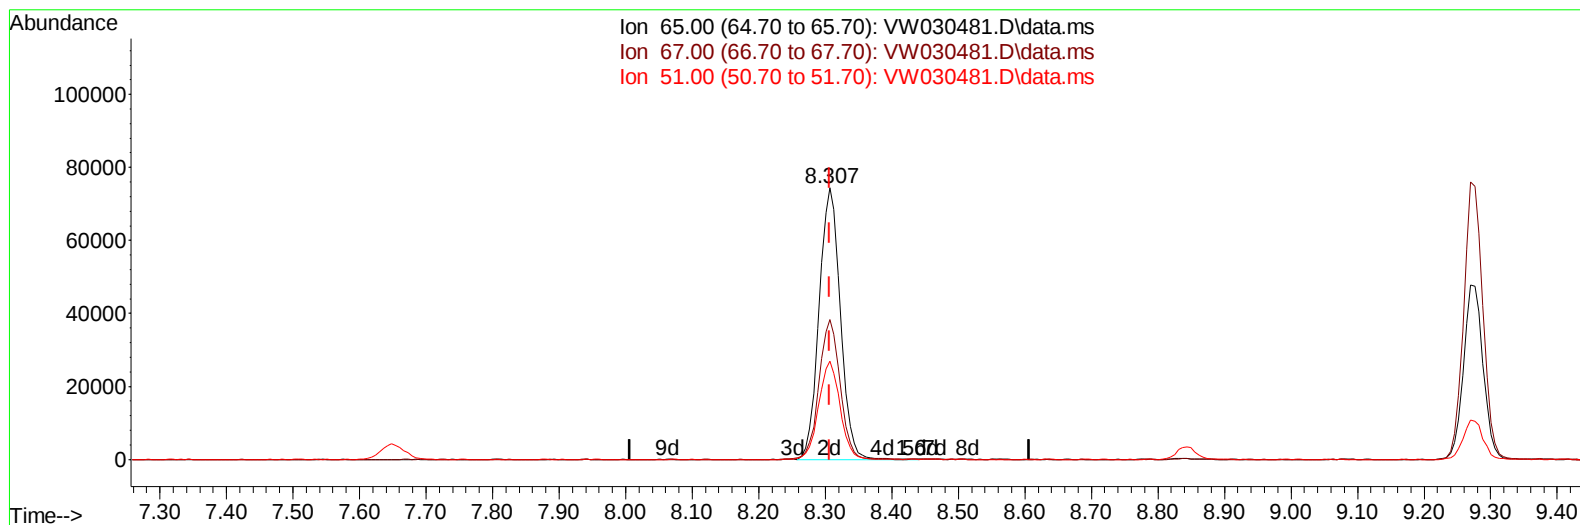

TIC: VW030481.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 36.02 ug/L m

response 165334

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.04#
51.00	109.40	0.09#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100924\
 Data File : VW030481.D
 Acq On : 09 Oct 2024 18:23
 Operator : SY/MD
 Sample : P4346-07
 Misc : 3.42g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW9

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:30:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		308643	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		200039	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		54179	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		142175	29.306	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	117.240%	
7) Chloroethane-d5	2.899	69		126588	34.471	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	137.880%	
11) 1,1-Dichloroethene-d2	4.021	65		55091	27.302	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	109.200%	
21) 2-Butanone-d5	7.075	46		55969	64.106	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	128.220%	
24) Chloroform-d	7.648	84		247284	28.016	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	112.080%	
26) 1,2-Dichloroethane-d4	8.307	65		165334m	36.022	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	144.080%#	
32) Benzene-d6	8.276	84		437563	37.688	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	150.760%#	
36) 1,2-Dichloropropane-d6	9.270	67		152190	44.660	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	178.640%#	
41) Toluene-d8	10.325	98		272326	25.694	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	102.760%	
43) trans-1,3-Dichloroprop...	10.575	79		41097	28.801	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	115.200%	
47) 2-Hexanone-d5	10.922	63		45454	103.561	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	207.120%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		109242	43.651	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	174.600%#	
66) 1,2-Dichlorobenzene-d4	13.849	152		53896	29.400	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	117.600%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030481.D
Acq On : 09 Oct 2024 18:23
Operator : SY/MD
Sample : P4346-07
Misc : 3.42g/10mL/MSVOA_W/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW9

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:30:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

