




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030483.D
 Acq On : 09 Oct 2024 19:11
 Operator : SY/MD
 Sample : P4346-09
 Misc : 2.84g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW9MSD

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

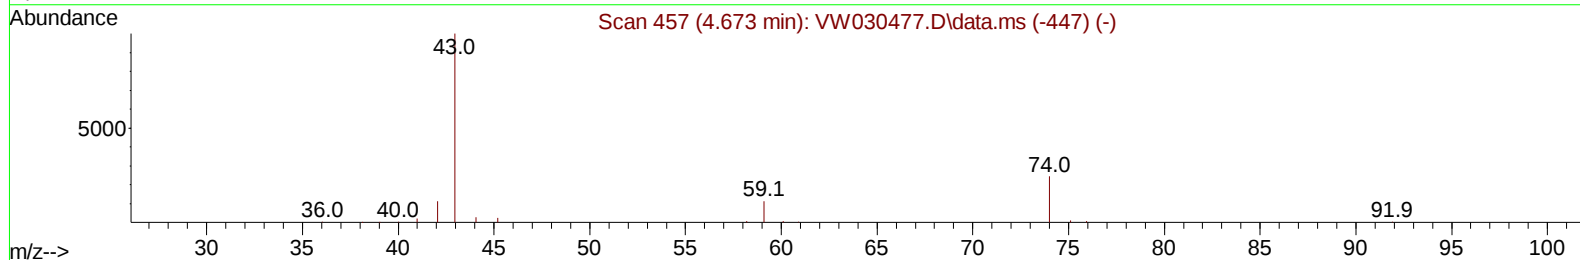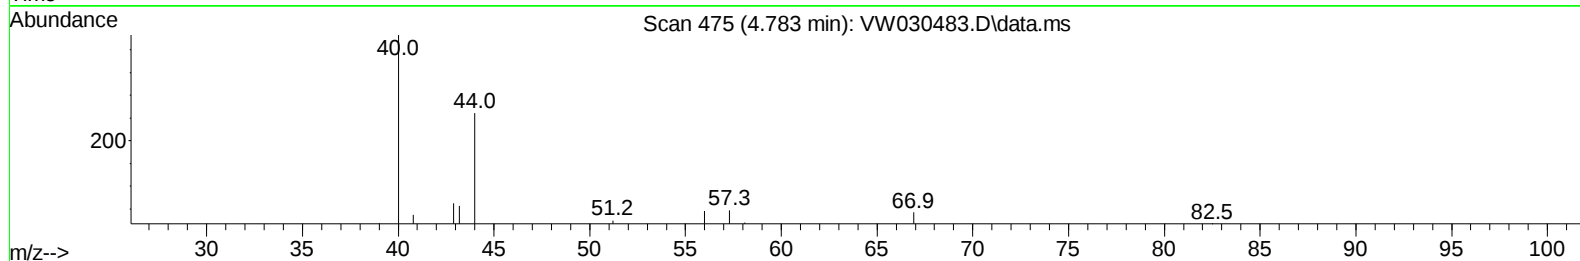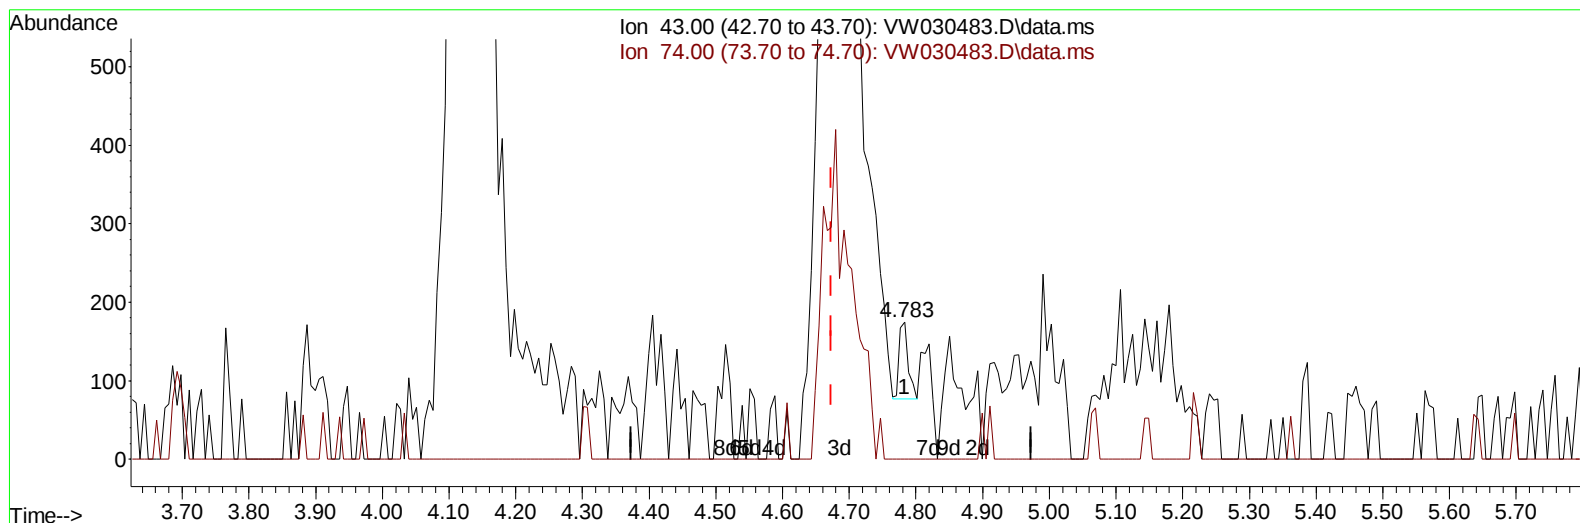

TIC: VW030483.D\data.ms

(15) Methyl Acetate (T)

4.783min (+ 0.110) 0.06 ug/L

response 89

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.10	21.35
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030483.D
 Acq On : 09 Oct 2024 19:11
 Operator : SY/MD
 Sample : P4346-09
 Misc : 2.84g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW9MSD

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

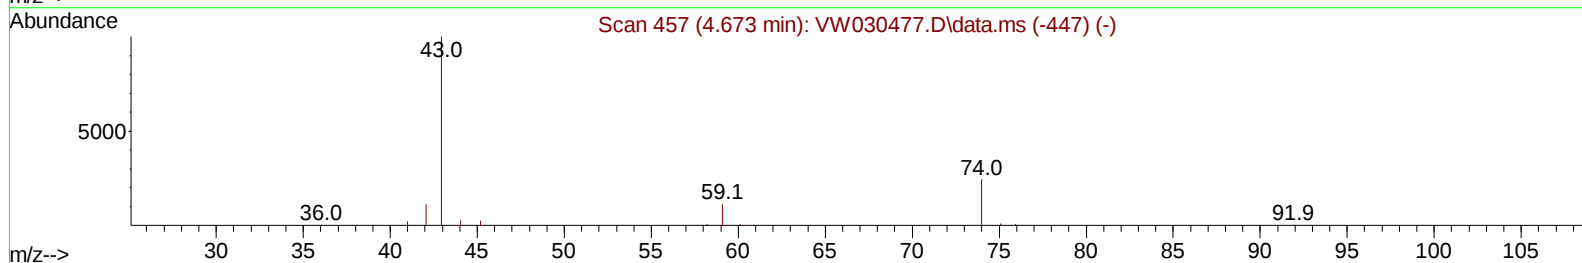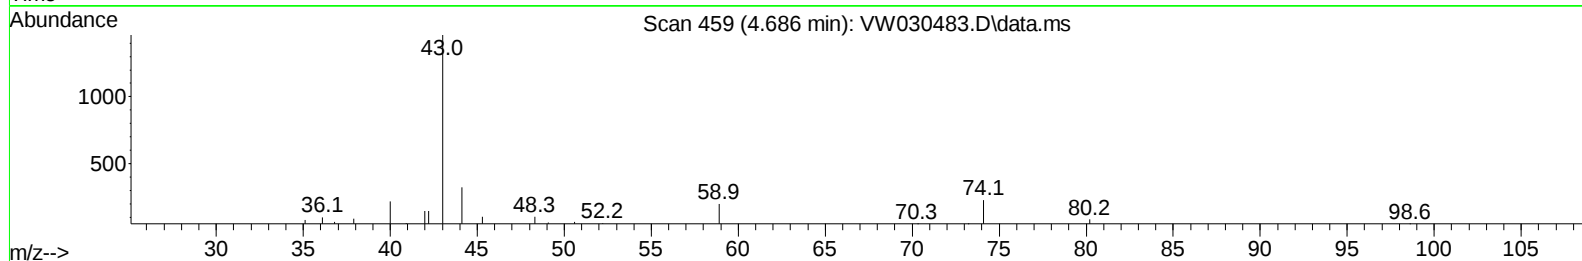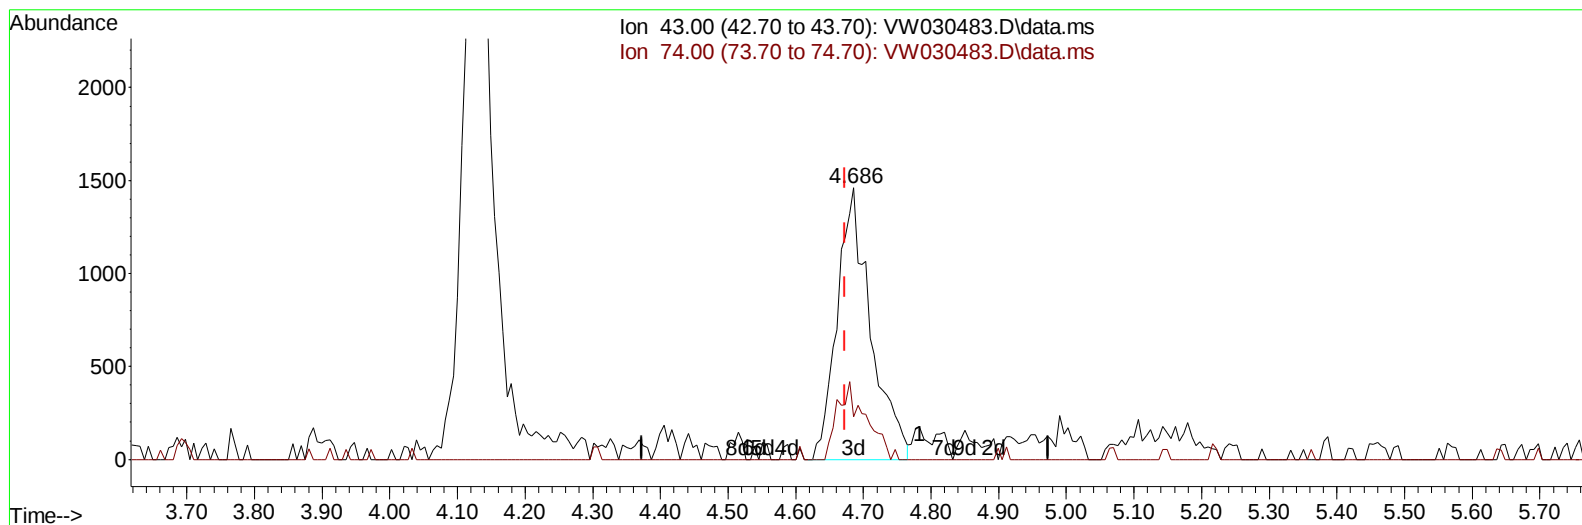

TIC: VW030483.D\data.ms

(15) Methyl Acetate (T)

4.686min (+ 0.012) 3.49 ug/L m

response 5014

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.10	0.38#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100924\
 Data File : VW030483.D
 Acq On : 09 Oct 2024 19:11
 Operator : SY/MD
 Sample : P4346-09
 Misc : 2.84g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW9MSD

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:31:06 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		280963	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		194198	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		62118	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		131755	29.834	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	119.320%	
7) Chloroethane-d5	2.899	69		116647	34.893	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	139.560%	
11) 1,1-Dichloroethene-d2	4.027	65		49910	27.171	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	108.680%	
21) 2-Butanone-d5	7.081	46		56592	71.206	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	142.420%#	
24) Chloroform-d	7.655	84		233441	29.053	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	116.200%	
26) 1,2-Dichloroethane-d4	8.307	65		155698	37.264	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	149.040%#	
32) Benzene-d6	8.276	84		408547	36.247	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	145.000%#	
36) 1,2-Dichloropropane-d6	9.276	67		142483	43.070	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	172.280%#	
41) Toluene-d8	10.325	98		269039	26.147	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	104.600%	
43) trans-1,3-Dichloroprop...	10.581	79		41758	30.144	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	120.560%	
47) 2-Hexanone-d5	10.922	63		46103	108.199	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	216.400%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		113475	46.706	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	186.840%#	
66) 1,2-Dichlorobenzene-d4	13.849	152		67484	32.107	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	128.440%#	
Target Compounds							
13) Acetone	4.119	43		9370	8.053	ug/L	98
15) Methyl Acetate	4.686	43		5014m	3.488	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030483.D
Acq On : 09 Oct 2024 19:11
Operator : SY/MD
Sample : P4346-09
Misc : 2.84g/10mL/MSVOA_W/SoIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAW9MSD

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:31:06 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

