




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030486.D
 Acq On : 09 Oct 2024 20:23
 Operator : SY/MD
 Sample : P4346-12
 Misc : 2.82g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX2

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

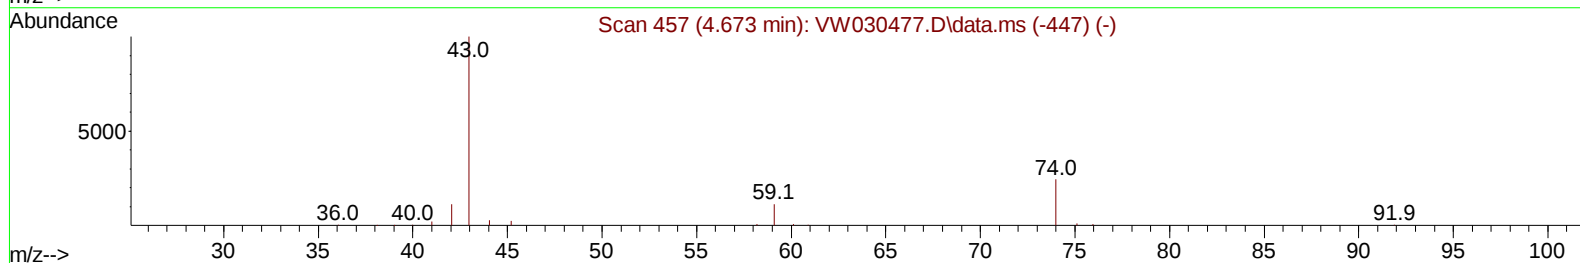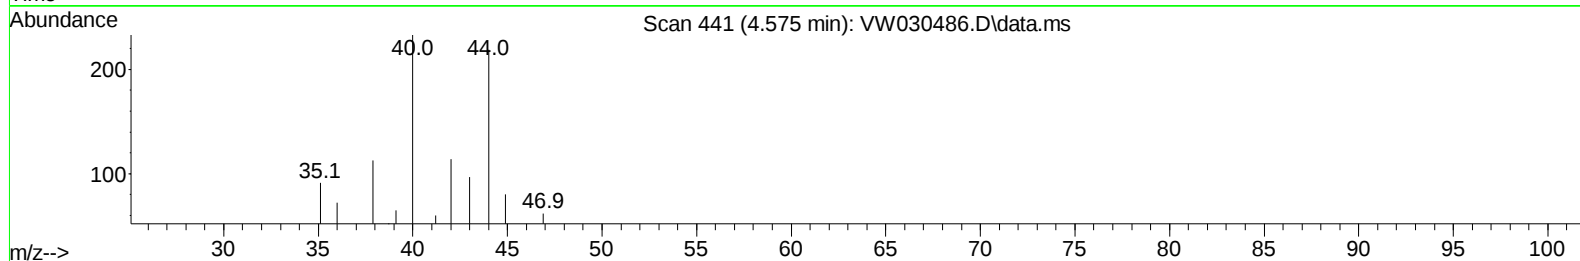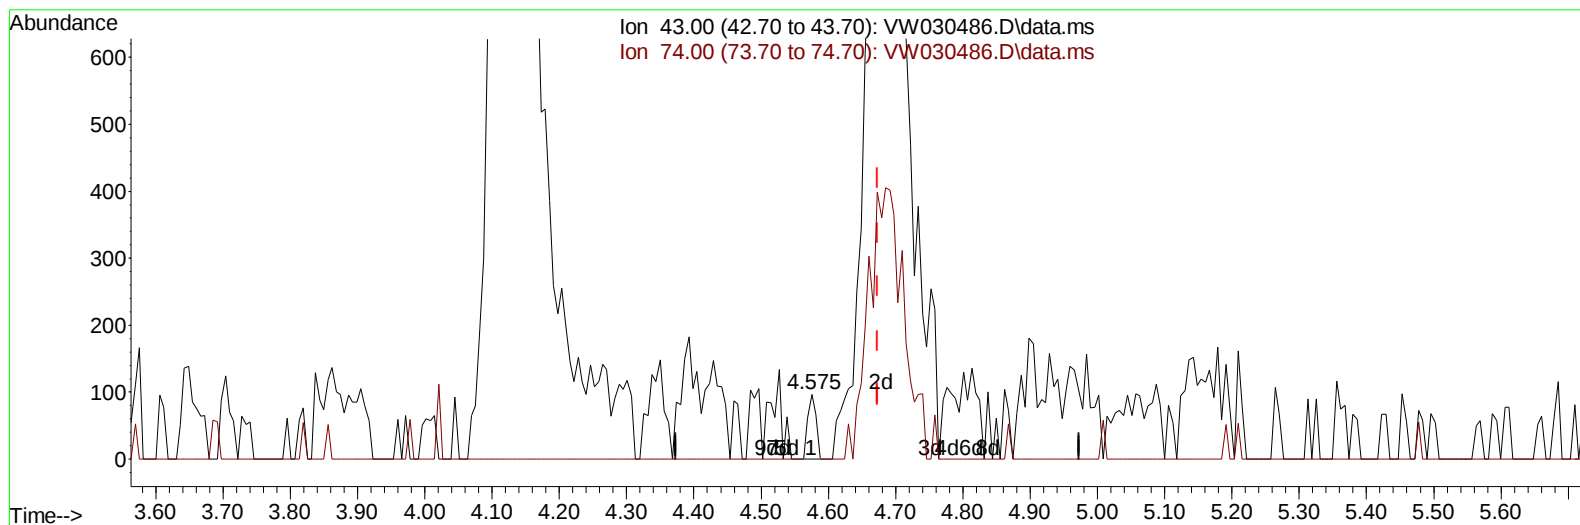

TIC: VW030486.D\data.ms

(15) Methyl Acetate (T)

4.575min (-0.098) 0.05 ug/L

response 82

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.10	23.17
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030486.D
 Acq On : 09 Oct 2024 20:23
 Operator : SY/MD
 Sample : P4346-12
 Misc : 2.82g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX2

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

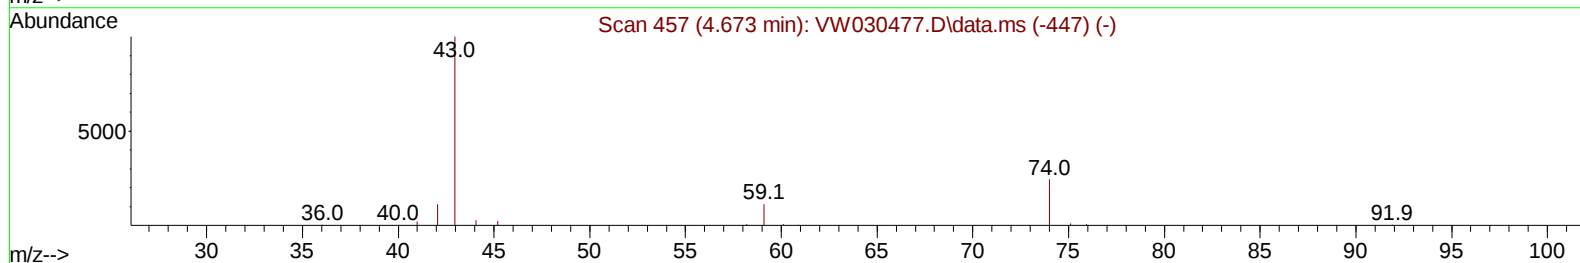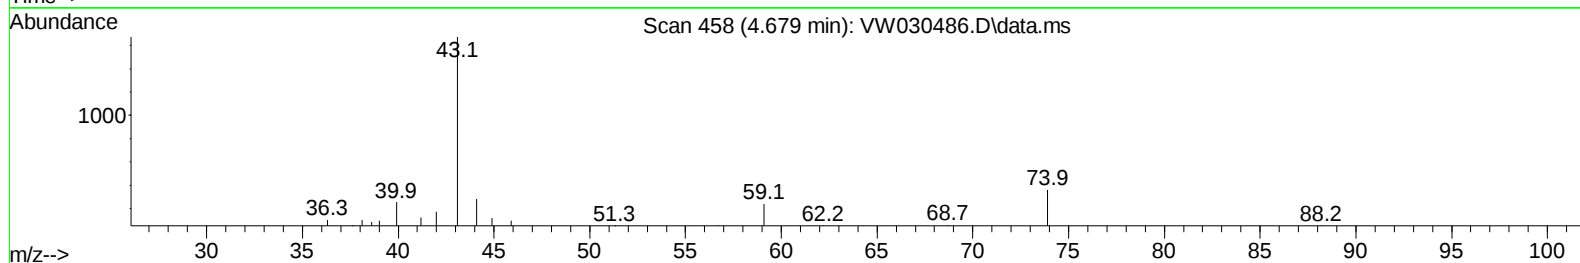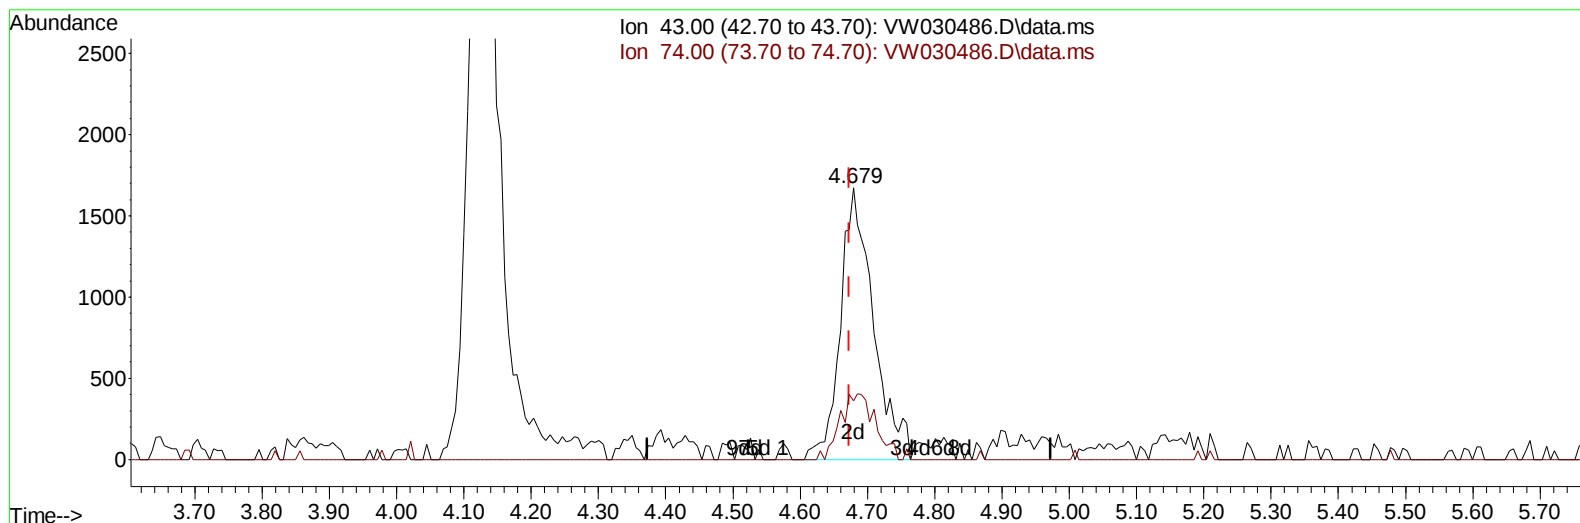

TIC: VW030486.D\data.ms

(15) Methyl Acetate (T)

4.679min (+ 0.006) 3.63 ug/L m

response 5678

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.10	0.33#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100924\
 Data File : VW030486.D
 Acq On : 09 Oct 2024 20:23
 Operator : SY/MD
 Sample : P4346-12
 Misc : 2.82g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX2

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:31:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		305476	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		197255	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152		42191	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.368	65		136100	28.345	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	113.360%	
7) Chloroethane-d5	2.899	69		120902	33.264	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	133.040%	
11) 1,1-Dichloroethene-d2	4.021	65		54842	27.461	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	109.840%	
21) 2-Butanone-d5	7.081	46		62491	72.318	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	144.640%#	
24) Chloroform-d	7.654	84		255816	29.283	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	117.120%	
26) 1,2-Dichloroethane-d4	8.306	65		166055	36.554	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	146.200%#	
32) Benzene-d6	8.276	84		462461	40.394	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	161.560%#	
36) 1,2-Dichloropropane-d6	9.270	67		153654	45.726	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	182.920%#	
41) Toluene-d8	10.324	98		325675	31.161	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	124.640%	
43) trans-1,3-Dichloroprop...	10.580	79		41525	29.512	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	118.040%	
47) 2-Hexanone-d5	10.922	63		48858	112.887	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	225.780%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		119437	48.398	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	193.600%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		78322	54.864	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	219.440%#	
Target Compounds							
13) Acetone	4.124	43		13135	10.383	ug/L	99
15) Methyl Acetate	4.679	43		5678m	3.633	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030486.D
Acq On : 09 Oct 2024 20:23
Operator : SY/MD
Sample : P4346-12
Misc : 2.82g/10mL/MSVOA_W/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX2

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:31:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

