




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030487.D
Acq On : 09 Oct 2024 20:47
Operator : SY/MD
Sample : P4346-13
Misc : 3.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX3

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

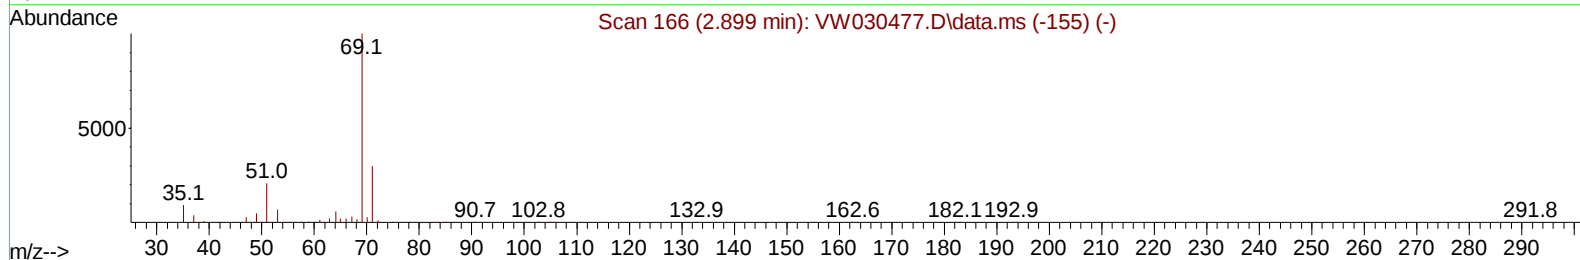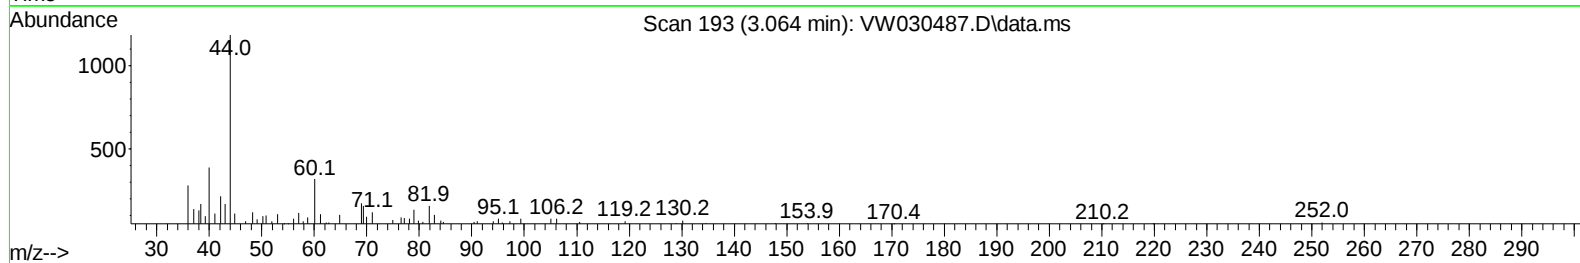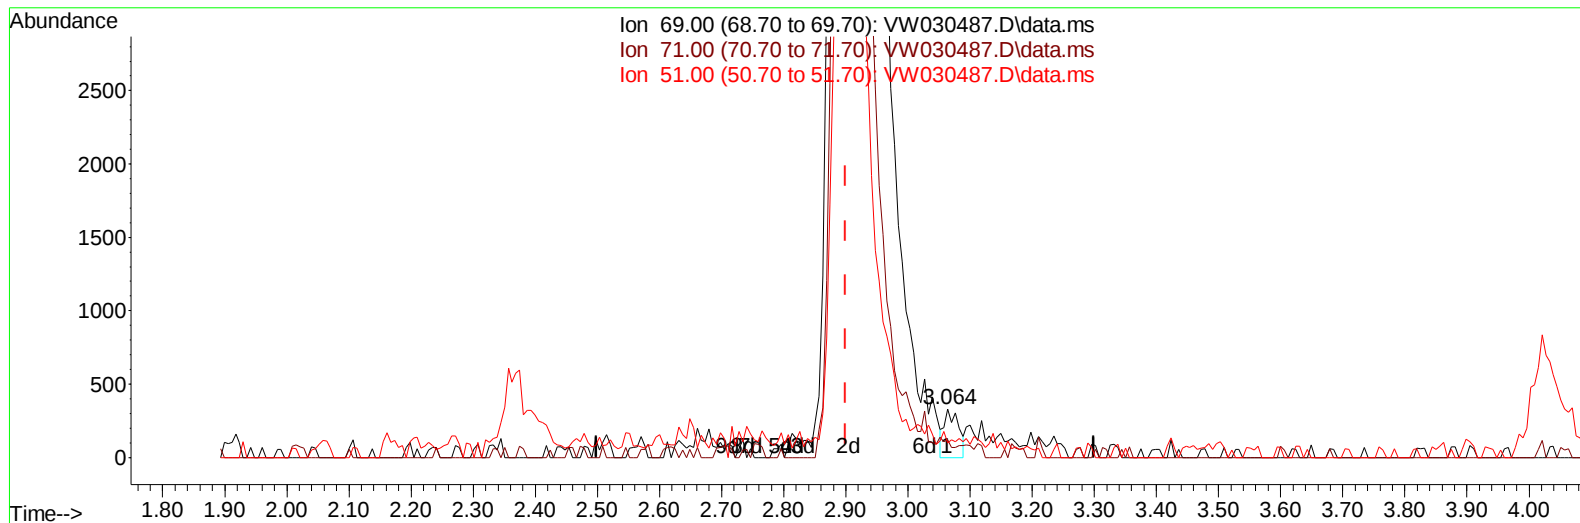

TIC: VW030487.D\data.ms

(7) Chloroethane-d5 (S)

3.064min (+ 0.165) 0.15 ug/L

response 518

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	30.50
51.00	10.20	8.30
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030487.D
 Acq On : 09 Oct 2024 20:47
 Operator : SY/MD
 Sample : P4346-13
 Misc : 3.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX3

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

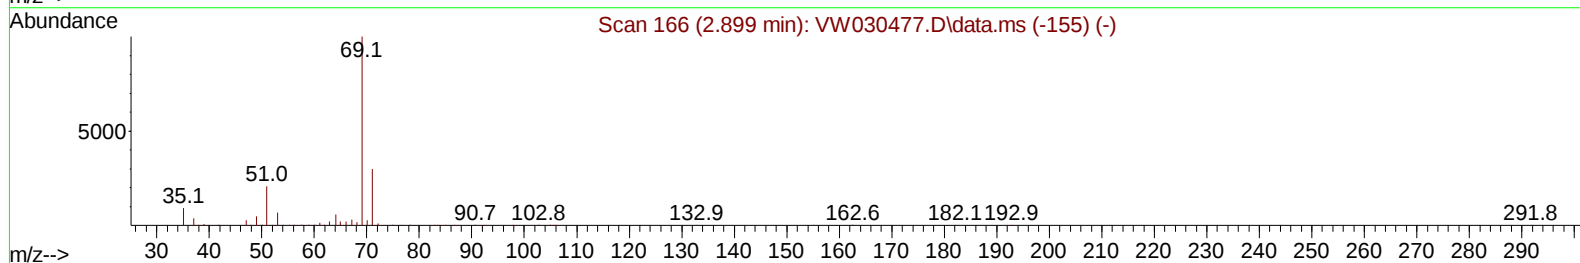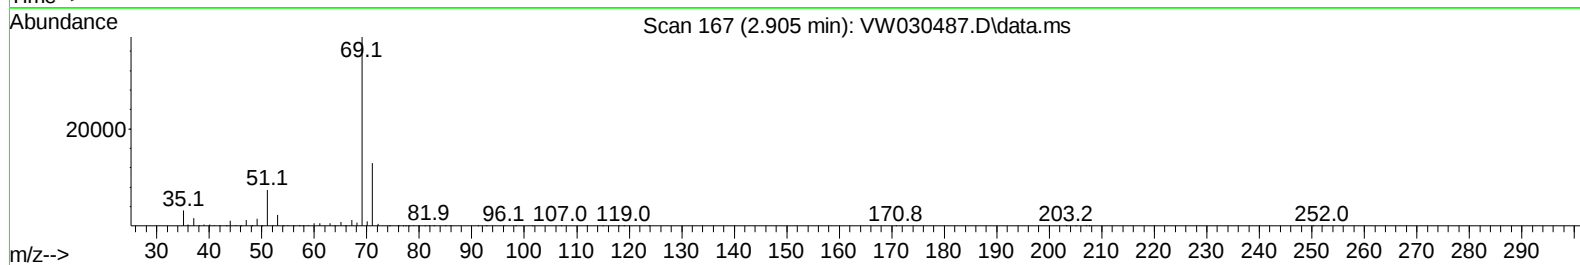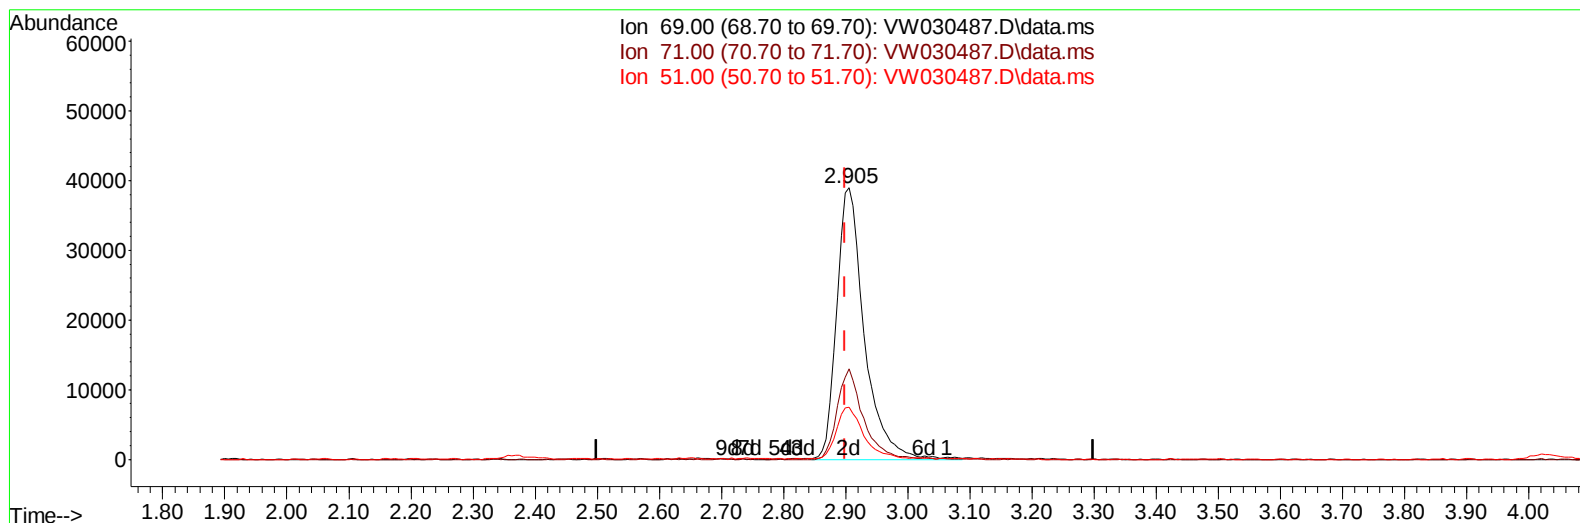

TIC: VW030487.D\data.ms

(7) Chloroethane-d5 (S)

2.905min (+ 0.006) 34.19 ug/L m

response 120652

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	0.13#
51.00	10.20	0.04#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030487.D
Acq On : 09 Oct 2024 20:47
Operator : SY/MD
Sample : P4346-13
Misc : 3.03g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX3

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

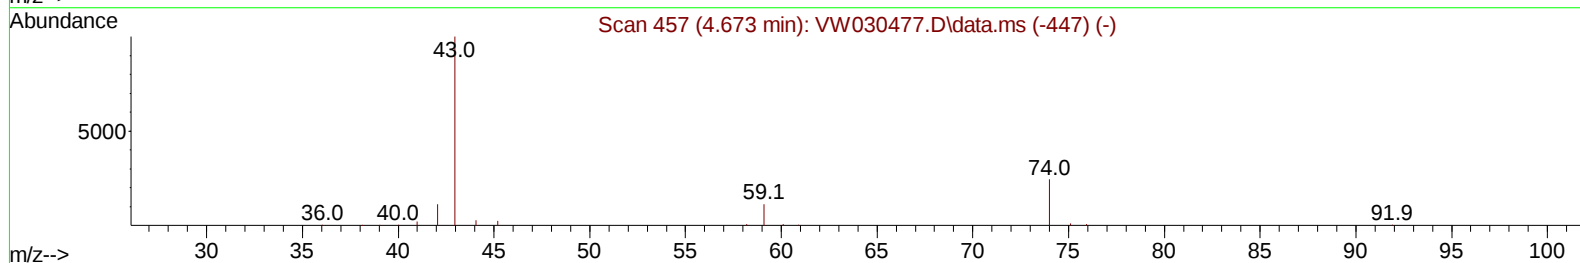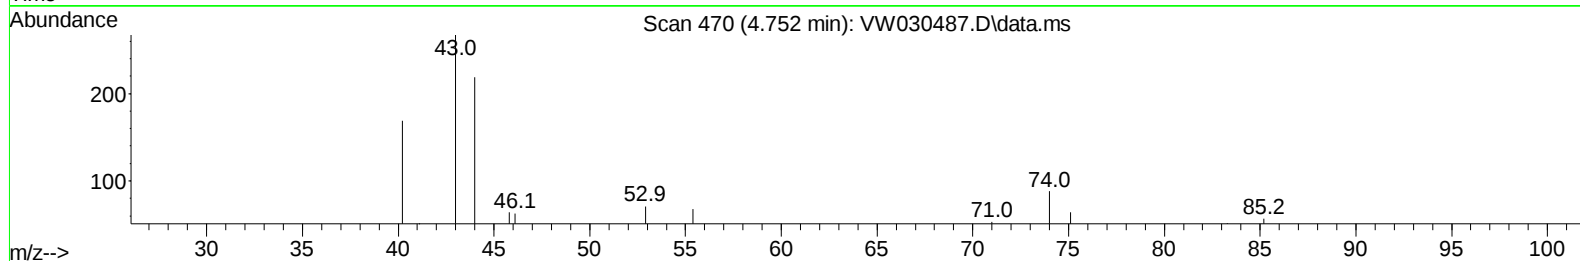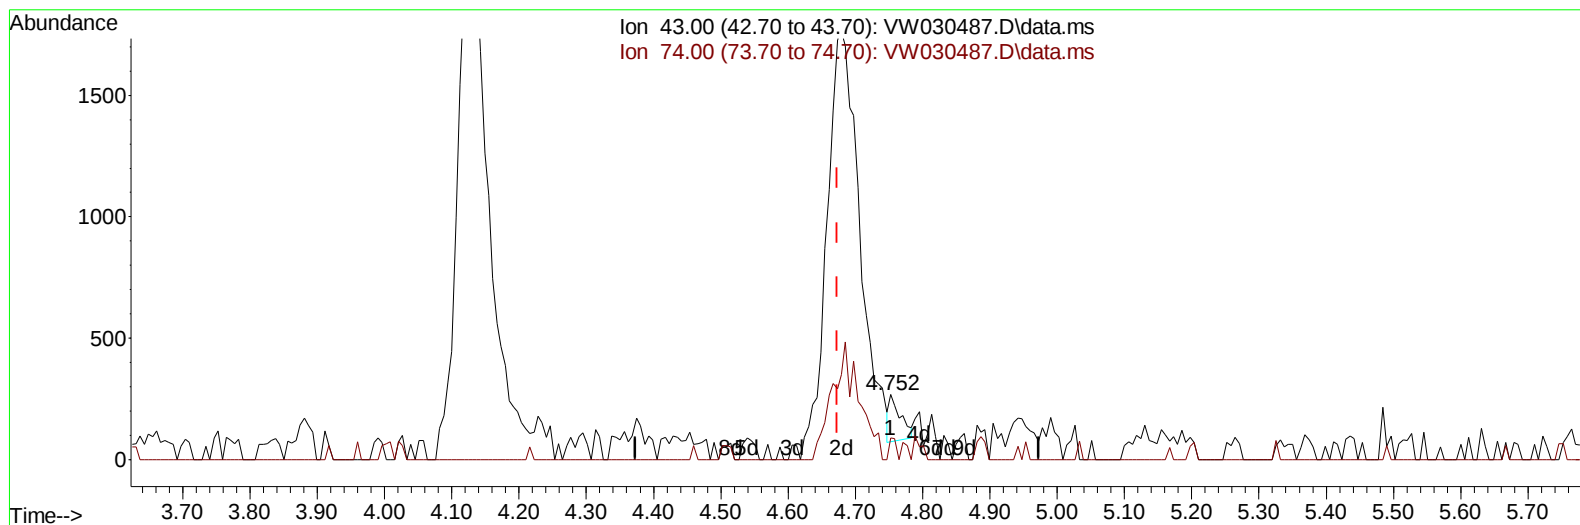

TIC: VW030487.D\data.ms

(15) Methyl Acetate (T)

4.752min (+ 0.079) 0.15 ug/L

response 230

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.10	27.83
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030487.D
 Acq On : 09 Oct 2024 20:47
 Operator : SY/MD
 Sample : P4346-13
 Misc : 3.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX3

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

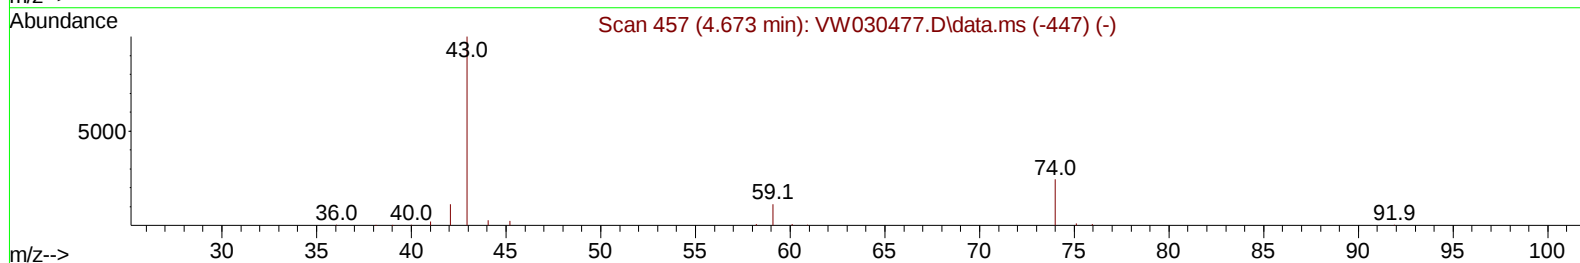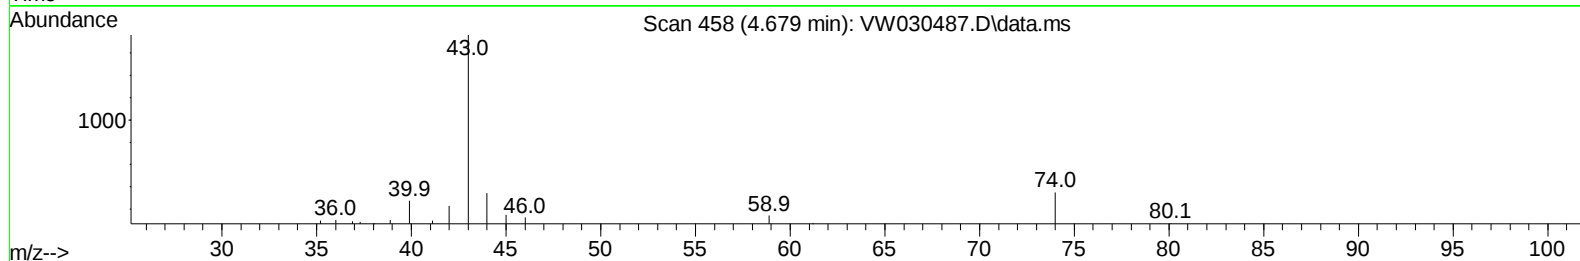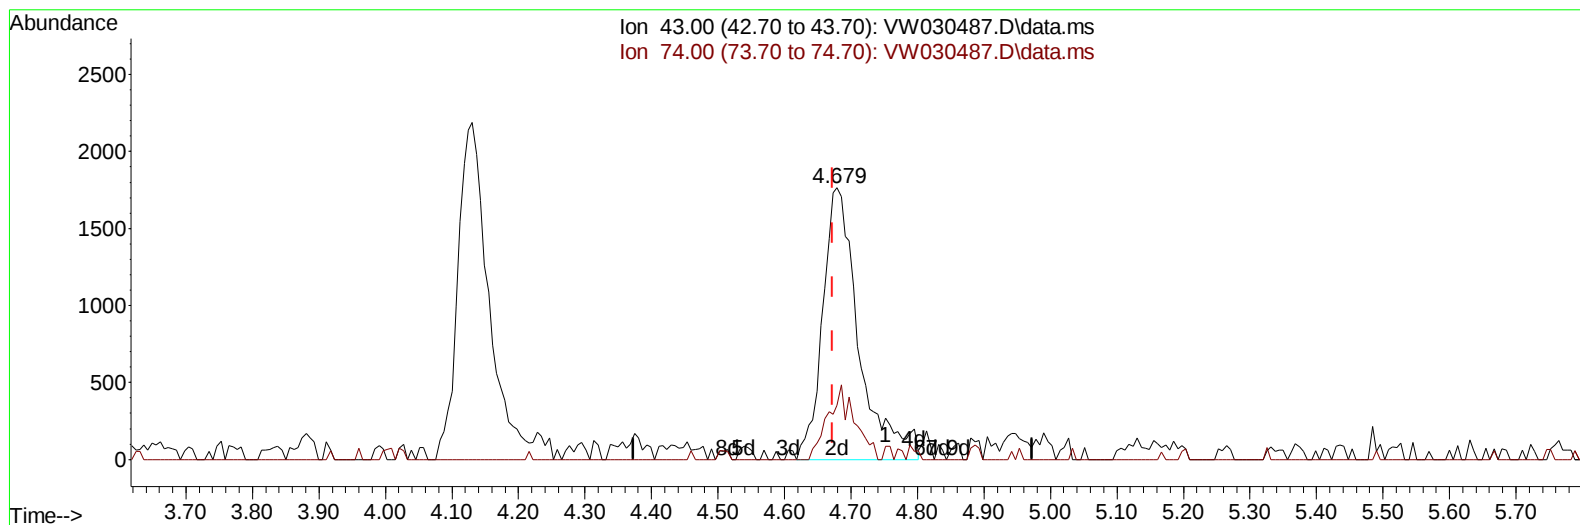

TIC: VW030487.D\data.ms

(15) Methyl Acetate (T)

4.679min (+ 0.006) 4.39 ug/L m

response 6661

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.10	0.96#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100924\
 Data File : VW030487.D
 Acq On : 09 Oct 2024 20:47
 Operator : SY/MD
 Sample : P4346-13
 Misc : 3.03g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX3

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		296612	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		205371	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		65959	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		137063	29.398	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	117.600%	
7) Chloroethane-d5	2.905	69		120652m	34.187	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	136.760%	
11) 1,1-Dichloroethene-d2	4.021	65		52061	26.847	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	107.400%	
21) 2-Butanone-d5	7.081	46		44800	53.395	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	106.780%	
24) Chloroform-d	7.654	84		235227	27.731	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	110.920%	
26) 1,2-Dichloroethane-d4	8.307	65		153991	34.911	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	139.640%#	
32) Benzene-d6	8.276	84		423587	35.537	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	142.160%#	
36) 1,2-Dichloropropane-d6	9.276	67		144025	41.167	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	164.680%#	
41) Toluene-d8	10.325	98		276461	25.407	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	101.640%	
43) trans-1,3-Dichloroprop...	10.581	79		40964	27.962	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	111.840%	
47) 2-Hexanone-d5	10.922	63		37443	83.094	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	166.180%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		107233	41.736	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	166.960%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		65047	29.146	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	116.600%	
Target Compounds							
13) Acetone	4.131	43		6972	5.676	ug/L	70
15) Methyl Acetate	4.679	43		6661m	4.390	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030487.D
Acq On : 09 Oct 2024 20:47
Operator : SY/MD
Sample : P4346-13
Misc : 3.03g/10mL/MSVOA_W/SoIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX3

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:32:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

