




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030489.D
Acq On : 09 Oct 2024 21:35
Operator : SY/MD
Sample : P4346-15
Misc : 2.87g/10mL/MSVOA_W/SOIL/A
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX5

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:32:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

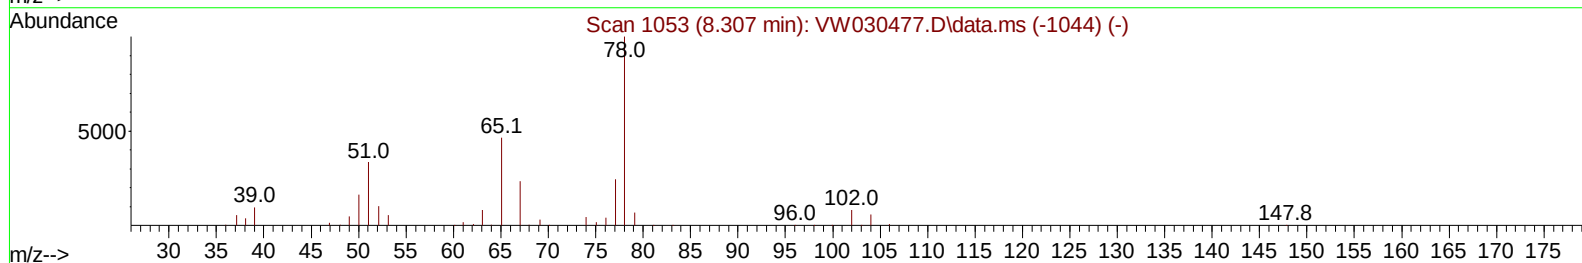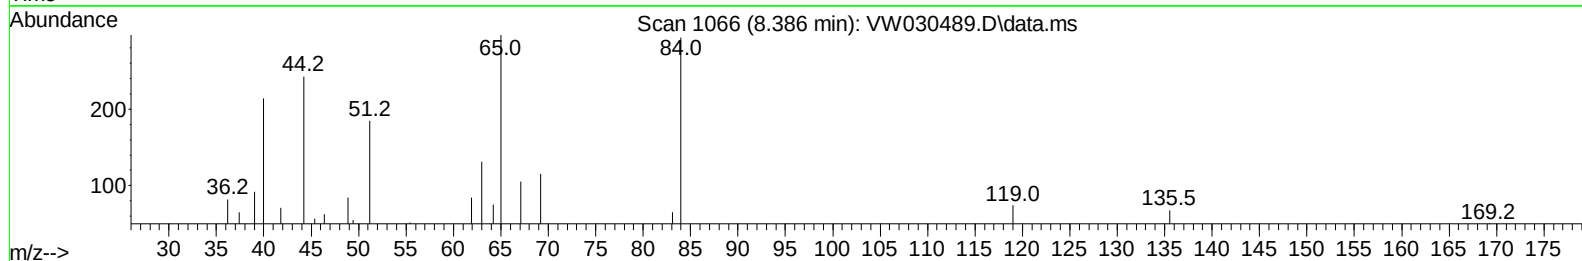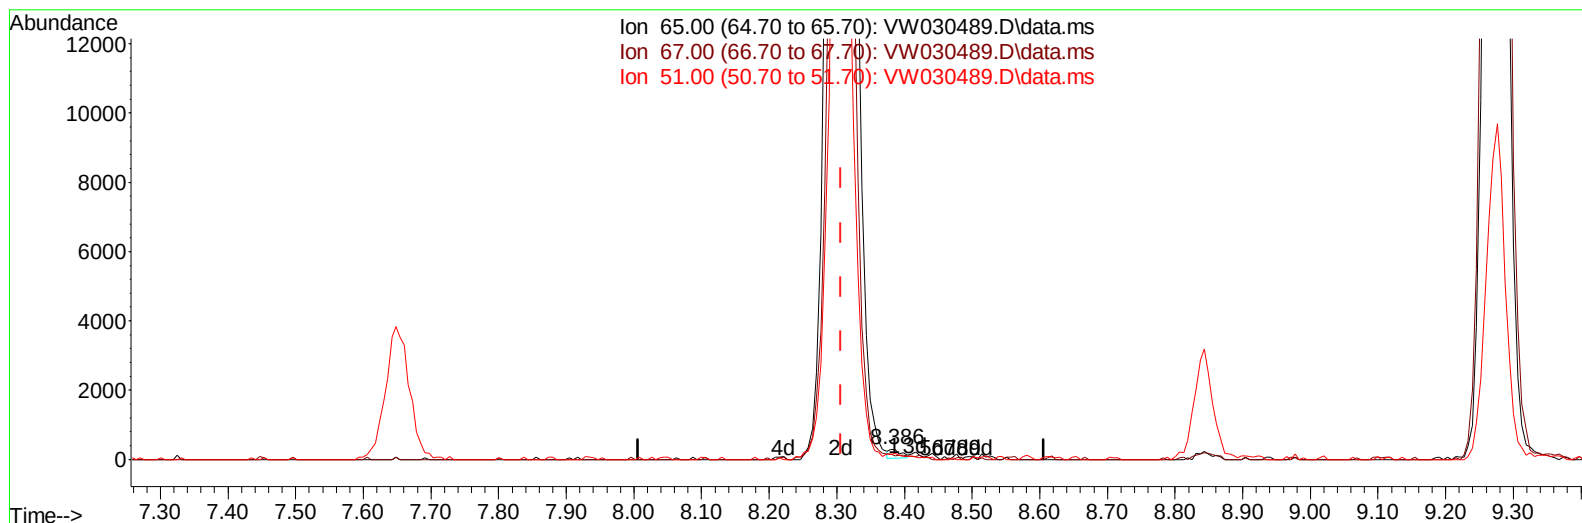

TIC: VW030489.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.386min (+ 0.079) 0.08 ug/L

response 312

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	60.90
51.00	109.40	78.85
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030489.D
 Acq On : 09 Oct 2024 21:35
 Operator : SY/MD
 Sample : P4346-15
 Misc : 2.87g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX5

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

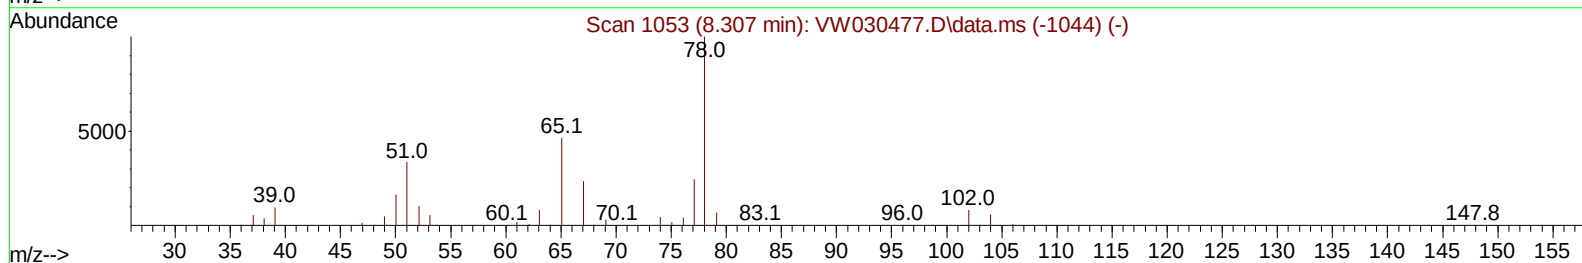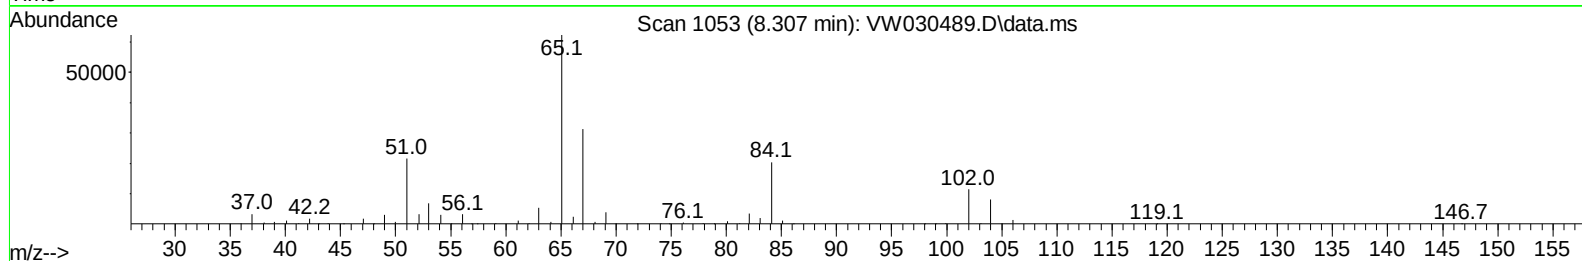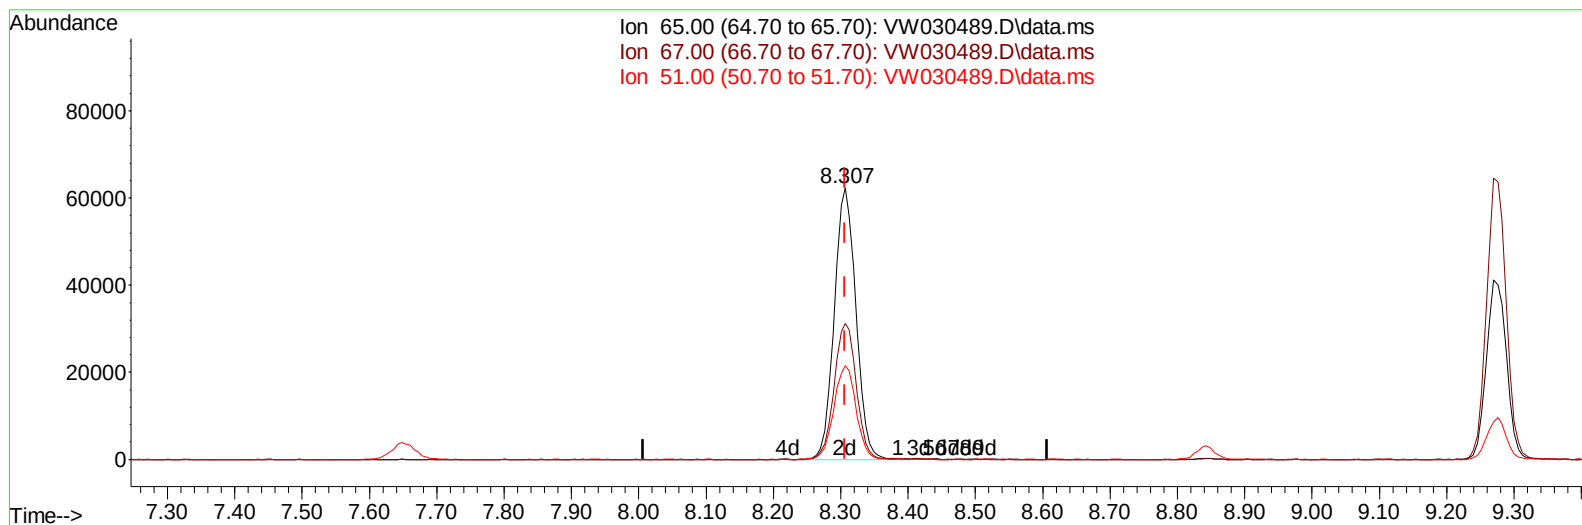

TIC: VW030489.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 34.28 ug/L m

response 139307

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.90	0.14#
51.00	109.40	0.18#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100924\
 Data File : VW030489.D
 Acq On : 09 Oct 2024 21:35
 Operator : SY/MD
 Sample : P4346-15
 Misc : 2.87g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX5

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	273283	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	173202	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	46937	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	131048	30.508	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	122.040%	
7) Chloroethane-d5	2.899	69	113511	34.909	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	139.640%	
11) 1,1-Dichloroethene-d2	4.021	65	48384	27.081	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	108.320%	
21) 2-Butanone-d5	7.075	46	40388	52.245	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	104.500%	
24) Chloroform-d	7.648	84	221963	28.401	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	113.600%	
26) 1,2-Dichloroethane-d4	8.307	65	139307m	34.278	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	137.120%#	
32) Benzene-d6	8.276	84	382689	38.069	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	152.280%#	
36) 1,2-Dichloropropane-d6	9.270	67	130548	44.246	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	177.000%#	
41) Toluene-d8	10.325	98	250728	27.322	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	109.280%	
43) trans-1,3-Dichloroprop...	10.575	79	35982	29.124	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	116.480%	
47) 2-Hexanone-d5	10.922	63	31472	82.815	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	165.640%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	99750	46.034	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	184.120%#	
66) 1,2-Dichlorobenzene-d4	13.848	152	55331	34.840	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	139.360%#	
Target Compounds						
15) Methyl Acetate	4.679	43	6257	4.476	ug/L #	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030489.D
Acq On : 09 Oct 2024 21:35
Operator : SY/MD
Sample : P4346-15
Misc : 2.87g/10mL/MSVOA_W/SOIL/A
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX5

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

