




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030490.D
 Acq On : 09 Oct 2024 21:59
 Operator : SY/MD
 Sample : P4346-17
 Misc : 5.46g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX7

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

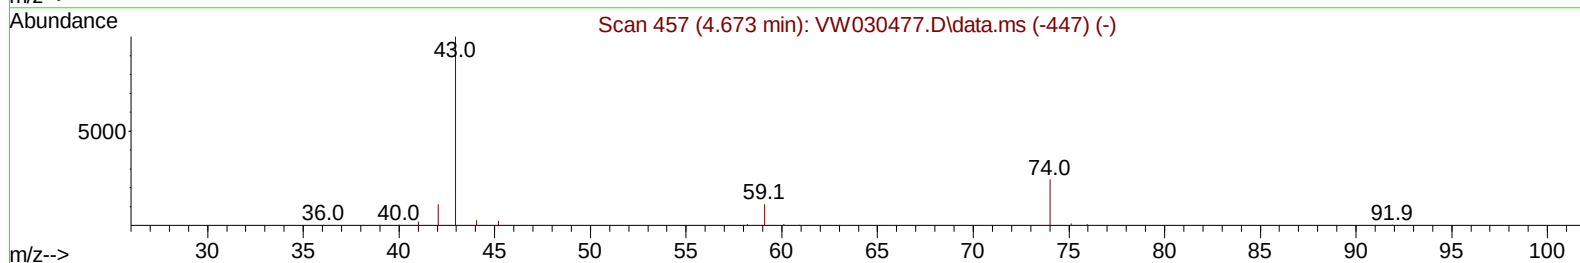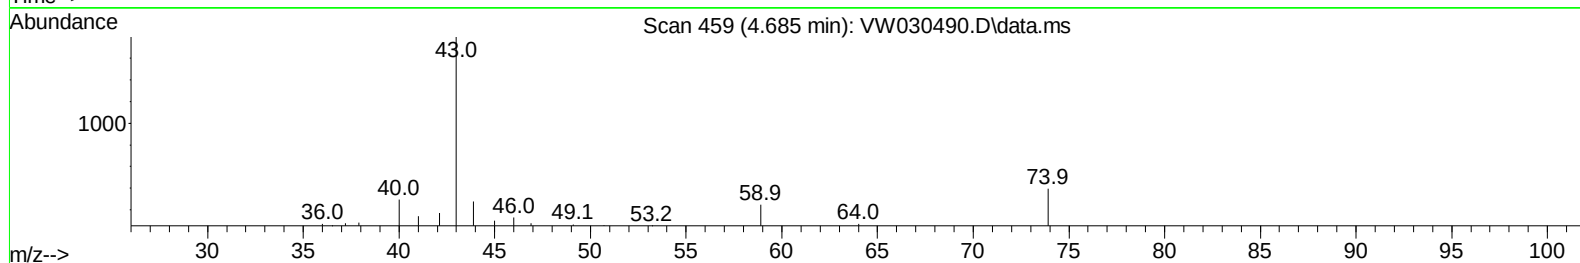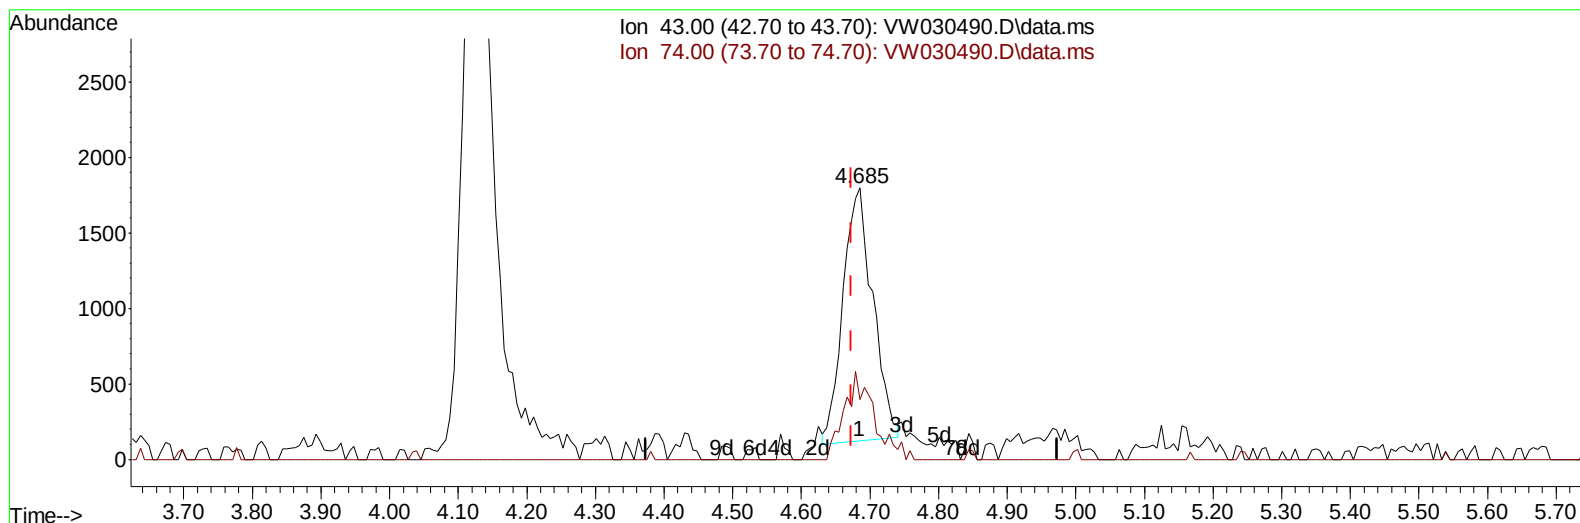

TIC: VW030490.D\data.ms

(15) Methyl Acetate (T)

4.685min (+ 0.012) 3.14 ug/L

response 5045

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.10	2.40#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030490.D
Acq On : 09 Oct 2024 21:59
Operator : SY/MD
Sample : P4346-17
Misc : 5.46g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX7

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

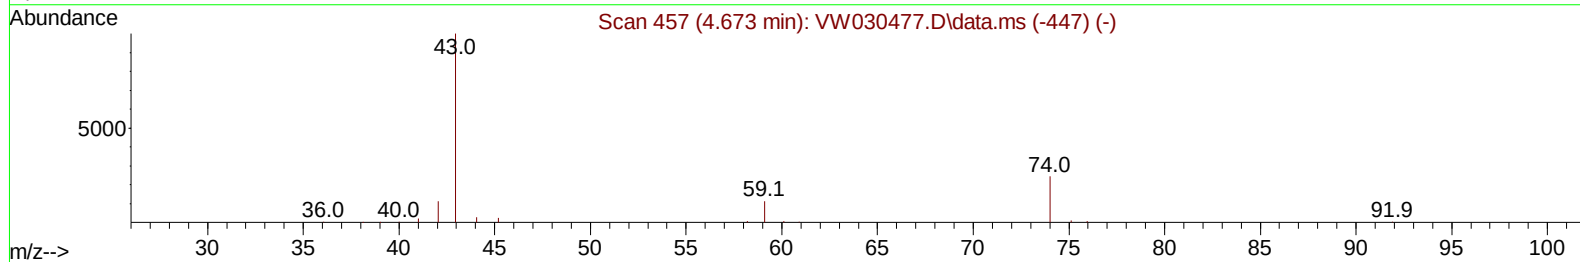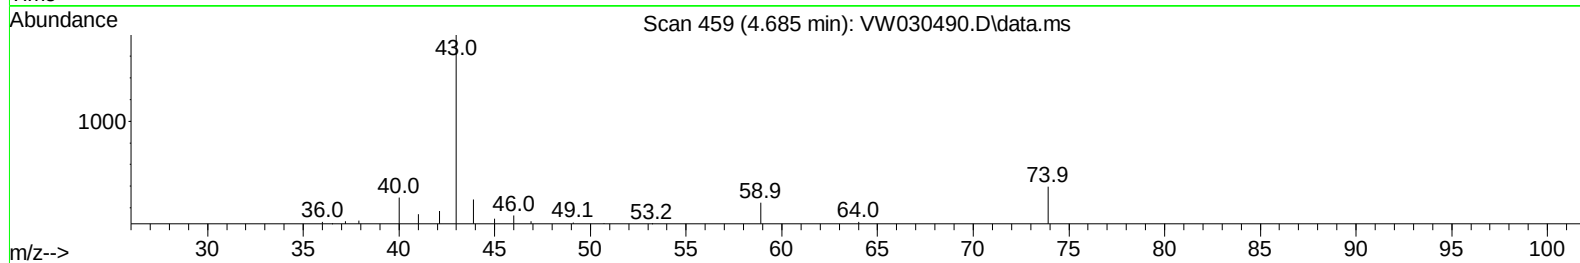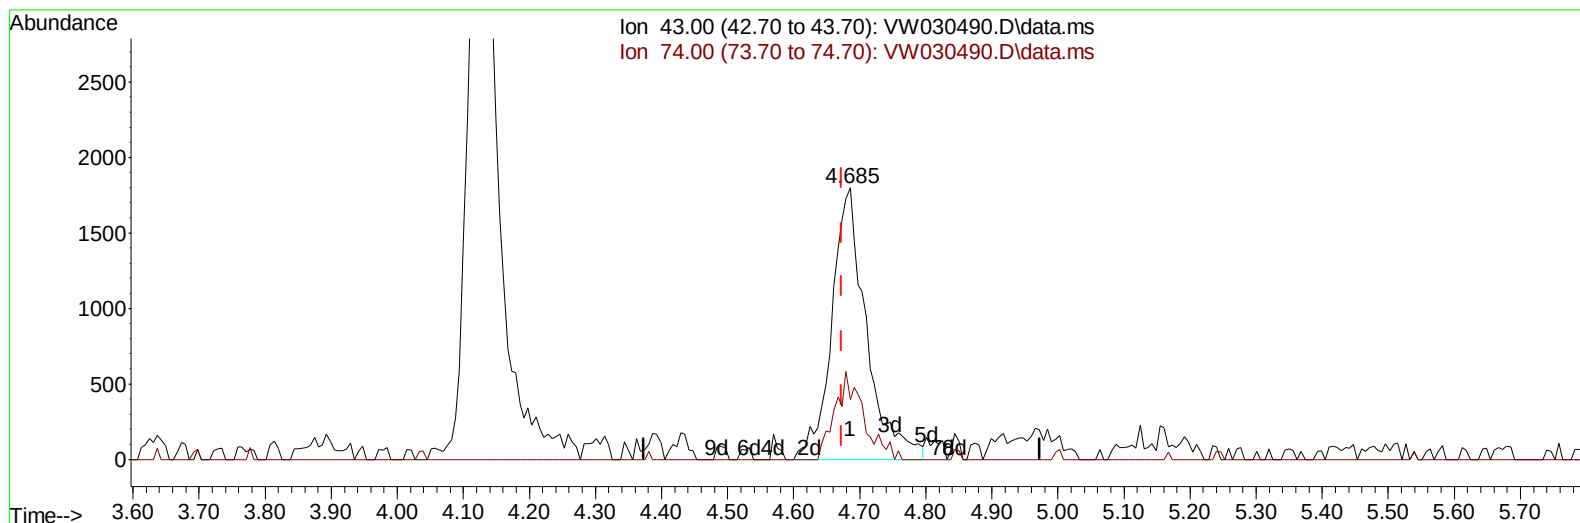

TIC: VW030490.D\data.ms

(15) Methyl Acetate (T)

4.685min (+ 0.012) 4.06 ug/L m

response 6529

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.10	1.85#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100924\
 Data File : VW030490.D
 Acq On : 09 Oct 2024 21:59
 Operator : SY/MD
 Sample : P4346-17
 Misc : 5.46g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX7

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		314515	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		201691	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		55317	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		137690	27.852	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	111.400%	
7) Chloroethane-d5	2.905	69		124966	33.394	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	133.560%	
11) 1,1-Dichloroethene-d2	4.027	65		56130	27.298	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	109.200%	
21) 2-Butanone-d5	7.081	46		53377	59.996	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	120.000%	
24) Chloroform-d	7.648	84		240600	26.750	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	107.000%	
26) 1,2-Dichloroethane-d4	8.307	65		157084	33.585	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	134.360%#	
32) Benzene-d6	8.276	84		444382	37.961	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	151.840%#	
36) 1,2-Dichloropropane-d6	9.276	67		147125	42.821	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	171.280%#	
41) Toluene-d8	10.325	98		287200	26.875	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	107.520%	
43) trans-1,3-Dichloroprop...	10.581	79		33536	23.310	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	93.240%	
47) 2-Hexanone-d5	10.922	63		38817	87.715	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	175.420%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		103015	40.826	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	163.320%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		61977	33.113	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	132.440%#	
Target Compounds							
13) Acetone	4.125	43		12272	9.422	ug/L	95
15) Methyl Acetate	4.685	43		6529m	4.058	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030490.D
Acq On : 09 Oct 2024 21:59
Operator : SY/MD
Sample : P4346-17
Misc : 5.46g/10mL/MSVOA_W/SoIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX7

Manual IntegrationsAPPROVED

Quant Time: Oct 10 01:32:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

