

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030480.D
 Acq On : 09 Oct 2024 17:59
 Operator : SY/MD
 Sample : P4346-06
 Misc : 3.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW8

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

Quant Time: Oct 10 01:30:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	110921	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	96764	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	30067	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	33663	19.308	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 77.240%			
7) Chloroethane-d5	2.899	69	38816	29.411	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 117.640%			
11) 1,1-Dichloroethene-d2	4.021	65	15973	22.027	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 88.120%			
21) 2-Butanone-d5	7.081	46	32246	102.771	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 205.540%#			
24) Chloroform-d	7.648	84	107104	33.764	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 135.040%			
26) 1,2-Dichloroethane-d4	8.307	65	80256m	48.655	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 194.600%#			
32) Benzene-d6	8.276	84	174196	31.017	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 124.080%			
36) 1,2-Dichloropropane-d6	9.276	67	68216	41.383	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 165.520%#			
41) Toluene-d8	10.325	98	118661	23.145	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 92.560%			
43) trans-1,3-Dichloroprop...	10.575	79	22228	32.203	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 128.800%			
47) 2-Hexanone-d5	10.922	63	24794	116.781	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 233.560%#			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	61504	50.805	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 203.240%#			
66) 1,2-Dichlorobenzene-d4	13.848	152	35322	34.720	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 138.880%#			
Target Compounds					Qvalue	
13) Acetone	4.131	43	5570	12.126	ug/L	53

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030480.D
Acq On : 09 Oct 2024 17:59
Operator : SY/MD
Sample : P4346-06
Misc : 3.27g/10mL/MSVOA_W/SOIL/A
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
EOAW8

Quant Time: Oct 10 01:30:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Romaben Patel 10/10/2024
Supervised By :Mahesh Dadoda 10/10/2024

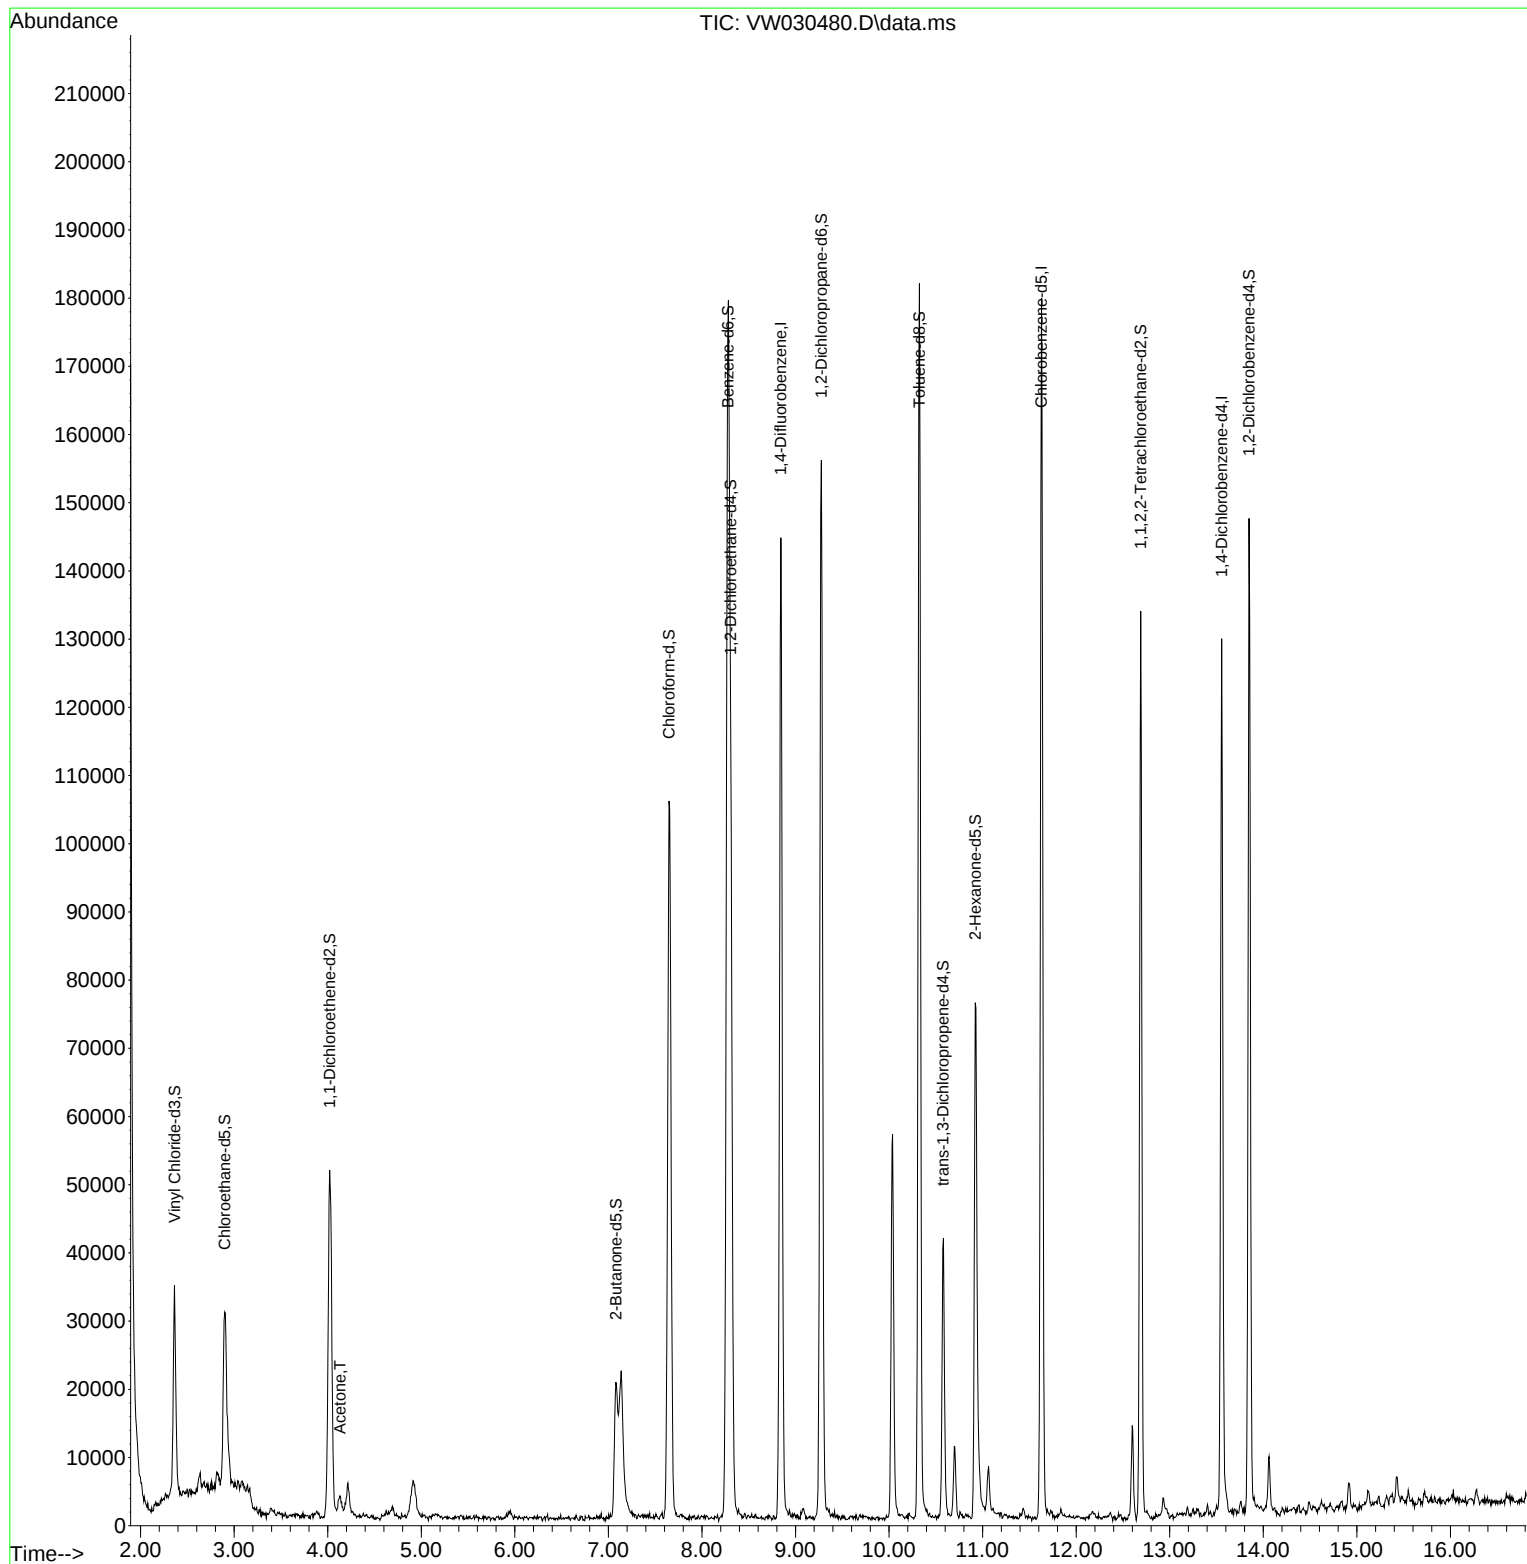

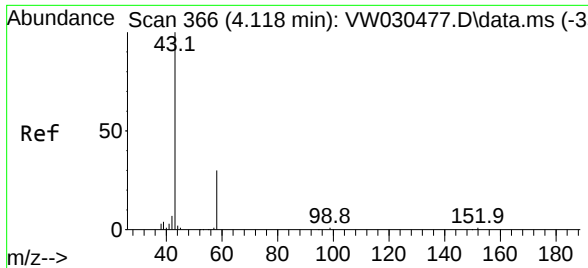

#13
 Acetone
 Concen: 12.126 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW030480.D
 Acq: 09 Oct 2024 17:59

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAW8

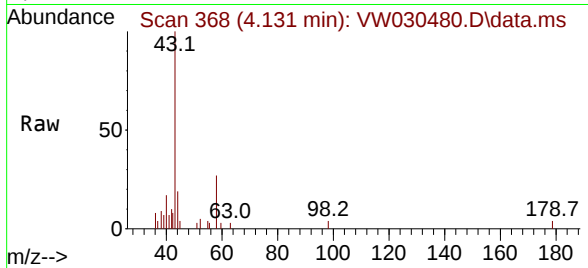

Tgt Ion: 43 Resp: 5570
 Ion Ratio Lower Upper
 43 100
 58 3.5 0.0 57.6

Manual Integrations
 APPROVED

Reviewed By :Romaben Patel 10/10/2024
 Supervised By :Mahesh Dadoda 10/10/2024

