

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030485.D
 Acq On : 09 Oct 2024 19:59
 Operator : SY/MD
 Sample : P4346-11
 Misc : 2.30g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX1

Quant Time: Oct 10 01:31:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	106024	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	73172	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	20939	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.363	65	57298	34.381	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 137.520%		
7) Chloroethane-d5		2.899	69	46526	36.882	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 147.520%		
11) 1,1-Dichloroethene-d2		4.021	65	20881	30.125	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 120.480%#		
21) 2-Butanone-d5		7.087	46	18327	61.108	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	= 122.220%		
24) Chloroform-d		7.654	84	85568	28.221	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 112.880%		
26) 1,2-Dichloroethane-d4		8.307	65	58361	37.015	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 148.080%#		
32) Benzene-d6		8.276	84	148079	34.868	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 139.480%#		
36) 1,2-Dichloropropane-d6		9.276	67	51711	41.485	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 165.920%#		
41) Toluene-d8		10.325	98	85530	22.061	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 88.240%		
43) trans-1,3-Dichloroprop...		10.581	79	13347	25.571	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 102.280%		
47) 2-Hexanone-d5		10.922	63	12572	78.306	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 156.620%#		
56) 1,1,2,2-Tetrachloroeth...		12.690	84	40817	44.588	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 178.360%#		
66) 1,2-Dichlorobenzene-d4		13.848	152	20697	29.213	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 116.840%		
Target Compounds							Qvalue
13) Acetone		4.131	43	3368	7.671	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030485.D
Acq On : 09 Oct 2024 19:59
Operator : SY/MD
Sample : P4346-11
Misc : 2.30g/10mL/MSVOA_W/SOIL/A
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX1

Quant Time: Oct 10 01:31:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

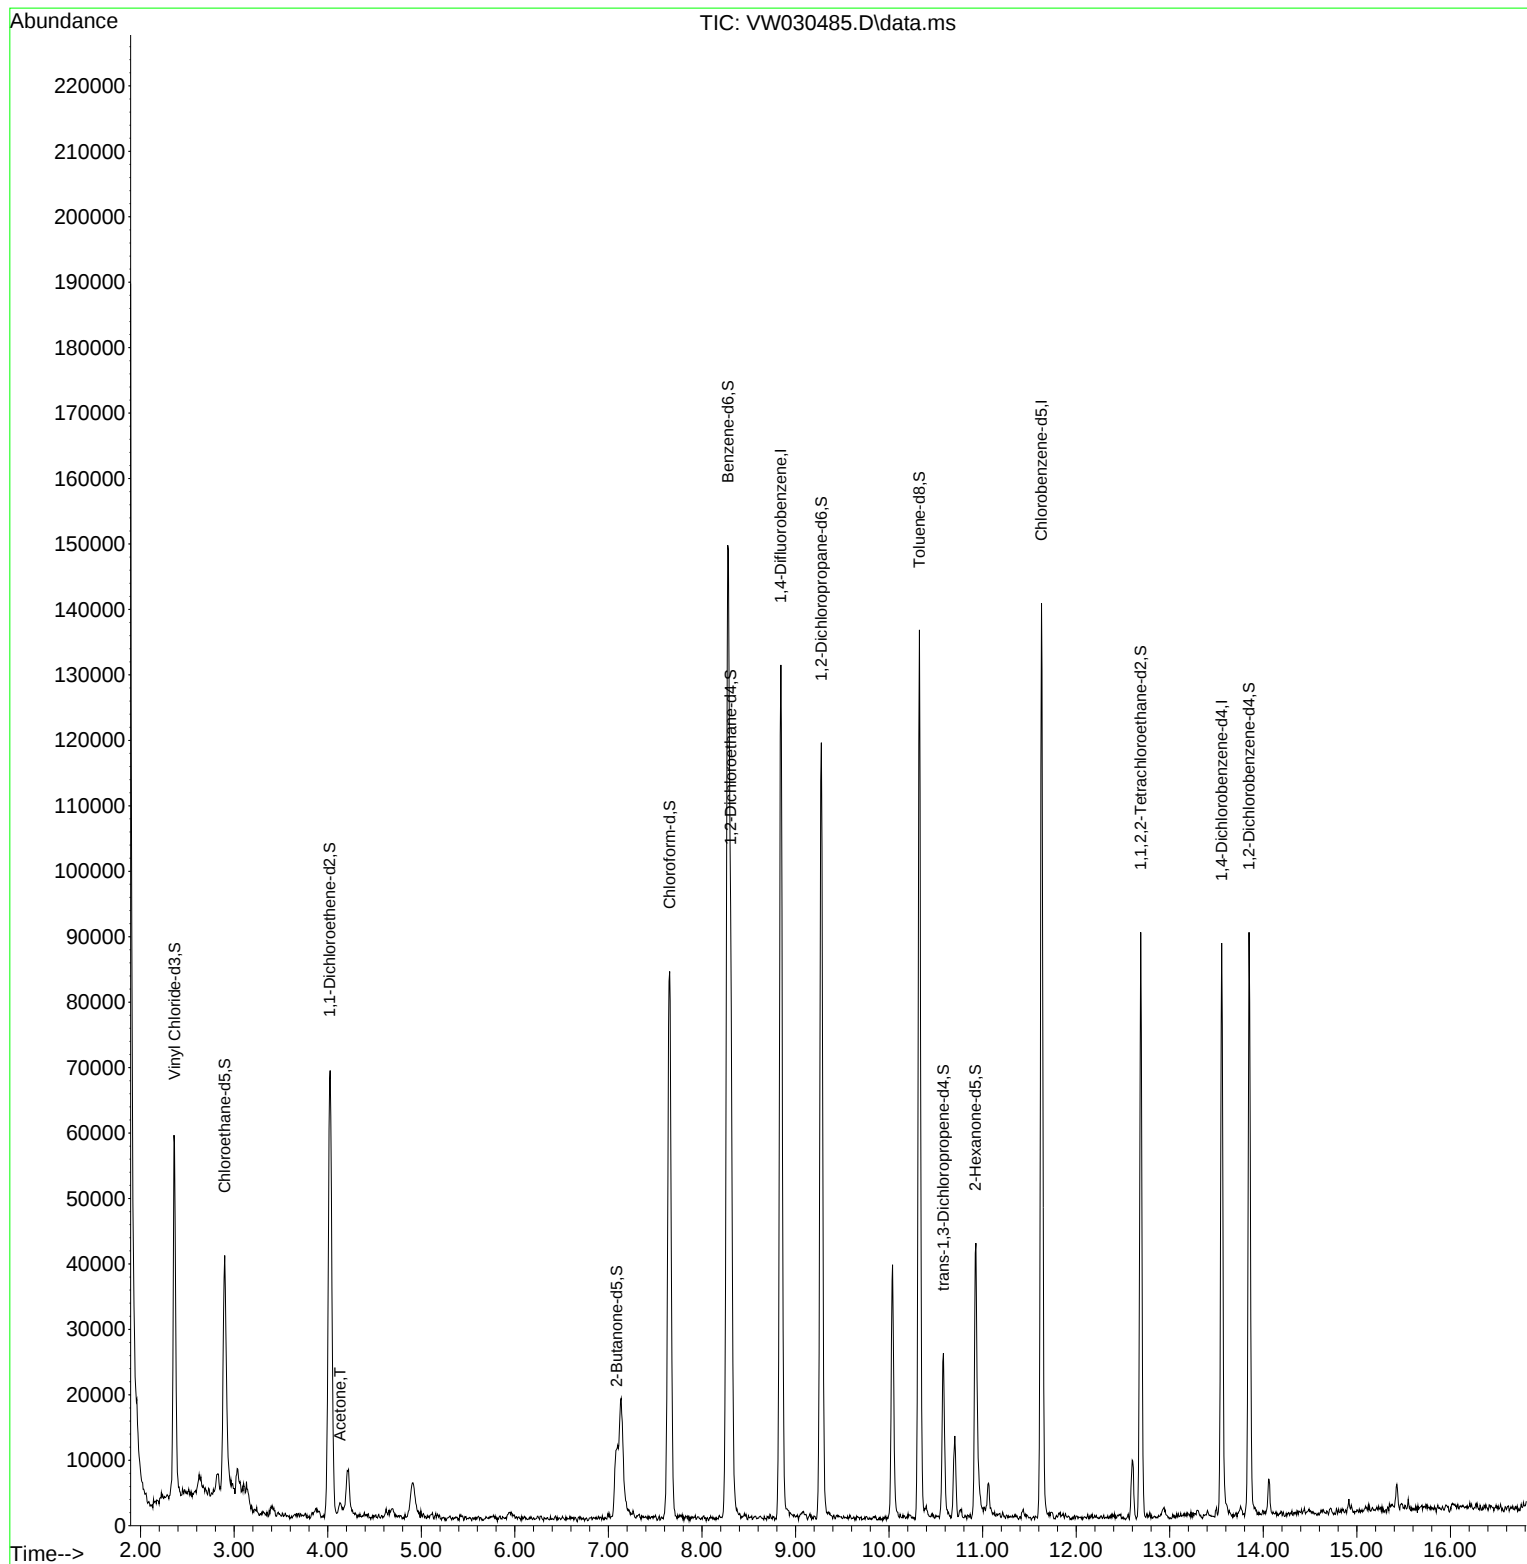

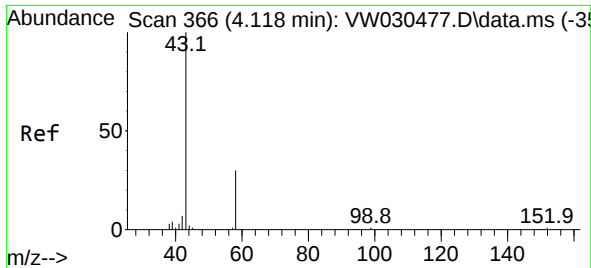

#13
 Acetone
 Concen: 7.671 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW030485.D
 Acq: 09 Oct 2024 19:59

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX1

Tgt Ion: 43 Resp: 3368
 Ion Ratio Lower Upper
 43 100
 58 27.9 0.0 57.6

