

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030491.D
 Acq On : 09 Oct 2024 22:23
 Operator : SY/MD
 Sample : P4346-18
 Misc : 3.21g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX8

Quant Time: Oct 10 01:32:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	251662	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	170137	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	53402	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.363	65	111791	28.260	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	113.040%	
7) Chloroethane-d5		2.899	69	99671	33.287	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	133.160%	
11) 1,1-Dichloroethene-d2		4.021	65	41666	25.324	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	101.280%	
21) 2-Butanone-d5		7.075	46	51473	72.305	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	144.620%#	
24) Chloroform-d		7.648	84	209237	29.073	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	116.280%	
26) 1,2-Dichloroethane-d4		8.307	65	139718	37.333	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	149.320%#	
32) Benzene-d6		8.276	84	339728	34.404	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	137.600%#	
36) 1,2-Dichloropropane-d6		9.276	67	124022	42.791	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	171.160%#	
41) Toluene-d8		10.325	98	218700	24.261	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.040%	
43) trans-1,3-Dichloroprop...		10.581	79	34197	28.177	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	112.720%	
47) 2-Hexanone-d5		10.922	63	41165	110.272	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	220.540%#	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	100719	47.319	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	189.280%#	
66) 1,2-Dichlorobenzene-d4		13.848	152	53006	29.335	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	117.360%	
Target Compounds							
13) Acetone		4.124	43	9955	9.552	ug/L	Qvalue 97
15) Methyl Acetate		4.679	43	4782	3.714	ug/L	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030491.D
Acq On : 09 Oct 2024 22:23
Operator : SY/MD
Sample : P4346-18
Misc : 3.21g/10mL/MSVOA_W/SOIL/A
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX8

Quant Time: Oct 10 01:32:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration




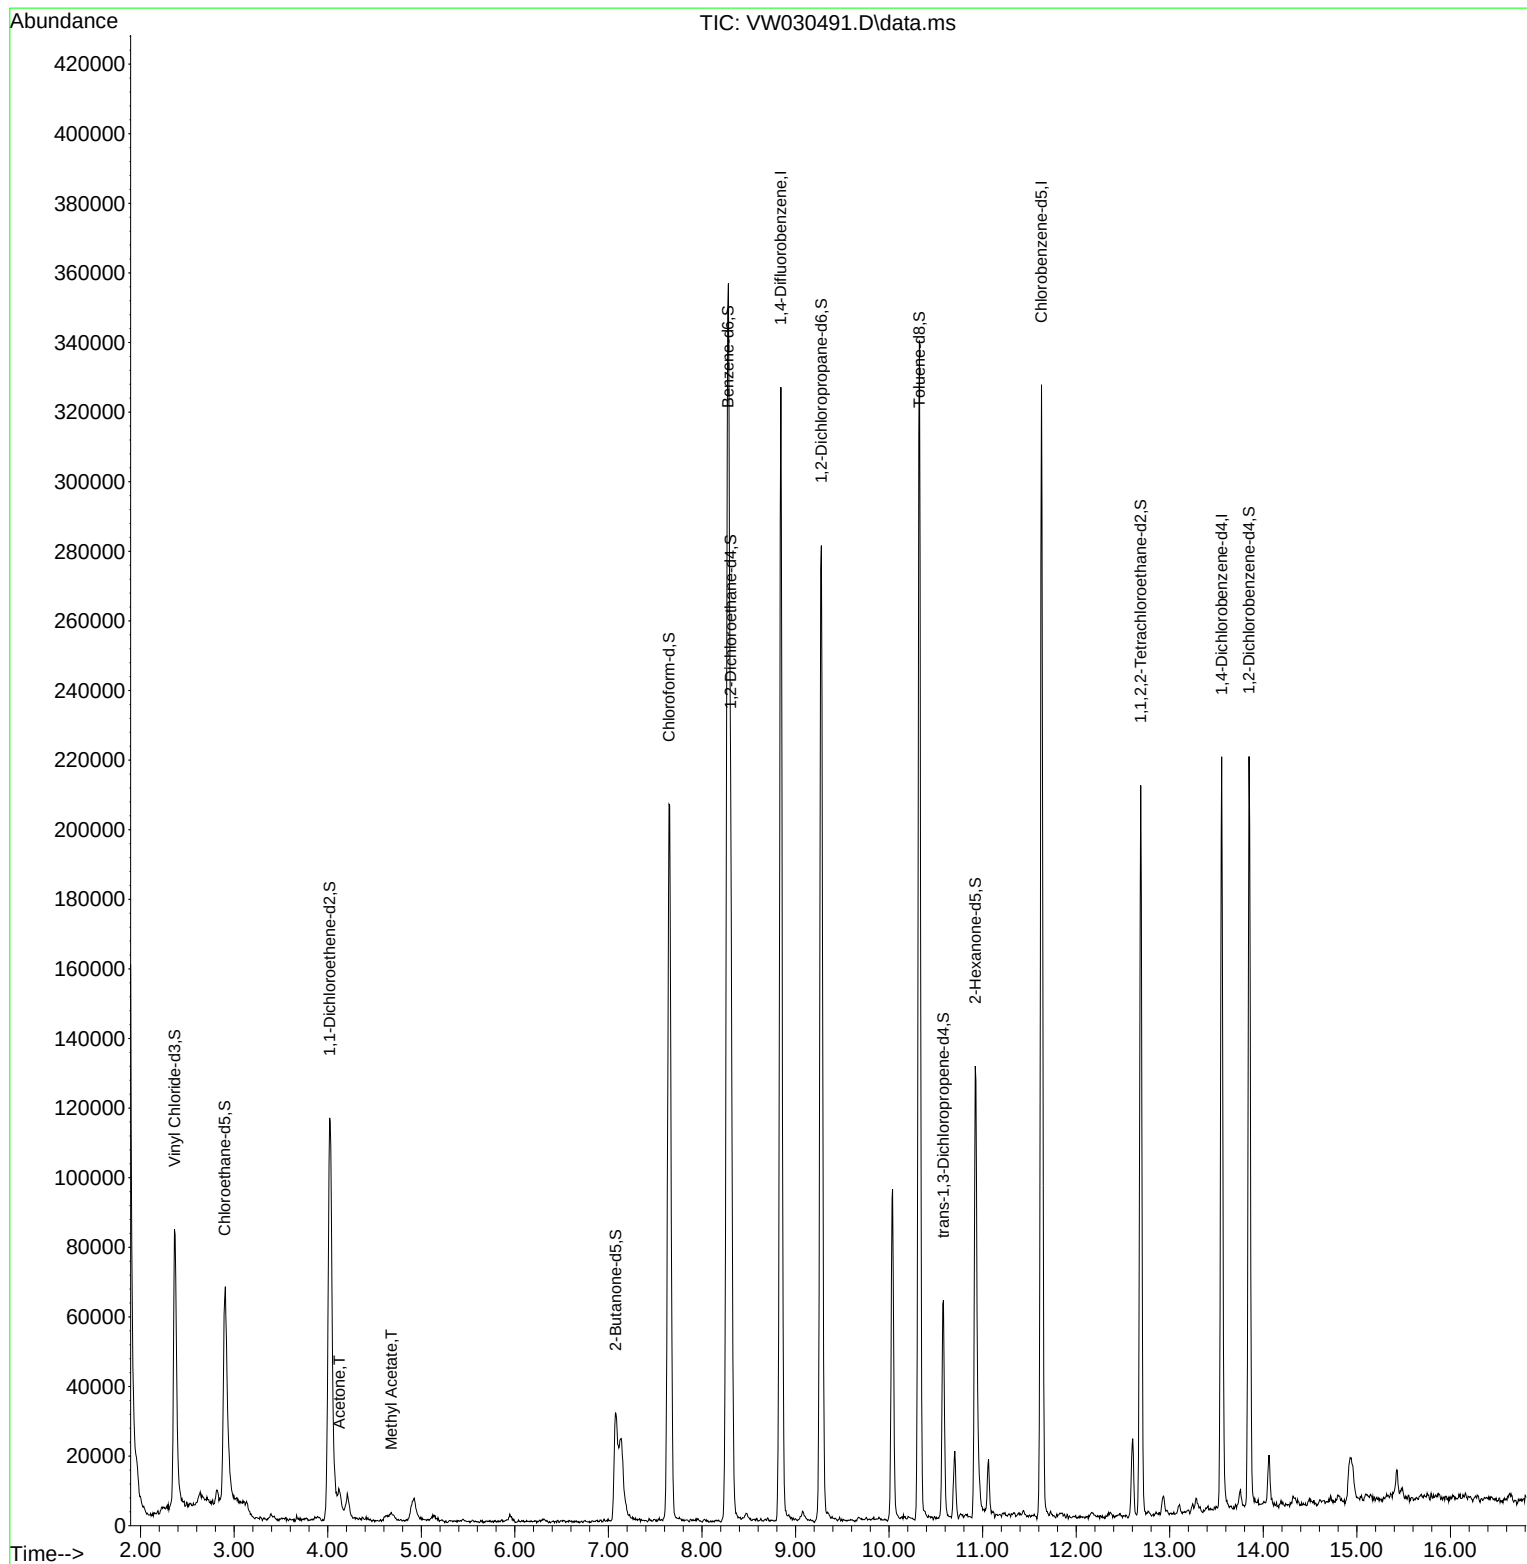


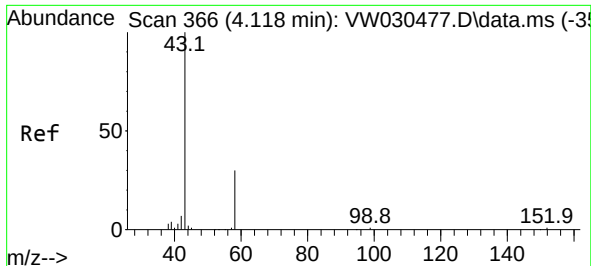

#13
Acetone
Concen: 9.552 ug/L
RT: 4.124 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW030491.D
Acq: 09 Oct 2024 22:23

Instrument :
MSVOA_W
ClientSampleId :
EOAX8

Tgt Ion: 43 Resp: 9955
Ion Ratio Lower Upper
43 100
58 30.5 0.0 57.6

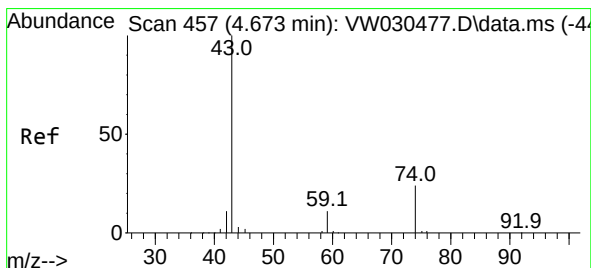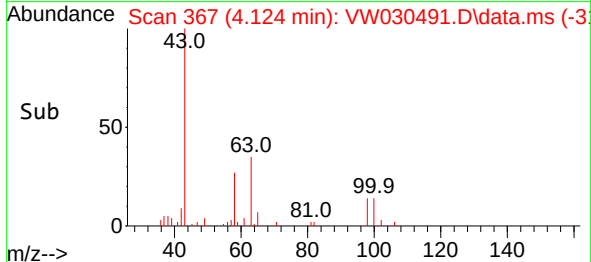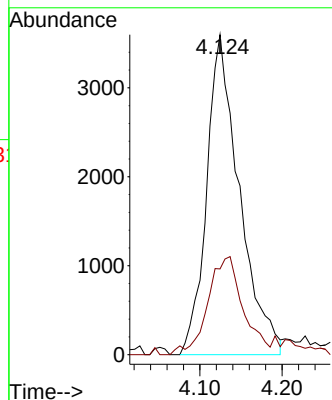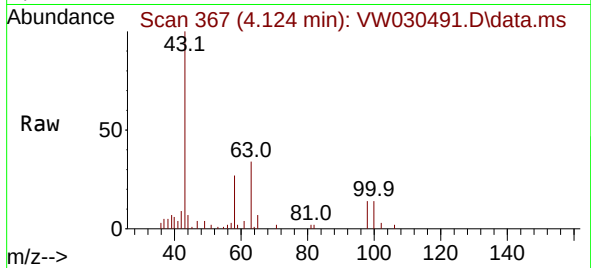

#15
Methyl Acetate
Concen: 3.714 ug/L
RT: 4.679 min Scan# 458
Delta R.T. 0.006 min
Lab File: VW030491.D
Acq: 09 Oct 2024 22:23

Tgt Ion: 43 Resp: 4782
Ion Ratio Lower Upper
43 100
74 17.3 19.3 28.9#

