

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
 Data File : VW030492.D
 Acq On : 09 Oct 2024 22:47
 Operator : SY/MD
 Sample : P4346-19
 Misc : 3.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX9

Quant Time: Oct 10 01:33:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 10 01:29:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	389650	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	302826	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	106384	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	145037	23.681	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.720%
7) Chloroethane-d5	2.899	69	126669	27.322	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	109.280%
11) 1,1-Dichloroethene-d2	4.027	65	58165	22.833	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	91.320%
21) 2-Butanone-d5	7.081	46	65372	59.310	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.620%
24) Chloroform-d	7.648	84	264074	23.698	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	8.307	65	154508	26.665	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.640%
32) Benzene-d6	8.276	84	492421	28.017	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	112.080%
36) 1,2-Dichloropropane-d6	9.276	67	155728	30.187	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	120.760%#
41) Toluene-d8	10.325	98	375448	23.400	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.600%
43) trans-1,3-Dichloroprop...	10.575	79	44615	20.654	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.600%
47) 2-Hexanone-d5	10.922	63	51002	76.759	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	153.520%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	113707	30.013	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	120.040%#
66) 1,2-Dichlorobenzene-d4	13.848	152	98324	27.315	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.280%
Target Compounds					Qvalue	
13) Acetone	4.143	43	16484	10.215	ug/L	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100924\
Data File : VW030492.D
Acq On : 09 Oct 2024 22:47
Operator : SY/MD
Sample : P4346-19
Misc : 3.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EOAX9

Quant Time: Oct 10 01:33:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 10 01:29:22 2024
Response via : Initial Calibration

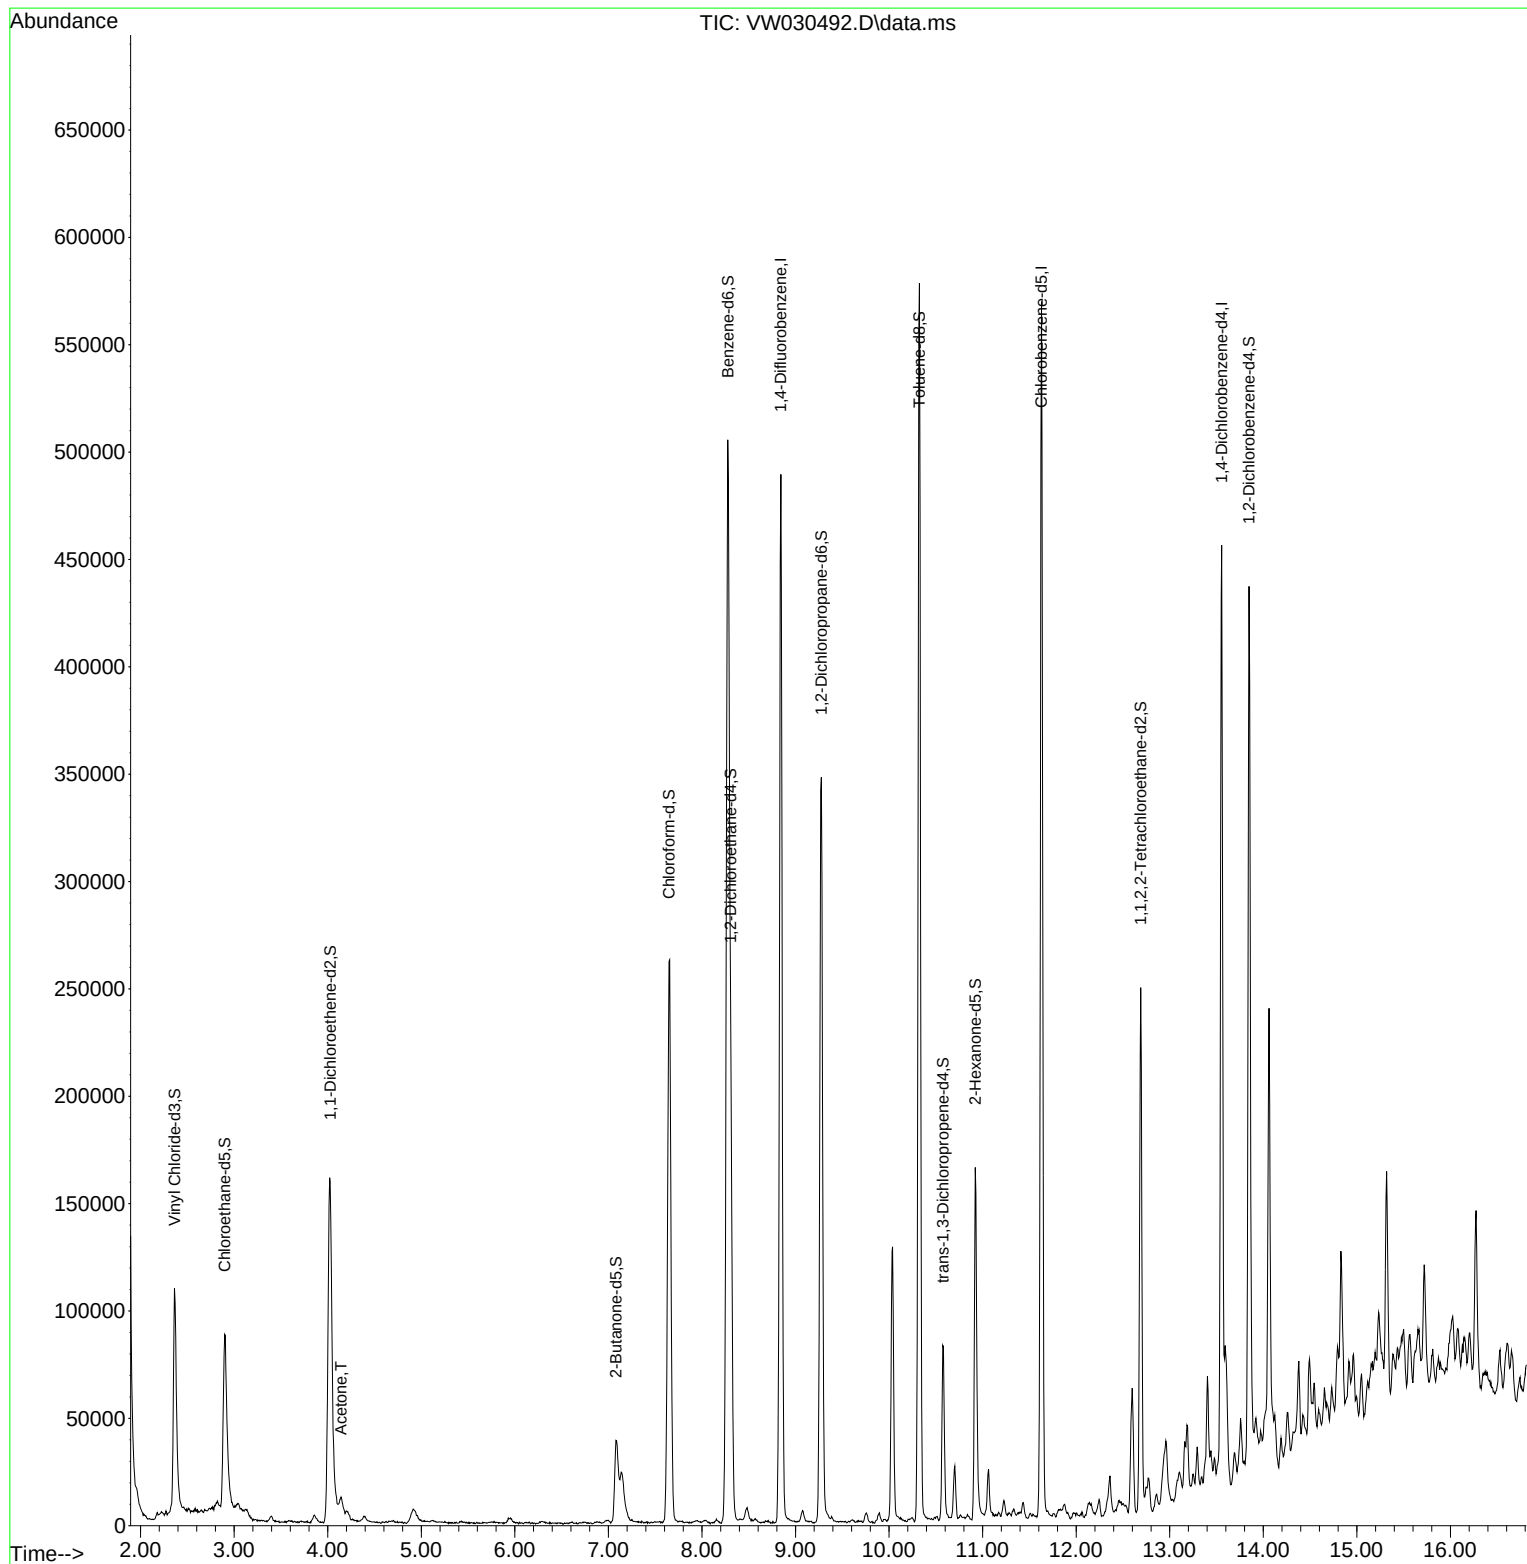

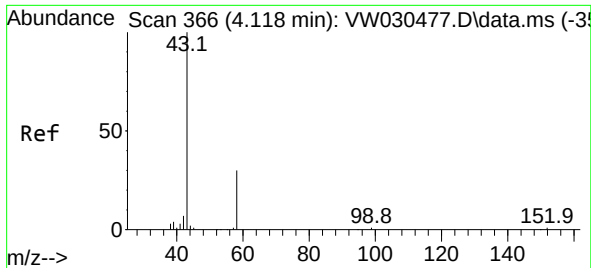

#13
 Acetone
 Concen: 10.215 ug/L
 RT: 4.143 min Scan# 31
 Delta R.T. 0.025 min
 Lab File: VW030492.D
 Acq: 09 Oct 2024 22:47

Instrument :
 MSVOA_W
 ClientSampleId :
 EOAX9

Tgt Ion: 43 Resp: 16484
 Ion Ratio Lower Upper
 43 100
 58 14.1 0.0 57.6

