

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024817.D
 Acq On : 10 Oct 2022 20:32
 Operator : SY/VA
 Sample : VW1010SBL02
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK421

Quant Time: Oct 11 02:00:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	528796	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	480715	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	229860	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	144490	26.116	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.480%
7) Chloroethane-d5	2.891	69	79712	24.793	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.160%
11) 1,1-Dichloroethene-d2	4.019	63	235820	18.416	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.680%
21) 2-Butanone-d5	7.080	46	88291	44.387	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.780%
24) Chloroform-d	7.647	84	329248	23.290	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.160%
26) 1,2-Dichloroethane-d4	8.305	65	178399	24.327	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.320%
32) Benzene-d6	8.275	84	722048	23.500	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	9.274	67	217690	23.189	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.760%
41) Toluene-d8	10.323	98	649241	23.642	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.560%
43) trans-1,3-Dichloroprop...	10.579	79	79893	19.110	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.440%
47) 2-Hexanone-d5	10.927	63	69311	43.152	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.300%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	155378	23.229	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.920%
66) 1,2-Dichlorobenzene-d4	13.847	152	189859	23.473	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.880%
Target Compounds						Qvalue
16) Methylene chloride	4.922	84	42786	4.120	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024817.D
Acq On : 10 Oct 2022 20:32
Operator : SY/VA
Sample : VW1010SBL02
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK421


Quant Time: Oct 11 02:00:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

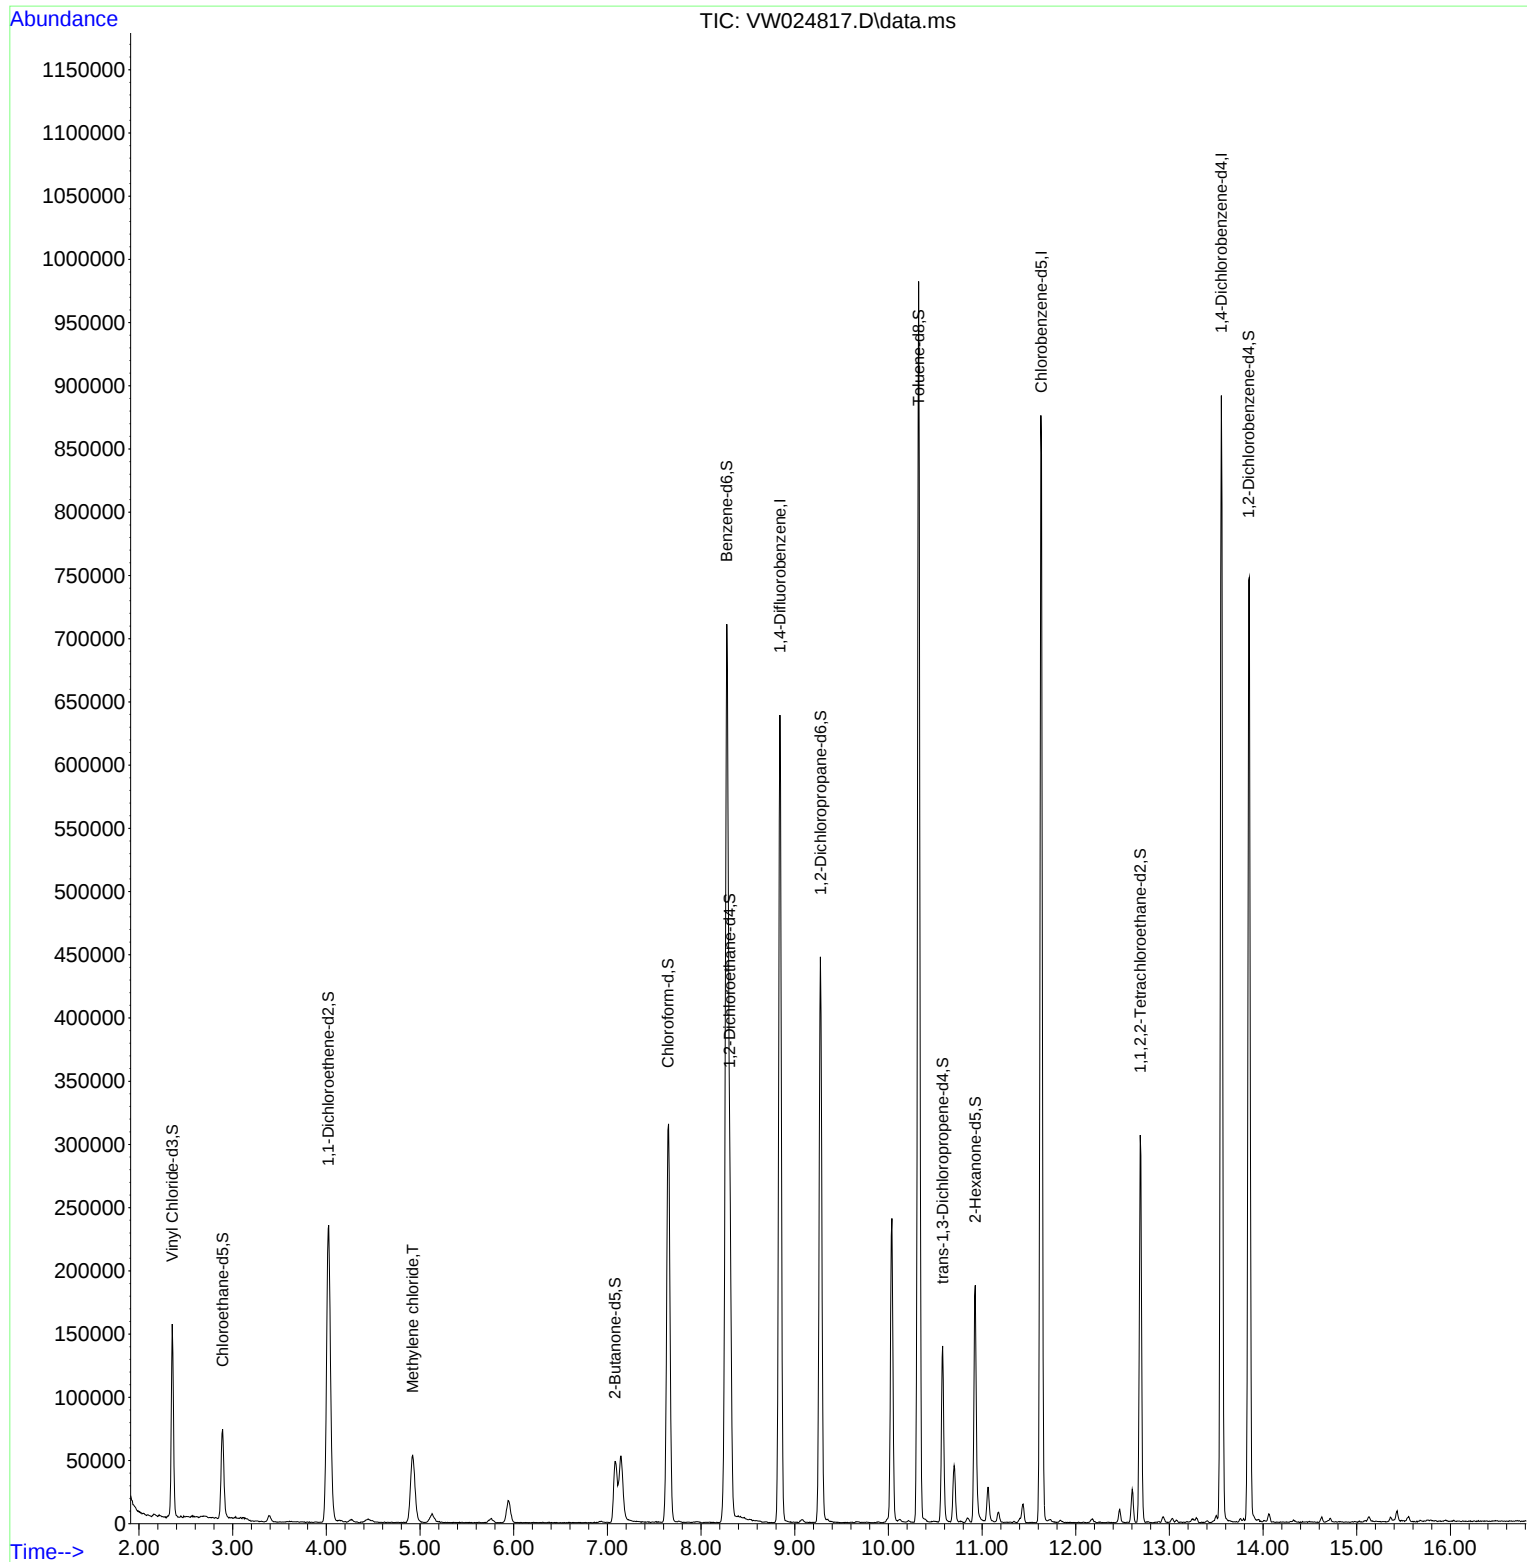

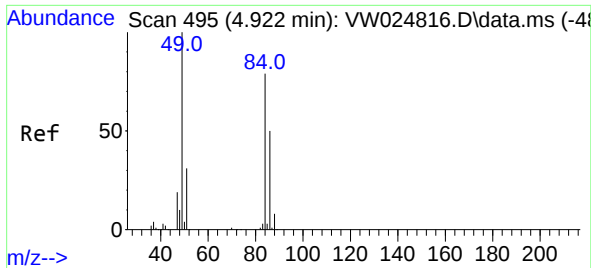

#16
Methylene chloride
Concen: 4.120 ug/L
RT: 4.922 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW024817.D
Acq: 10 Oct 2022 20:32

Instrument :
MSVOA_W
ClientSampleId :
VBLK421

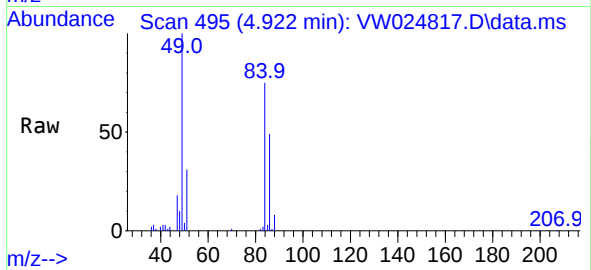

Tgt Ion: 84 Resp: 42786

Ion	Ratio	Lower	Upper
84	100		
86	64.3	44.0	81.8
49	132.6	87.4	162.2

