

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024823.D
 Acq On : 10 Oct 2022 22:57
 Operator : SY/VA
 Sample : N5024-06RE
 Misc : 4.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BF6RE

Quant Time: Oct 11 02:01:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	451203	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	303534	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	69181	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	117760	24.945	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.800%
7) Chloroethane-d5	2.885	69	73930	26.950	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.800%
11) 1,1-Dichloroethene-d2	4.019	63	180895	16.556	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.240%
21) 2-Butanone-d5	7.080	46	104453	61.543	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.080%
24) Chloroform-d	7.647	84	349762	28.996	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	116.000%
26) 1,2-Dichloroethane-d4	8.305	65	181463	29.000	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	116.000%
32) Benzene-d6	8.275	84	573658	29.569	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	118.280%
36) 1,2-Dichloropropane-d6	9.274	67	222186	37.483	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	149.920%#
41) Toluene-d8	10.323	98	427169	24.635	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.560%
43) trans-1,3-Dichloroprop...	10.579	79	62032	23.499	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.000%
47) 2-Hexanone-d5	10.926	63	67631	66.684	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	133.360%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	152567	36.122	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	144.480%#
66) 1,2-Dichlorobenzene-d4	13.853	152	56243	23.103	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.400%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4871	0.587	ug/L #	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024823.D
Acq On : 10 Oct 2022 22:57
Operator : SY/VA
Sample : N5024-06RE
Misc : 4.60g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BF6RE

Quant Time: Oct 11 02:01:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

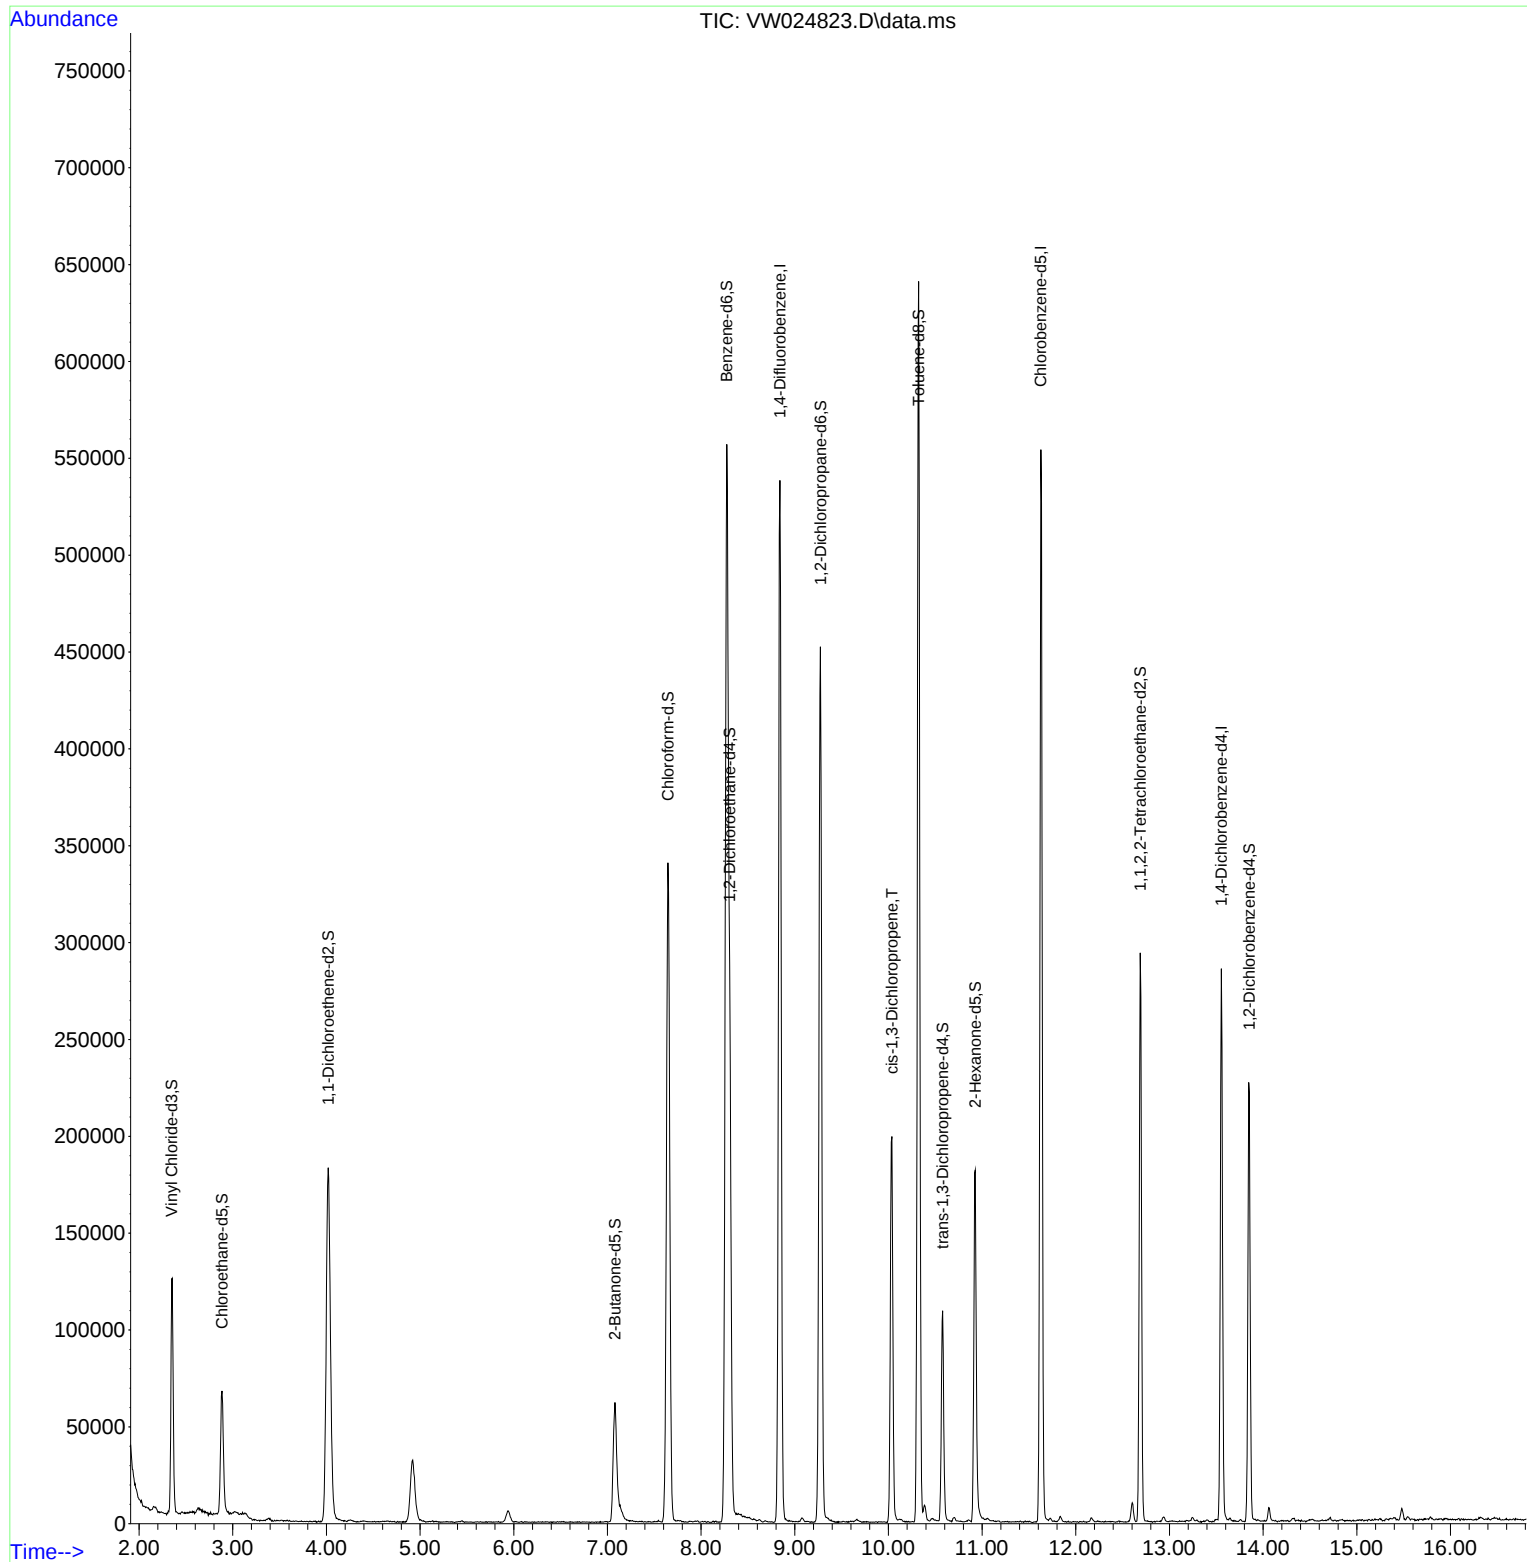

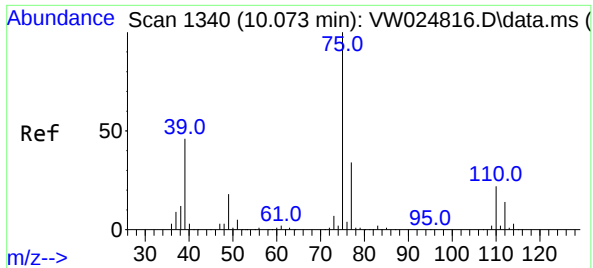

#39
 cis-1,3-Dichloropropene
 Concen: 0.587 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW024823.D
 Acq: 10 Oct 2022 22:57

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BF6RE

Tgt Ion: 75 Resp: 4871

Ion	Ratio	Lower	Upper
75	100		
77	46.6	22.4	41.6#

