

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024831.D
 Acq On : 11 Oct 2022 02:11
 Operator : SY/VA
 Sample : N5064-07
 Misc : 6.47g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COBN4

Quant Time: Oct 11 06:37:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	418434	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	357608	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	147593	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	87575	20.004	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.000%
7) Chloroethane-d5	2.885	69	49810	19.579	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.320%
11) 1,1-Dichloroethene-d2	4.019	63	141612	13.976	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.920%
21) 2-Butanone-d5	7.080	46	90688	57.617	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.240%
24) Chloroform-d	7.653	84	268444	23.998	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.000%
26) 1,2-Dichloroethane-d4	8.305	65	157548	27.150	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	108.600%
32) Benzene-d6	8.275	84	513505	22.466	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.880%
36) 1,2-Dichloropropane-d6	9.274	67	177724	25.449	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.800%
41) Toluene-d8	10.323	98	420105	20.564	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.240%
43) trans-1,3-Dichloroprop...	10.573	79	56401	18.135	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.560%
47) 2-Hexanone-d5	10.927	63	68452	57.288	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.580%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	160034	32.161	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	128.640%#
66) 1,2-Dichlorobenzene-d4	13.847	152	117229	22.572	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.280%
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	12528	1.975	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024831.D
Acq On : 11 Oct 2022 02:11
Operator : SY/VA
Sample : N5064-07
Misc : 6.47g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BN4


Quant Time: Oct 11 06:37:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

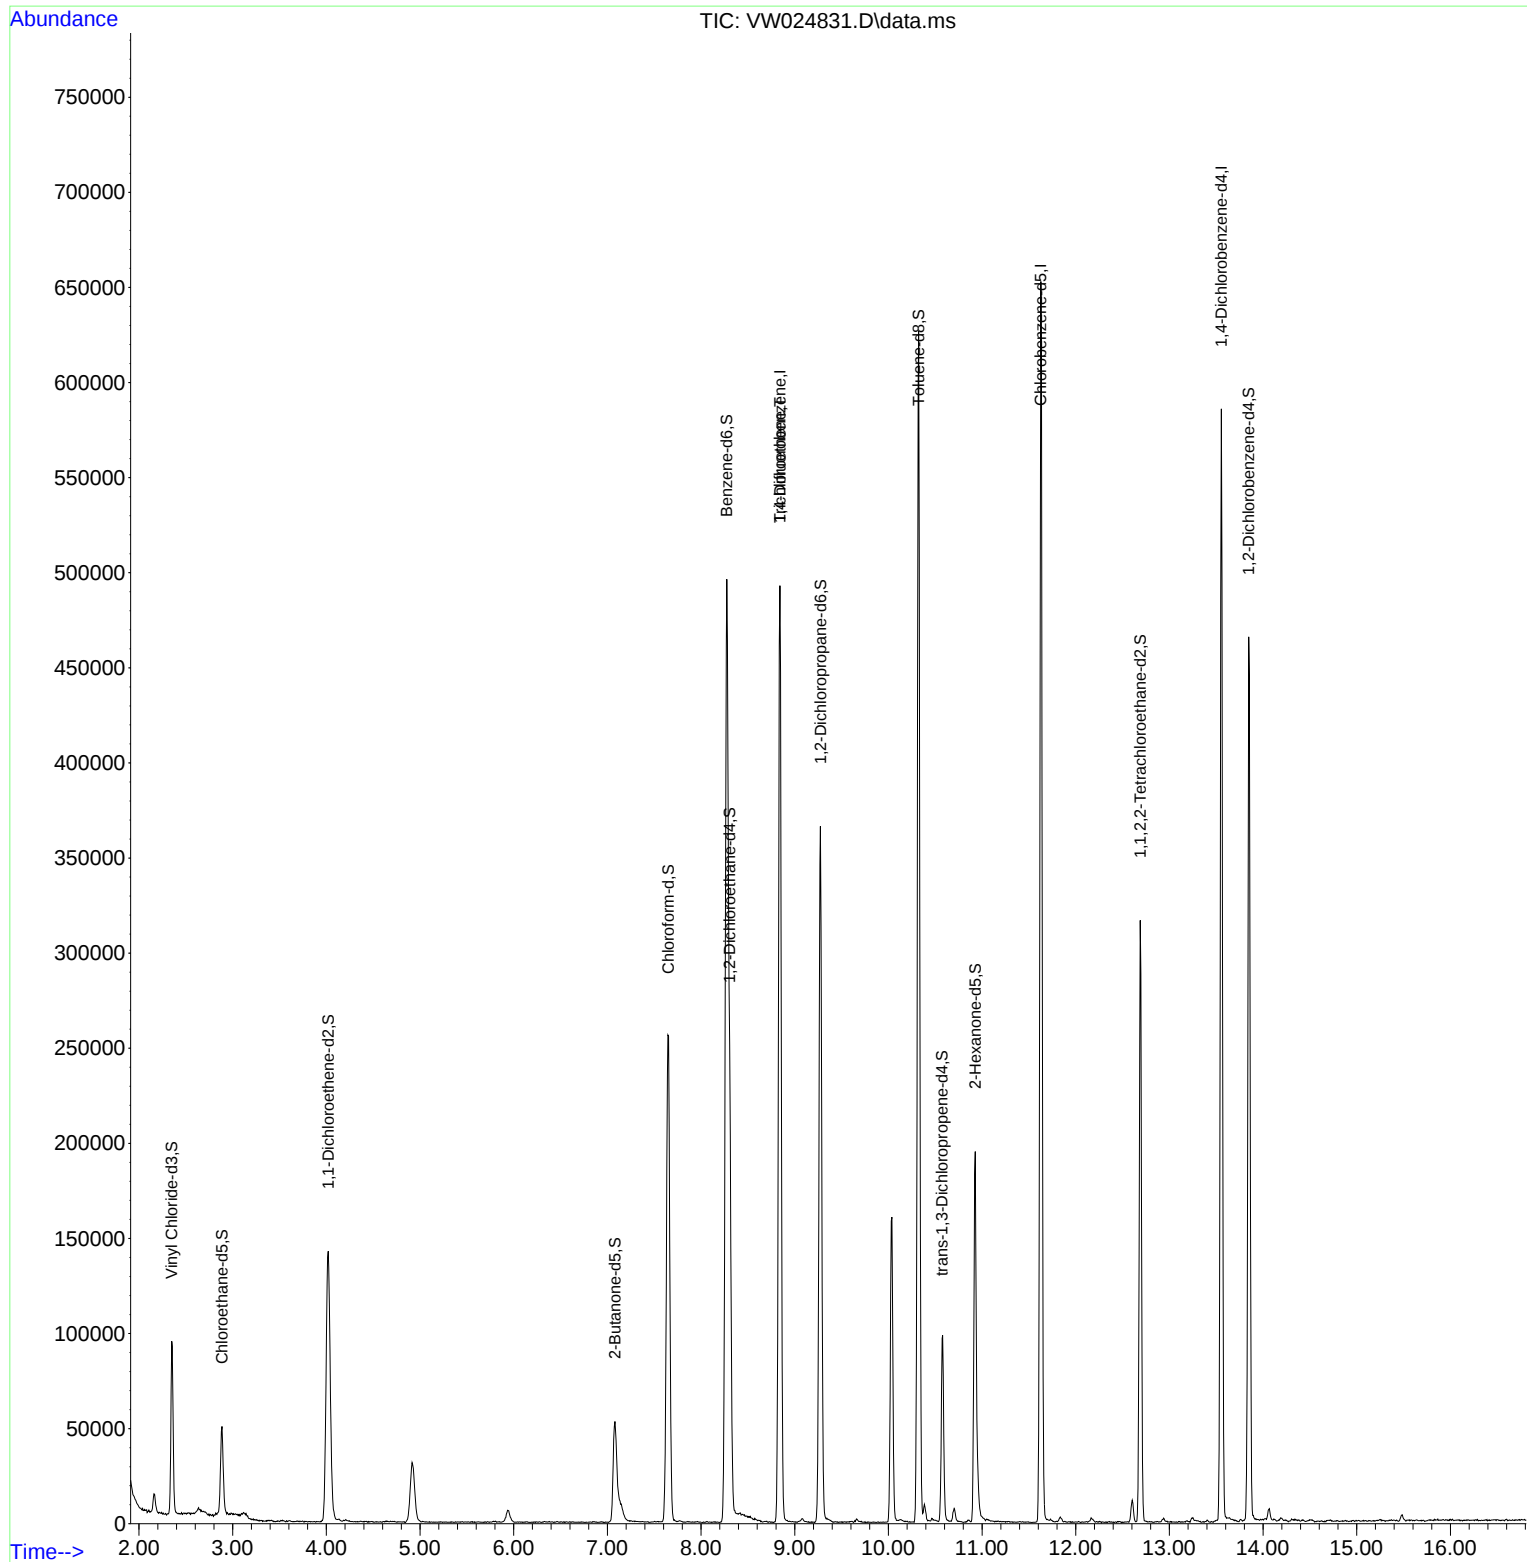

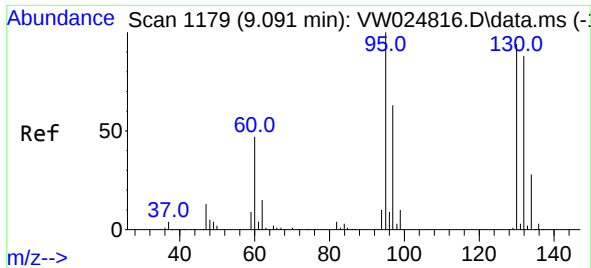

#34
Trichloroethene
Concen: 1.975 ug/L
RT: 8.842 min Scan# 11
Delta R.T. -0.250 min
Lab File: VW024831.D
Acq: 11 Oct 2022 02:11

Instrument :
MSVOA_W
ClientSampleId :
C0BN4

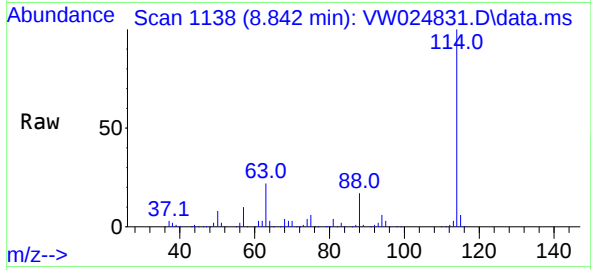

Tgt Ion: 95 Resp: 12528

Ion	Ratio	Lower	Upper
95	100		
97	0.0	43.5	80.9#
132	0.0	61.2	113.8#
130	0.0	68.5	127.1#

