




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010222\
Data File : VW024819.D
Acq On : 10 Oct 2022 21:21
Operator : SY/VA
Sample : N5023-13
Misc : 6.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BD2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/11/2022
Supervised By :Mahesh Dadoda 10/11/2022

Quant Time: Oct 11 02:00:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

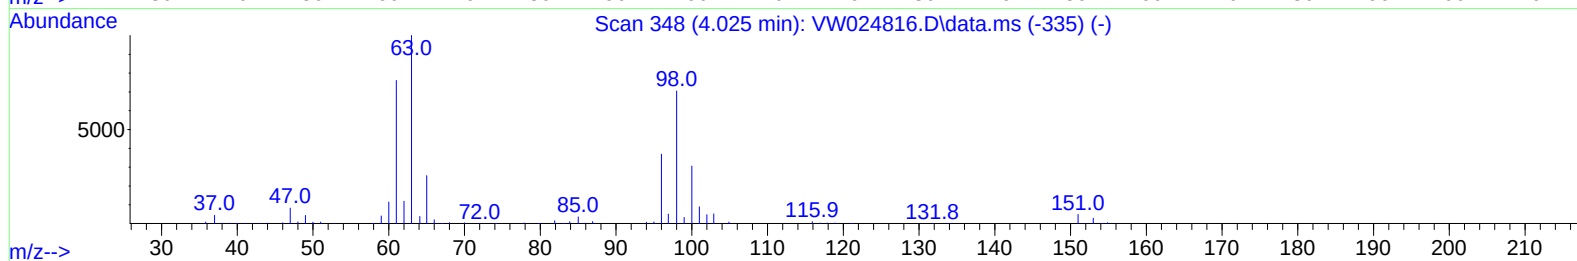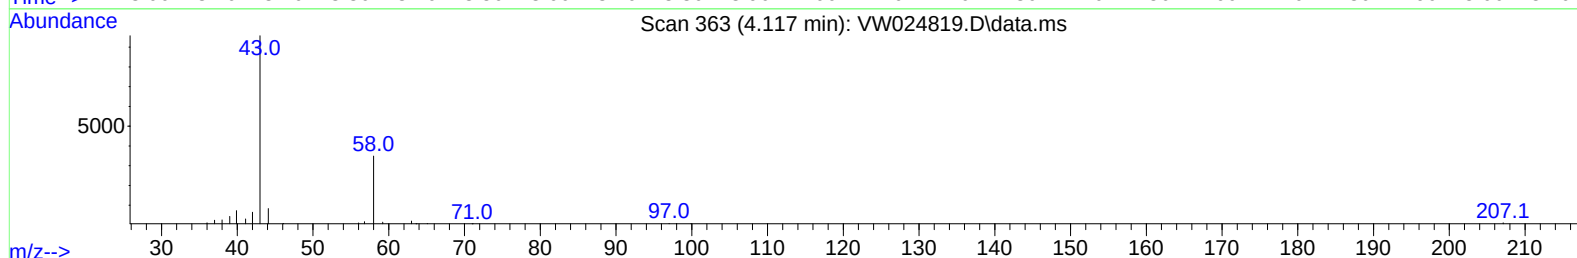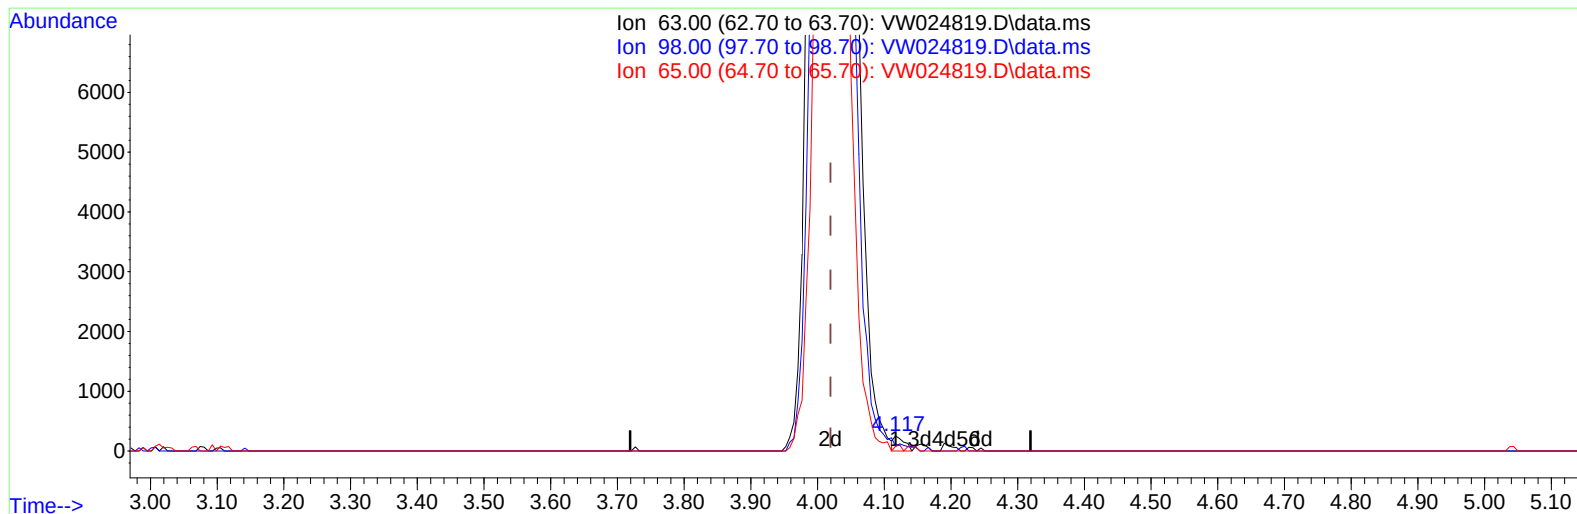

TIC: VW024819.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.117min (+ 0.097) 0.02 ug/L

response	270	
Ion	Exp%	Act%
63.00	100.00	100.00
98.00	74.00	58.52
65.00	22.40	24.81
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024819.D
Acq On : 10 Oct 2022 21:21
Operator : SY/VA
Sample : N5023-13
Misc : 6.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BD2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/11/2022
Supervised By :Mahesh Dadoda 10/11/2022

Quant Time: Oct 11 02:00:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

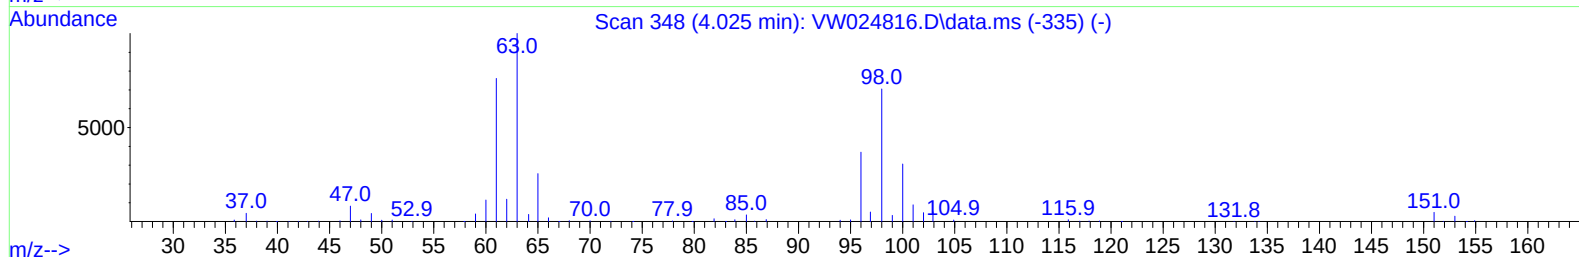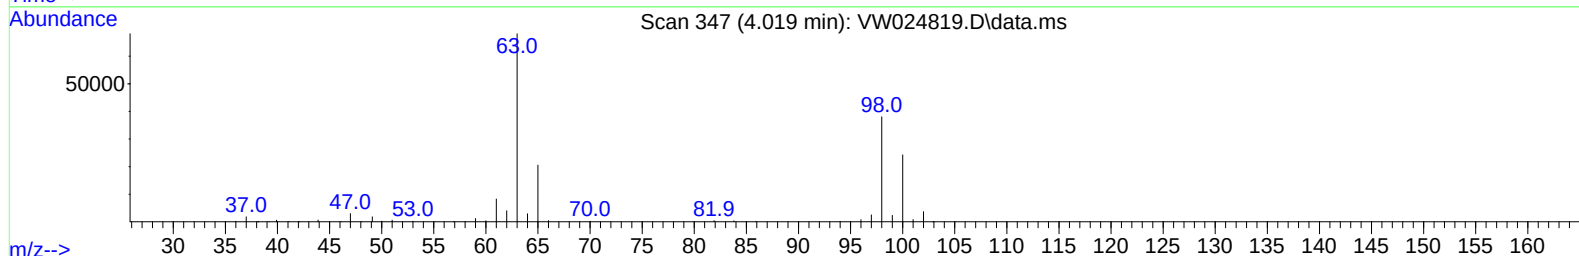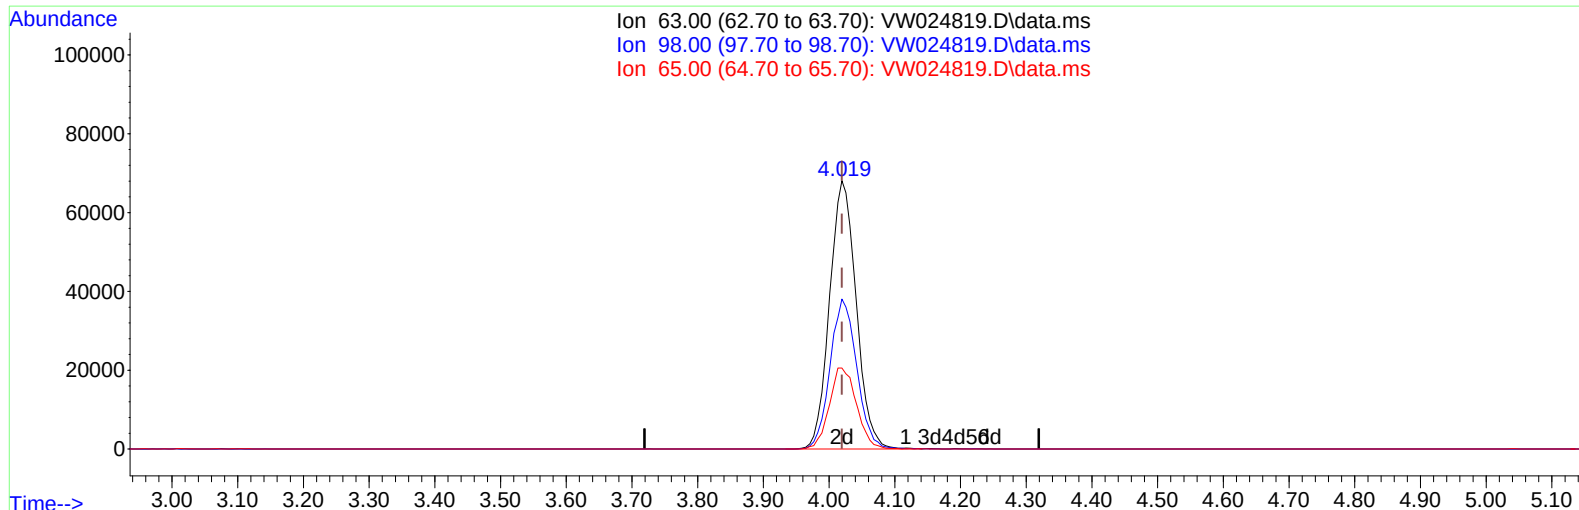

TIC: VW024819.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 13.65 ug/L m

response 191850

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	74.00	0.08#
65.00	22.40	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024819.D
 Acq On : 10 Oct 2022 21:21
 Operator : SY/VA
 Sample : N5023-13
 Misc : 6.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BD2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/11/2022
 Supervised By :Mahesh Dadoda 10/11/2022

Quant Time: Oct 11 02:00:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	580577	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	479870	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	181751	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	115216	18.968	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.880%		
7) Chloroethane-d5	2.892	69	69437	19.671	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	78.680%		
11) 1,1-Dichloroethene-d2	4.019	63	191850m	13.646	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	54.600%		
21) 2-Butanone-d5	7.086	46	94616	43.325	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.640%		
24) Chloroform-d	7.653	84	347731	22.404	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.600%		
26) 1,2-Dichloroethane-d4	8.305	65	177375	22.030	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.120%		
32) Benzene-d6	8.275	84	680829	22.197	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.800%		
36) 1,2-Dichloropropane-d6	9.274	67	225903	24.106	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	96.440%		
41) Toluene-d8	10.323	98	559239	20.400	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.600%		
43) trans-1,3-Dichloroprop...	10.579	79	69177	16.576	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	66.320%		
47) 2-Hexanone-d5	10.927	63	71520	44.605	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	89.220%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	160726	24.071	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	96.280%		
66) 1,2-Dichlorobenzene-d4	13.853	152	144597	22.609	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.440%		
Target Compounds					Qvalue	
13) Acetone	4.141	43	77340	48.539	ug/L	98
22) 2-Butanone	7.183	43	25463	9.991	ug/L #	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024819.D
Acq On : 10 Oct 2022 21:21
Operator : SY/VA
Sample : N5023-13
Misc : 6.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BD2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/11/2022
Supervised By :Mahesh Dadoda 10/11/2022

Quant Time: Oct 11 02:00:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

