

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024832.D
 Acq On : 11 Oct 2022 02:35
 Operator : SY/VA
 Sample : N5064-08
 Misc : 7.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP4

Manual IntegrationsAPPROVED

Quant Time: Oct 11 06:37:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

10/11/2022
 Supervised By :Mahesh
 Dadoda

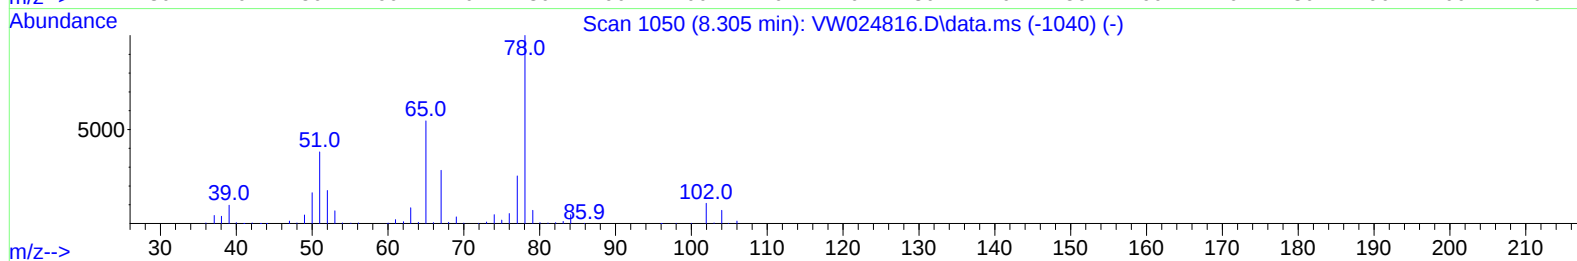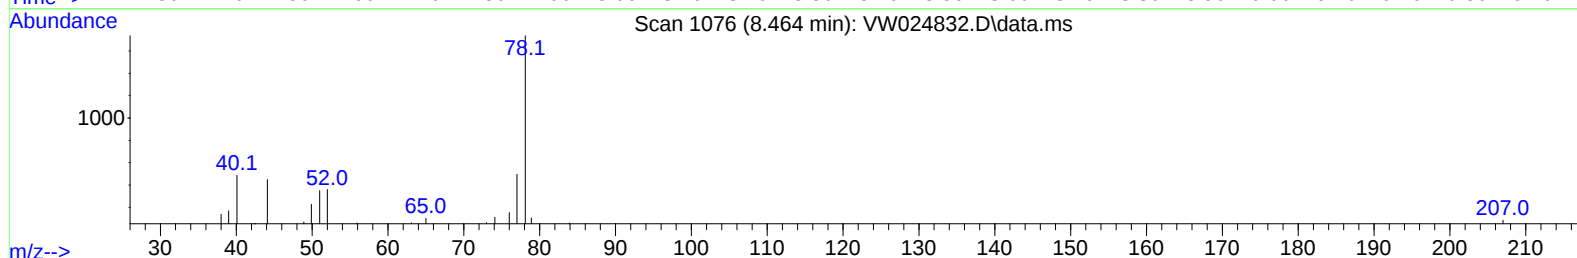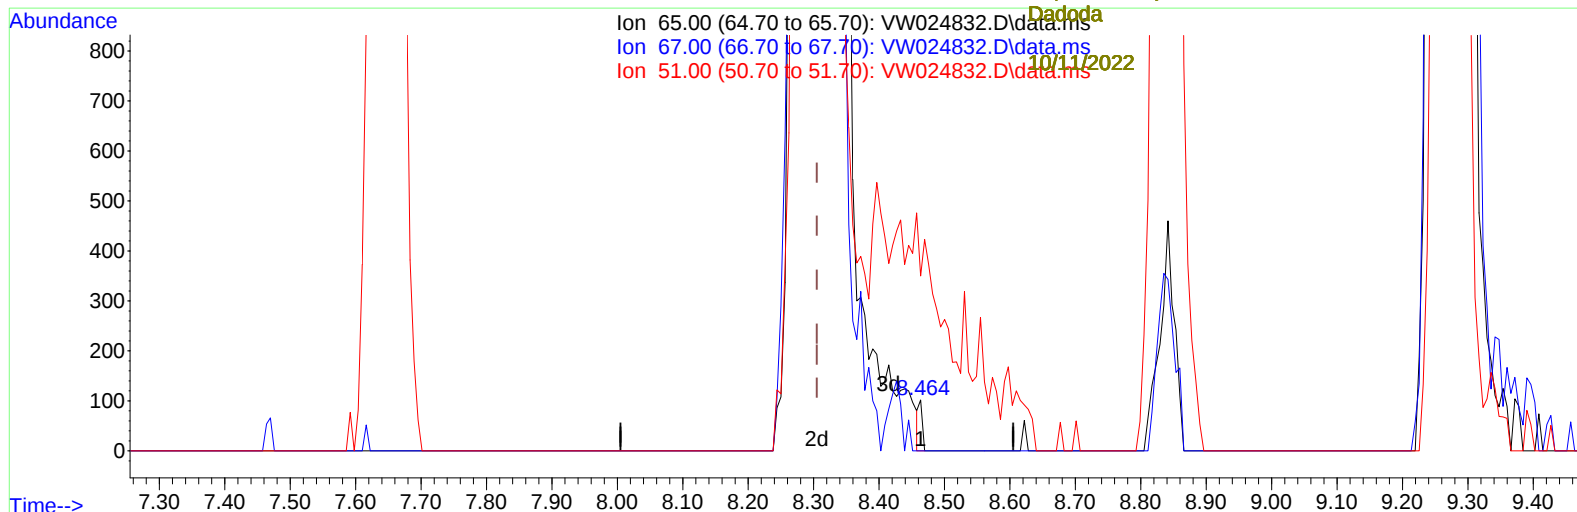

TIC: VW024832.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.464min (+ 0.158) 0.01 ug/L

response 37

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.90	62.16
51.00	118.70	124.32
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024832.D
 Acq On : 11 Oct 2022 02:35
 Operator : SY/VA
 Sample : N5064-08
 Misc : 7.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP4

Manual IntegrationsAPPROVED

Quant Time: Oct 11 06:37:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

10/11/2022
 Supervised By :Mahesh
 Dadoda

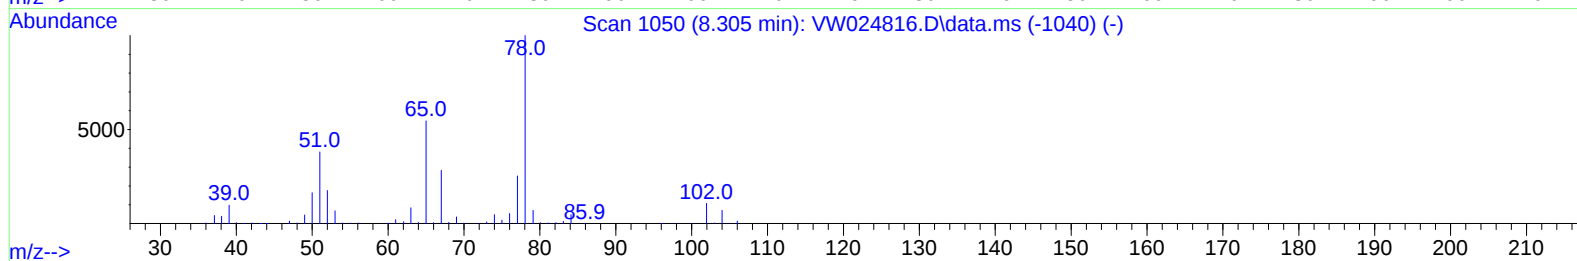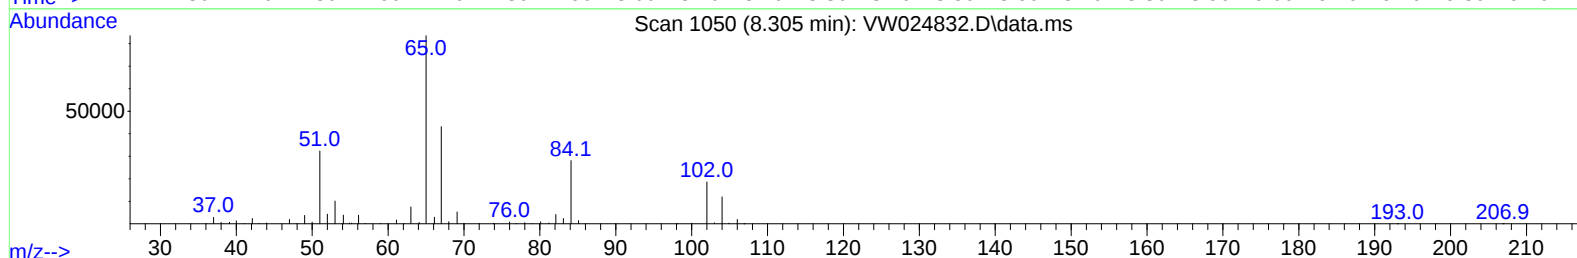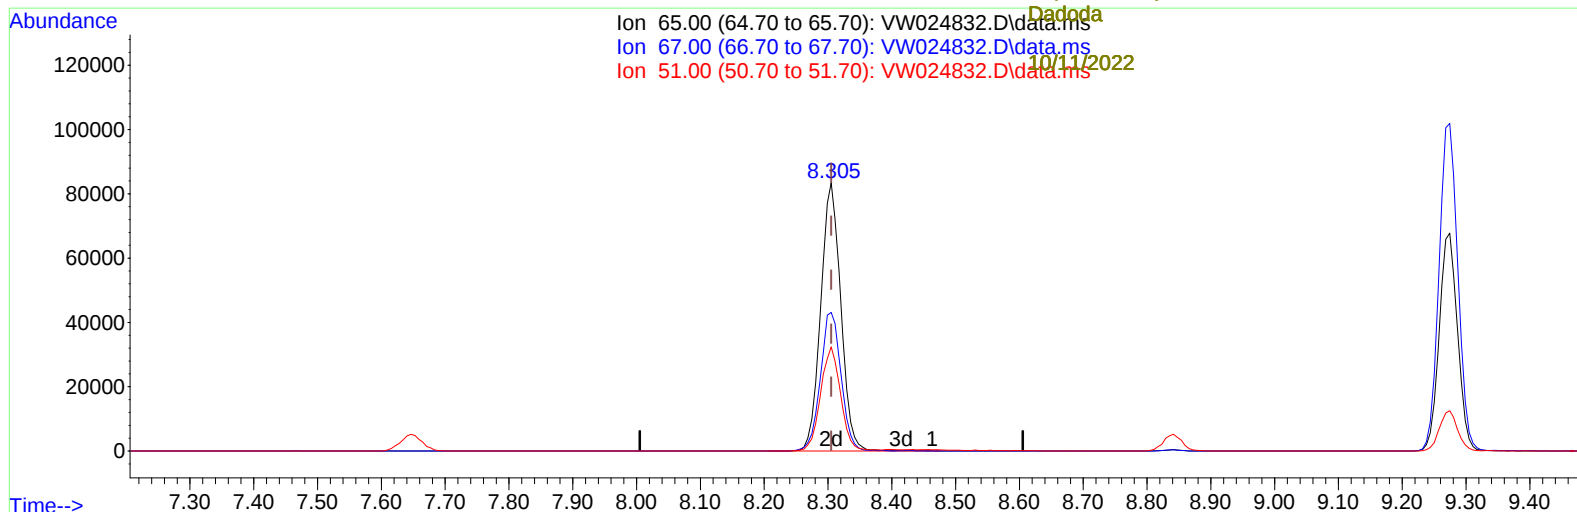

TIC: VW024832.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 24.66 ug/L m

response 182271

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.90	0.01#
51.00	118.70	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024832.D
 Acq On : 11 Oct 2022 02:35
 Operator : SY/VA
 Sample : N5064-08
 Misc : 7.09g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP4

Manual IntegrationsAPPROVED

Quant Time: Oct 11 06:37:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

10/11/2022
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		533034	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		485248	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		214206	25.000	ug/L	0.00

10/11/2022

System Monitoring Compounds

4) Vinyl Chloride-d3	2.349	65		105109	18.847	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.400%	
7) Chloroethane-d5	2.885	69		63381	19.557	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.240%	
11) 1,1-Dichloroethene-d2	4.019	63		166218	12.877	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.520%	
21) 2-Butanone-d5	7.080	46		124541	62.114	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.220%	
24) Chloroform-d	7.647	84		321474	22.560	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.240%	
26) 1,2-Dichloroethane-d4	8.305	65		182271m	24.657	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.640%	
32) Benzene-d6	8.268	84		625930	20.181	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.720%	
36) 1,2-Dichloropropane-d6	9.274	67		208856	22.040	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.160%	
41) Toluene-d8	10.323	98		533603	19.249	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.000%	
43) trans-1,3-Dichloroprop...	10.579	79		74343	17.616	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.480%	
47) 2-Hexanone-d5	10.920	63		96200	59.333	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.660%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		193453	28.651	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.600%	
66) 1,2-Dichlorobenzene-d4	13.847	152		164564	21.832	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.320%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024832.D
Acq On : 11 Oct 2022 02:35
Operator : SY/VA
Sample : N5064-08
Misc : 7.09g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BP4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

10/11/2022
Supervised By :Mahesh
Dadoda

10/11/2022

