

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024835.D
Acq On : 11 Oct 2022 03:48
Operator : SY/VA
Sample : N5064-11
Misc : 7.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
C0BR6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

10/11/2022
Supervised By :Mahesh
Dadoda
10/11/2022
Supervised By :Mahesh
Dadoda

Quant Time: Oct 11 06:38:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

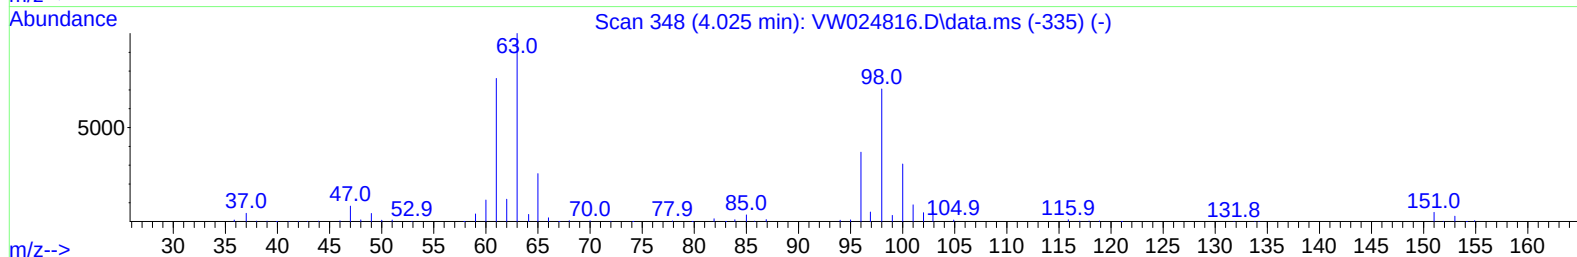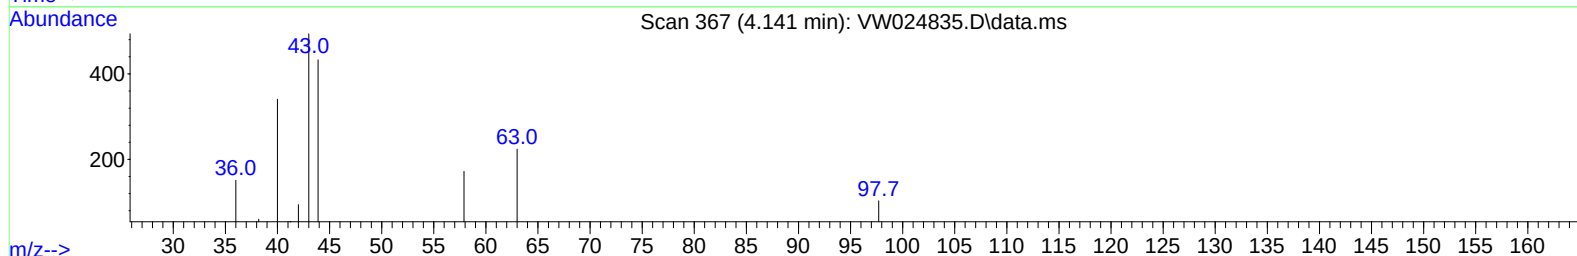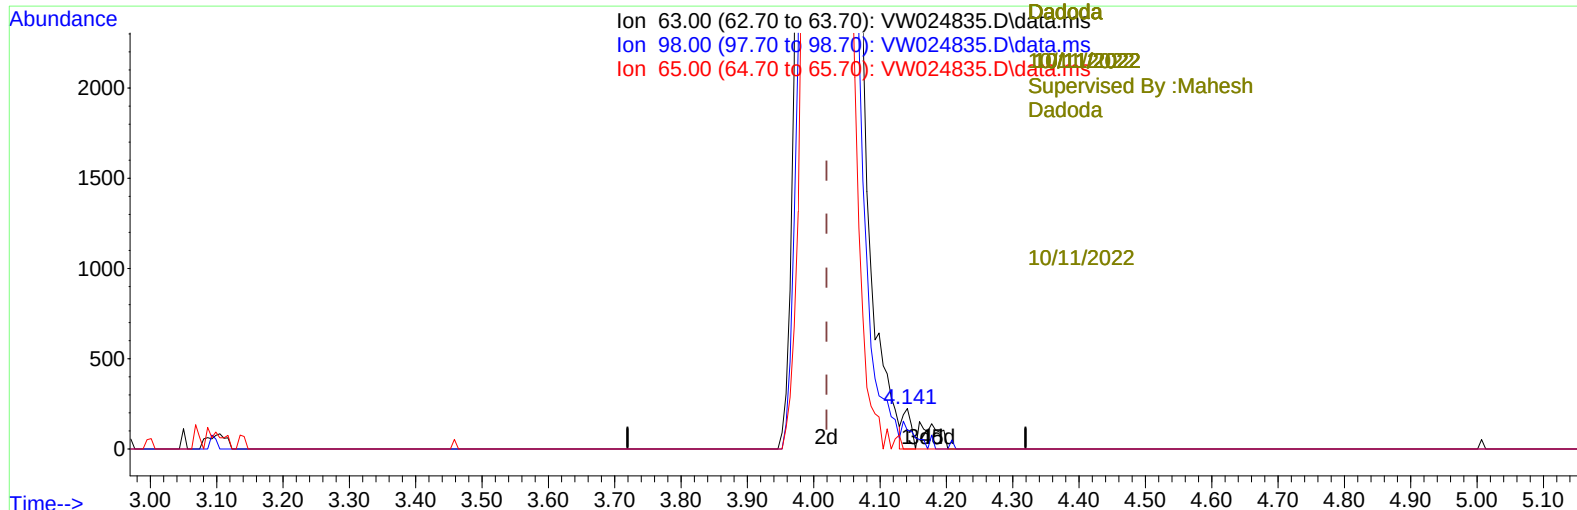

TIC: VW024835.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.141min (+ 0.122) 0.02 ug/L

response 199

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	74.00	85.93
65.00	22.40	24.62
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024835.D
Acq On : 11 Oct 2022 03:48
Operator : SY/VA
Sample : N5064-11
Misc : 7.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BR6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

10/11/2022

Supervised By :Mahesh




Dadoda

10/11/2022

Supervised By :Mahesh

Dadoda

Quant Time: Oct 11 06:38:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 07 03:04:02 2022
Response via : Initial Calibration

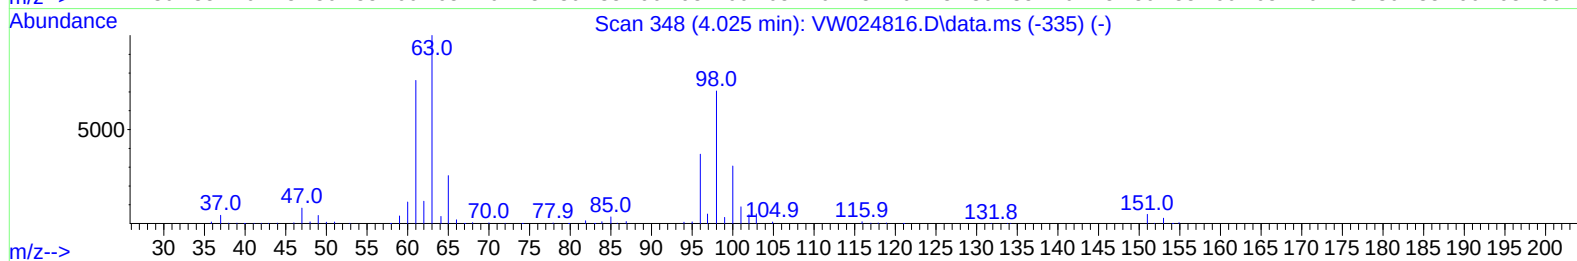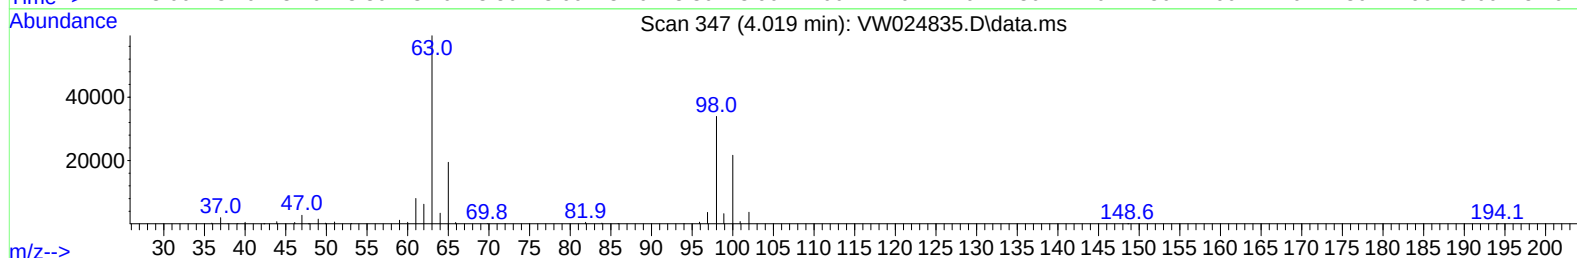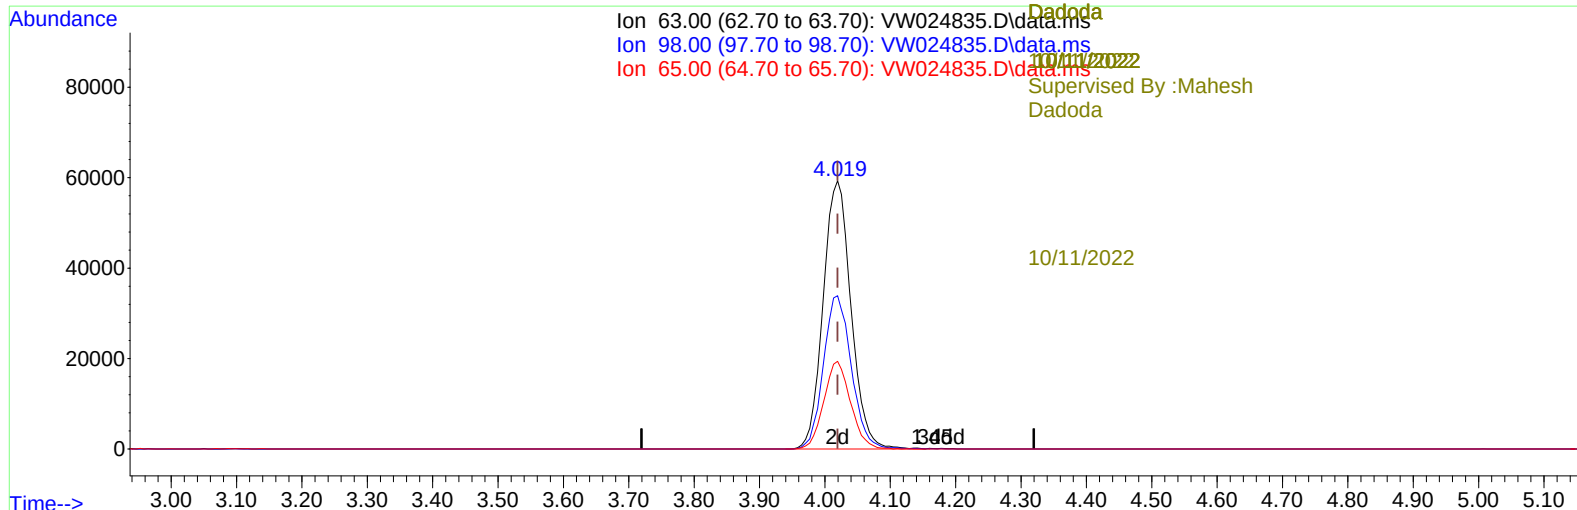

TIC: VW024835.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.019min (-0.000) 13.29 ug/L m

response 175803

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	74.00	0.10#
65.00	22.40	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
 Data File : VW024835.D
 Acq On : 11 Oct 2022 03:48
 Operator : SY/VA
 Sample : N5064-11
 Misc : 7.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BR6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

10/11/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Oct 11 06:38:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 07 03:04:02 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		546369	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		488385	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		246397	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		109085	19.083	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.320%	
7) Chloroethane-d5	2.885	69		65024	19.574	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.280%	
11) 1,1-Dichloroethene-d2	4.019	63		175803m	13.287	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.160%	
21) 2-Butanone-d5	7.074	46		117328	57.088	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.180%	
24) Chloroform-d	7.647	84		325462	22.282	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.120%	
26) 1,2-Dichloroethane-d4	8.305	65		178426	23.548	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.200%	
32) Benzene-d6	8.275	84		635288	20.351	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.400%	
36) 1,2-Dichloropropane-d6	9.274	67		212150	22.244	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.960%	
41) Toluene-d8	10.323	98		551532	19.768	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.080%	
43) trans-1,3-Dichloroprop...	10.579	79		73520	17.310	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.240%	
47) 2-Hexanone-d5	10.920	63		91296	55.946	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.900%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		192897	28.385	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.520%	
66) 1,2-Dichlorobenzene-d4	13.853	152		190180	21.934	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.720%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101022\
Data File : VW024835.D
Acq On : 11 Oct 2022 03:48
Operator : SY/VA
Sample : N5064-11
Misc : 7.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BR6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

10/11/2022
Supervised By :Mahesh
Dadoda

10/11/2022
Supervised By :Mahesh
Dadoda

